

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022889.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 13:21
 Operator : DD/AJ
 Sample : VBF1105S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 00:32:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	432743	19.223 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.695	1825	0.057 ng/ml
6) t Toluene	10.628	4645	0.108 ng/ml
8) t m-Xylene	13.199	1432	0.038 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	550	0.019 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022889.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 13:21
Operator : DD/AJ
Sample : VBF1105S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 00:32:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

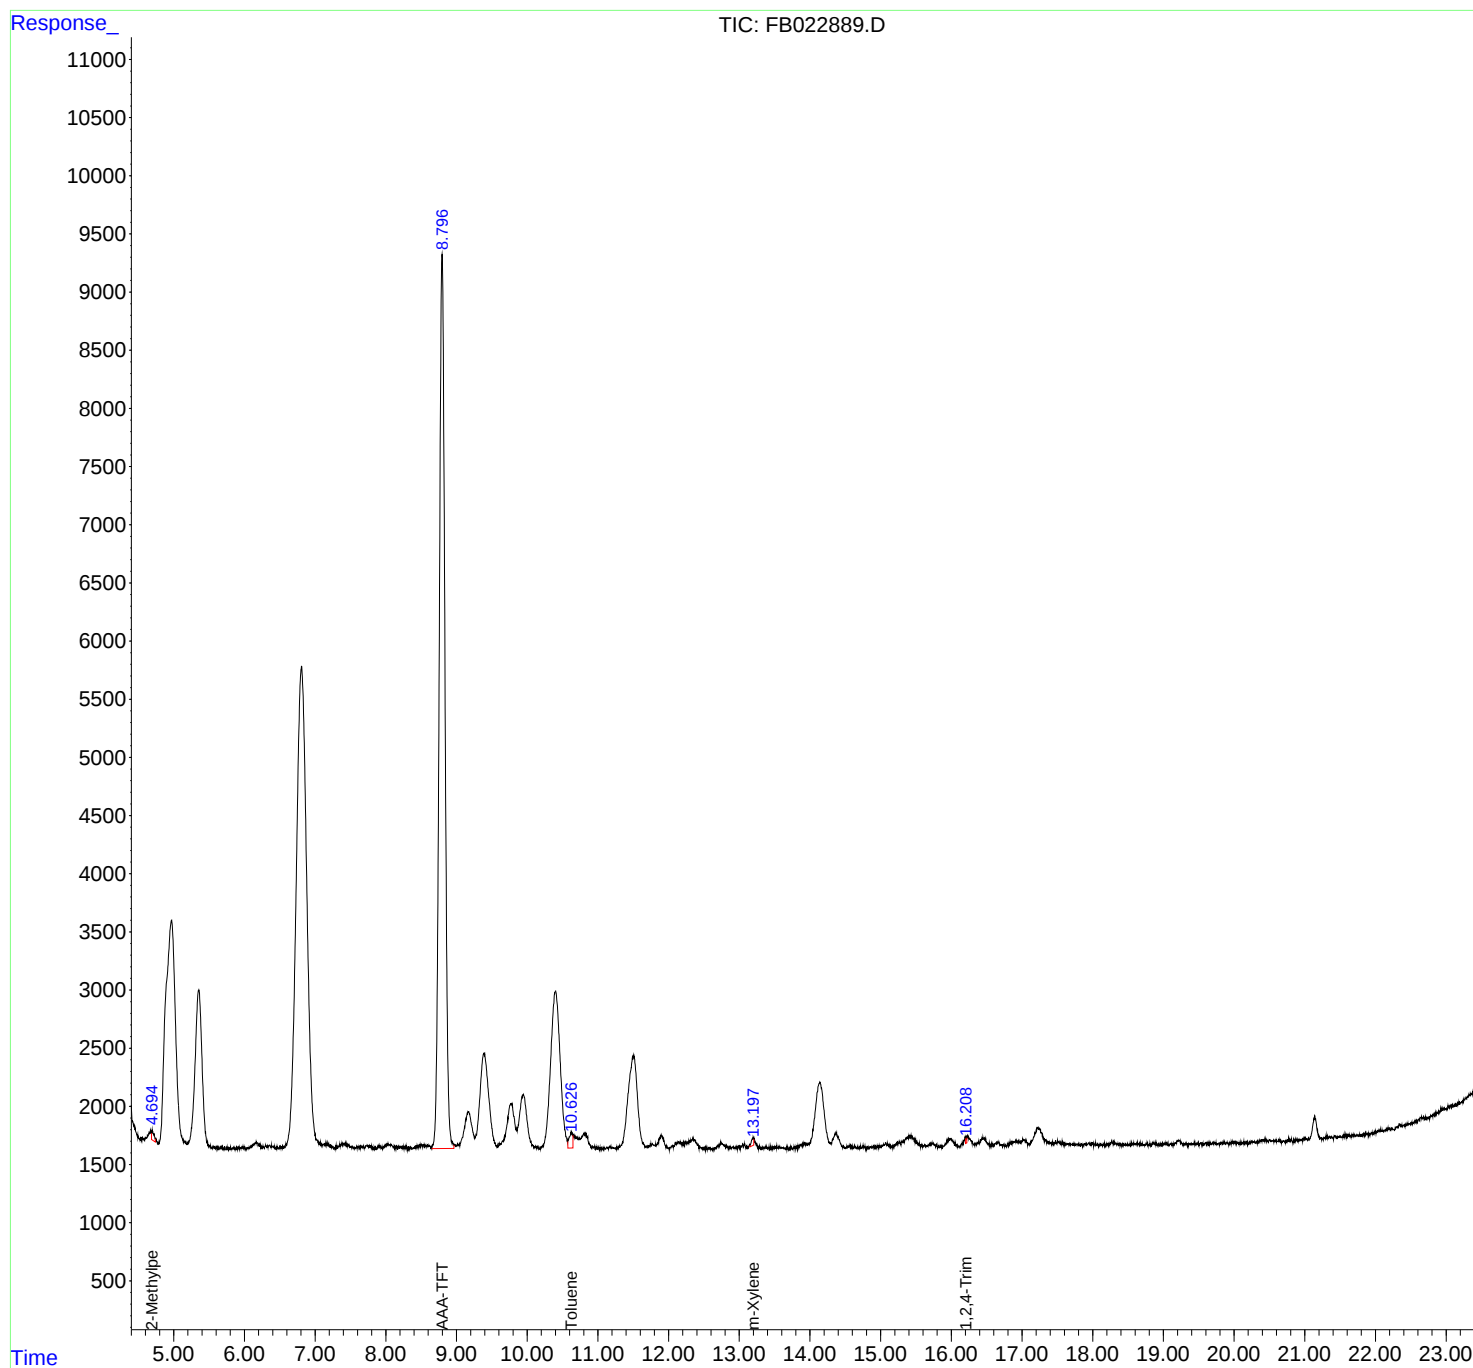


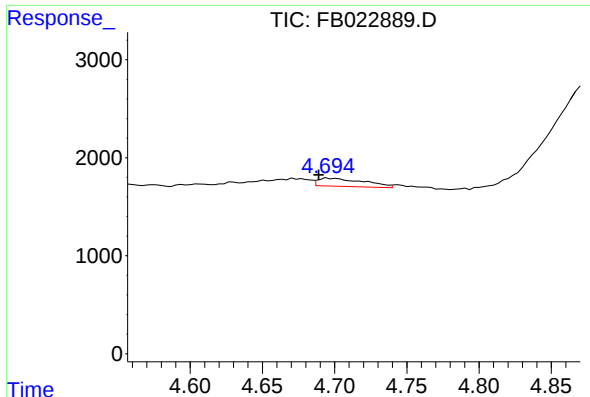

#1 2-Methylpentane


R.T.: 4.695 min
Delta R.T.: 0.006 min
Response: 1825
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :

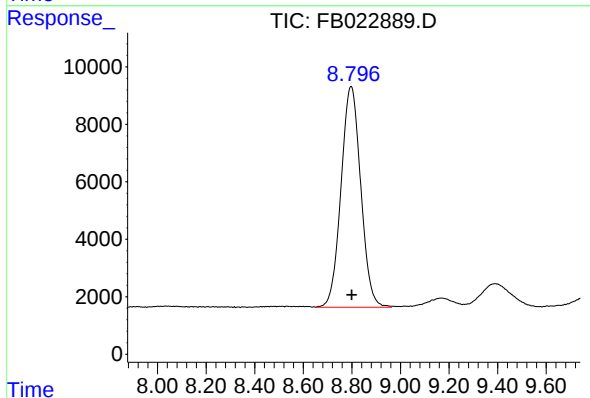


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 432743
Conc: 19.22 ng/ml

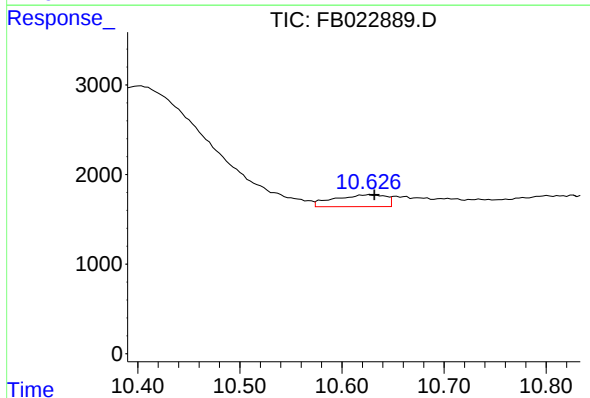


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 4645
Conc: 0.11 ng/ml

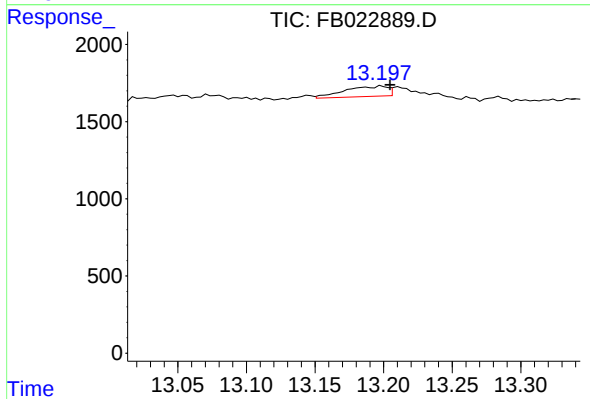

#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 1432
Conc: 0.04 ng/ml

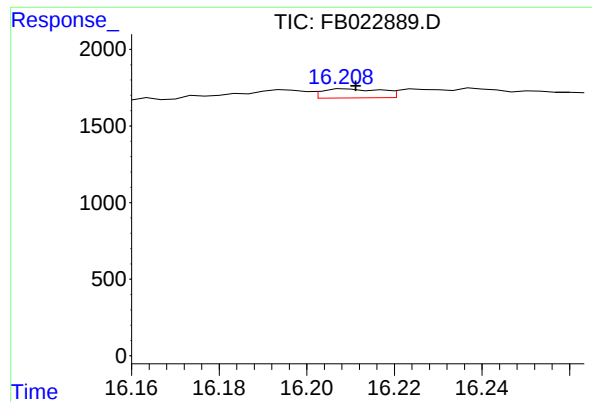

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 550
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :