

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022890.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 13:51
 Operator : DD/AJ
 Sample : K5609-15 250X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 00:32:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.817	799879	35.531 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.683	521623	16.216 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	762334	21.596 ng/ml
3) t n-Heptane	7.753	1413430	40.633 ng/ml
4) t Benzene	7.887	484078	11.176 ng/ml
6) t Toluene	10.628	5233788	121.404 ng/ml
7) t Ethylbenzene	13.068	1319059	33.041 ng/ml
8) t m-Xylene	13.199	5010570	132.670 ng/ml
9) t O-Xylene	13.929	1817679	51.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	1679926	59.239 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022890.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 13:51
Operator : DD/AJ
Sample : K5609-15 250X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 00:32:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

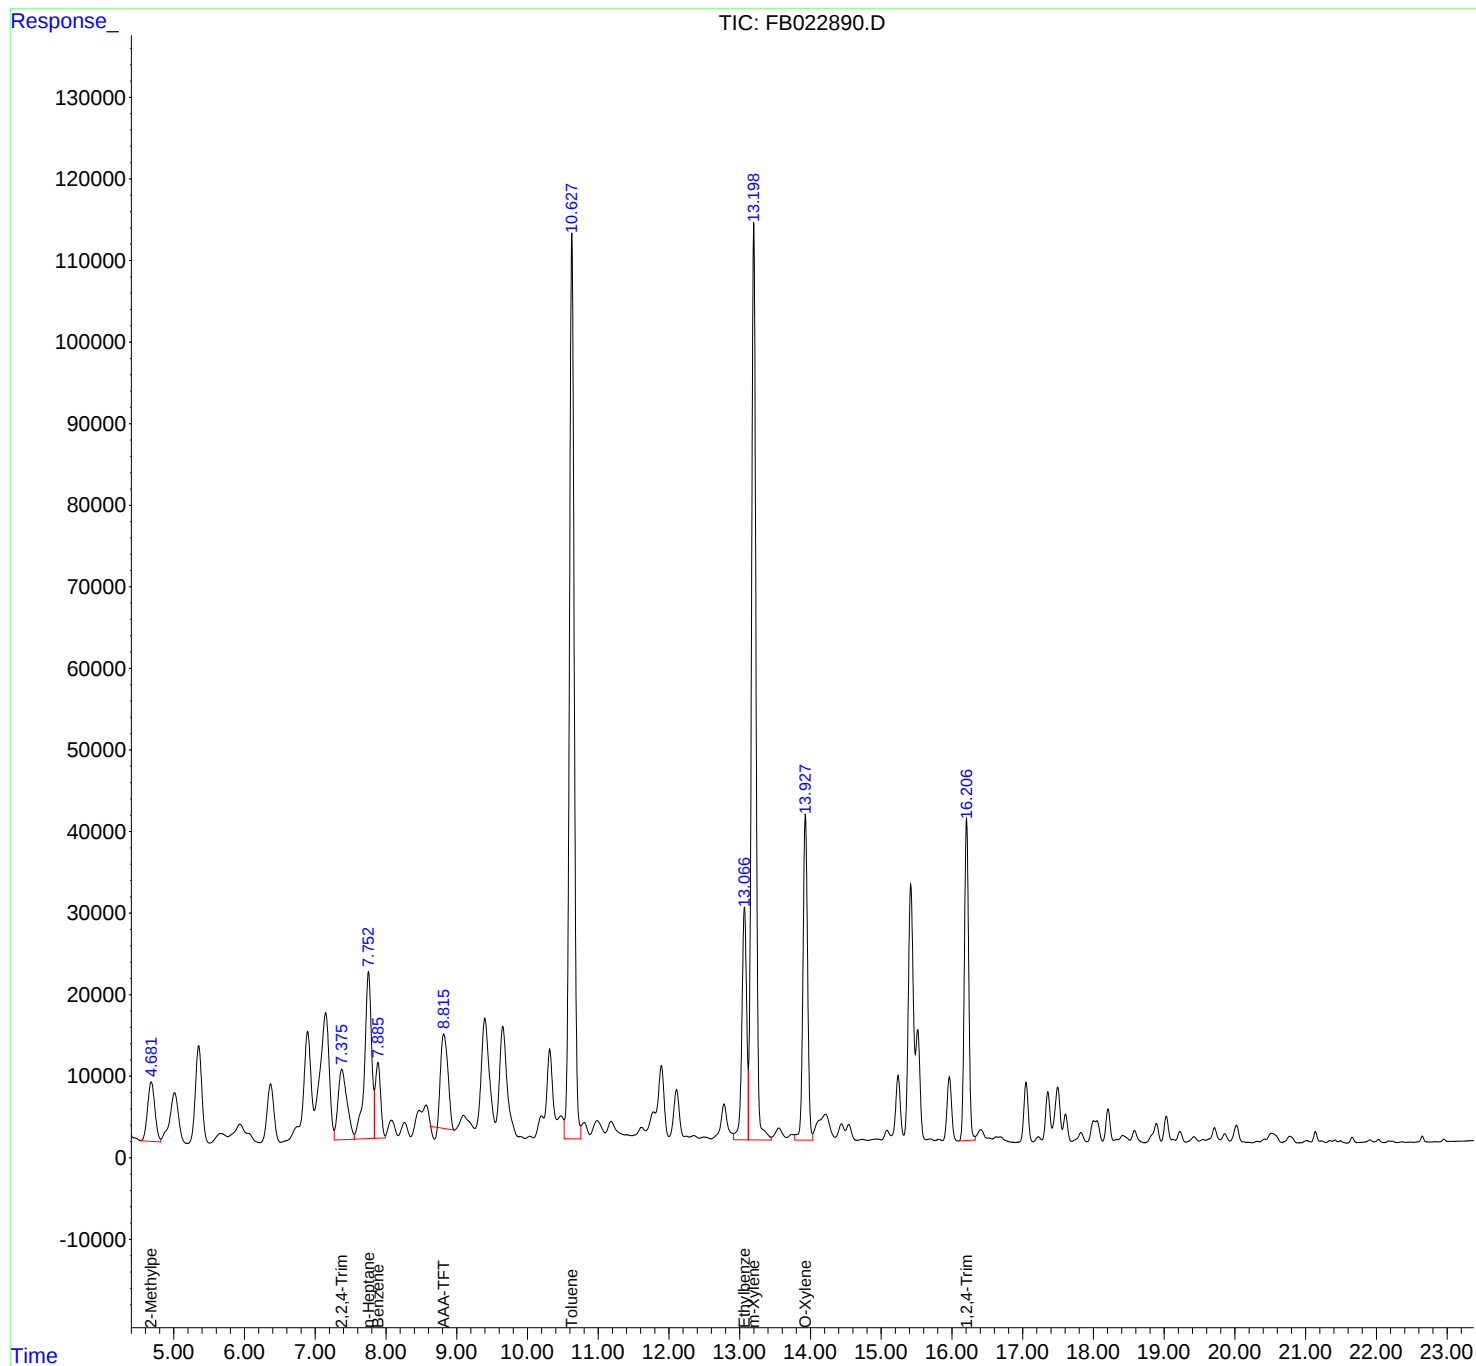


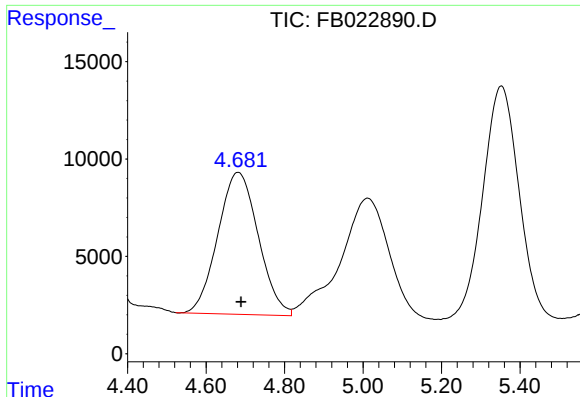

#1 2-Methylpentane


R.T.: 4.683 min
Delta R.T.: -0.006 min
Response: 521623
Conc: 16.22 ng/ml

Instrument :
FID_B
ClientSampleId :

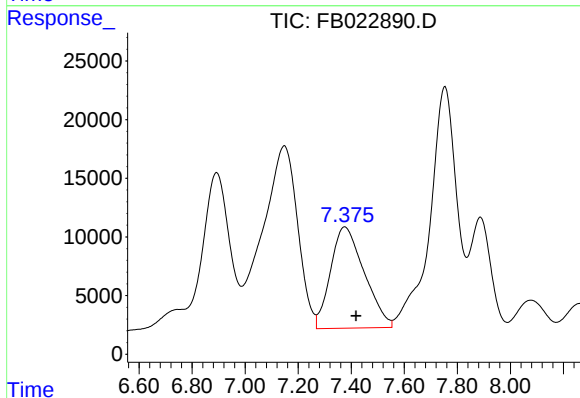


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.042 min
Response: 762334
Conc: 21.60 ng/ml

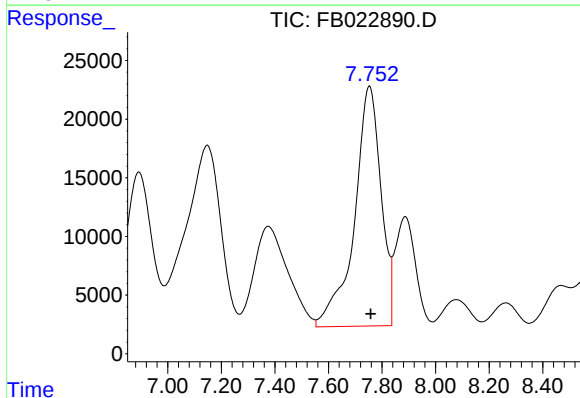


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 1413430
Conc: 40.63 ng/ml

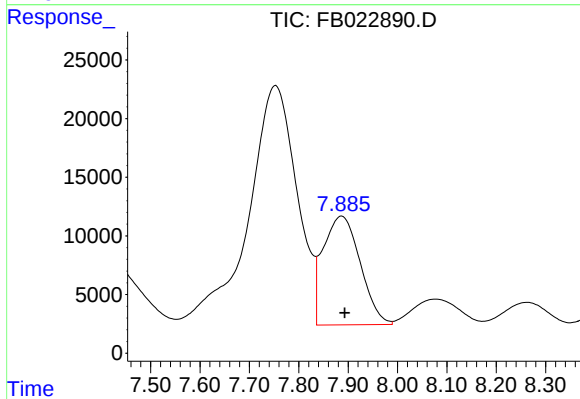

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 484078
Conc: 11.18 ng/ml

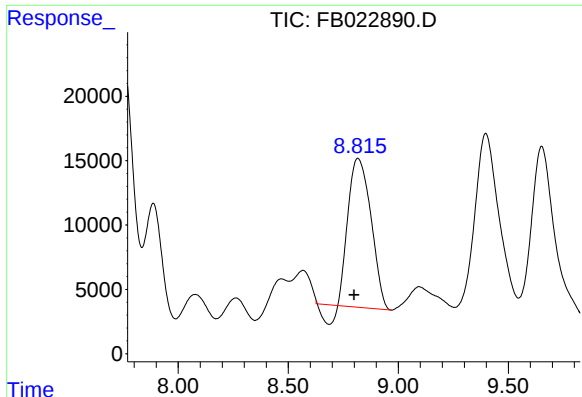

#5 AAA-TFT


R.T.: 8.817 min
Delta R.T.: 0.017 min
Response: 799879
Conc: 35.53 ng/ml

Instrument :
FID_B
ClientSampleId :

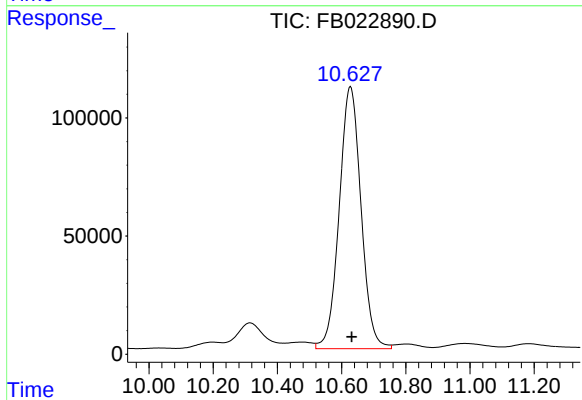


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 5233788
Conc: 121.40 ng/ml

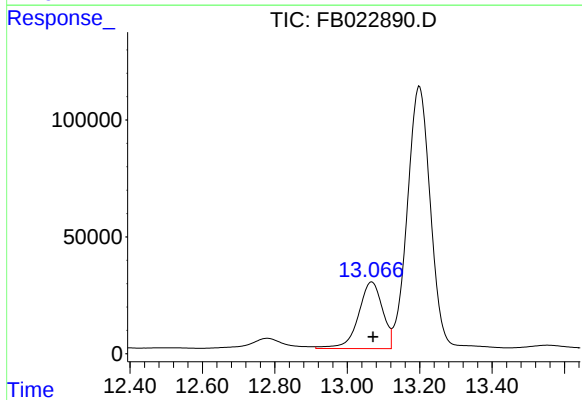


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 1319059
Conc: 33.04 ng/ml

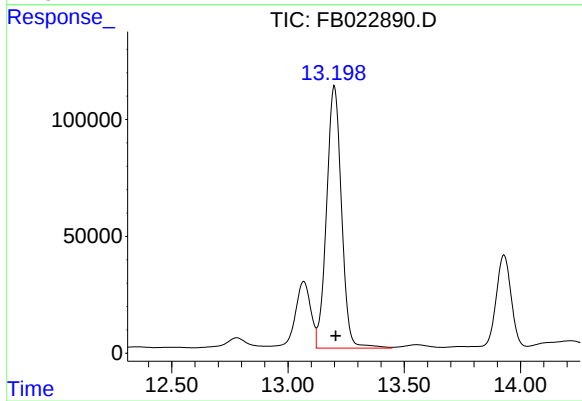

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 5010570
Conc: 132.67 ng/ml

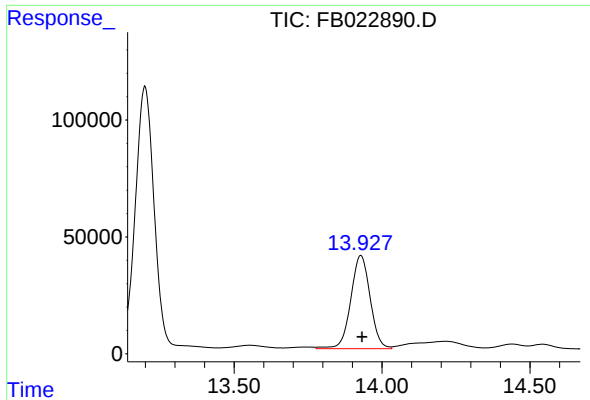

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 1817679
Conc: 51.00 ng/ml

Instrument :
FID_B
ClientSampleId :

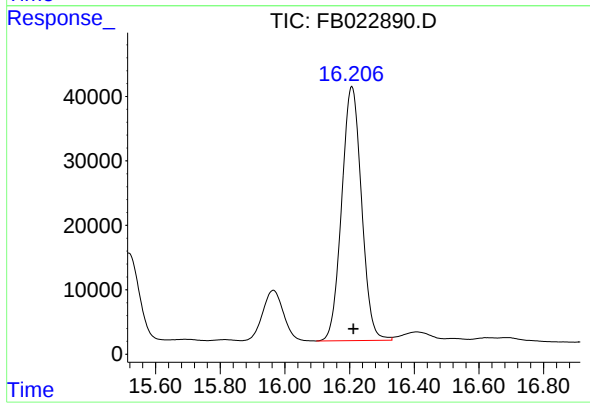

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.004 min
Response: 1679926
Conc: 59.24 ng/ml