

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022894.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 17:21
 Operator : DD/AJ
 Sample : K5609-15 300X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 07:49:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.812	669698	29.749 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	385687	11.990 ng/ml
2) t 2,2,4-Trimethylpentane	7.379	539521	15.284 ng/ml
3) t n-Heptane	7.756	1004703	28.883 ng/ml
4) t Benzene	7.890	345762	7.983 ng/ml
6) t Toluene	10.630	3782478	87.739 ng/ml
7) t Ethylbenzene	13.070	933777	23.390 ng/ml
8) t m-Xylene	13.201	3484172	92.254 ng/ml
9) t O-Xylene	13.931	1268889	35.602 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	1206003	42.527 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022894.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 17:21
Operator : DD/AJ
Sample : K5609-15 300X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 07:49:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

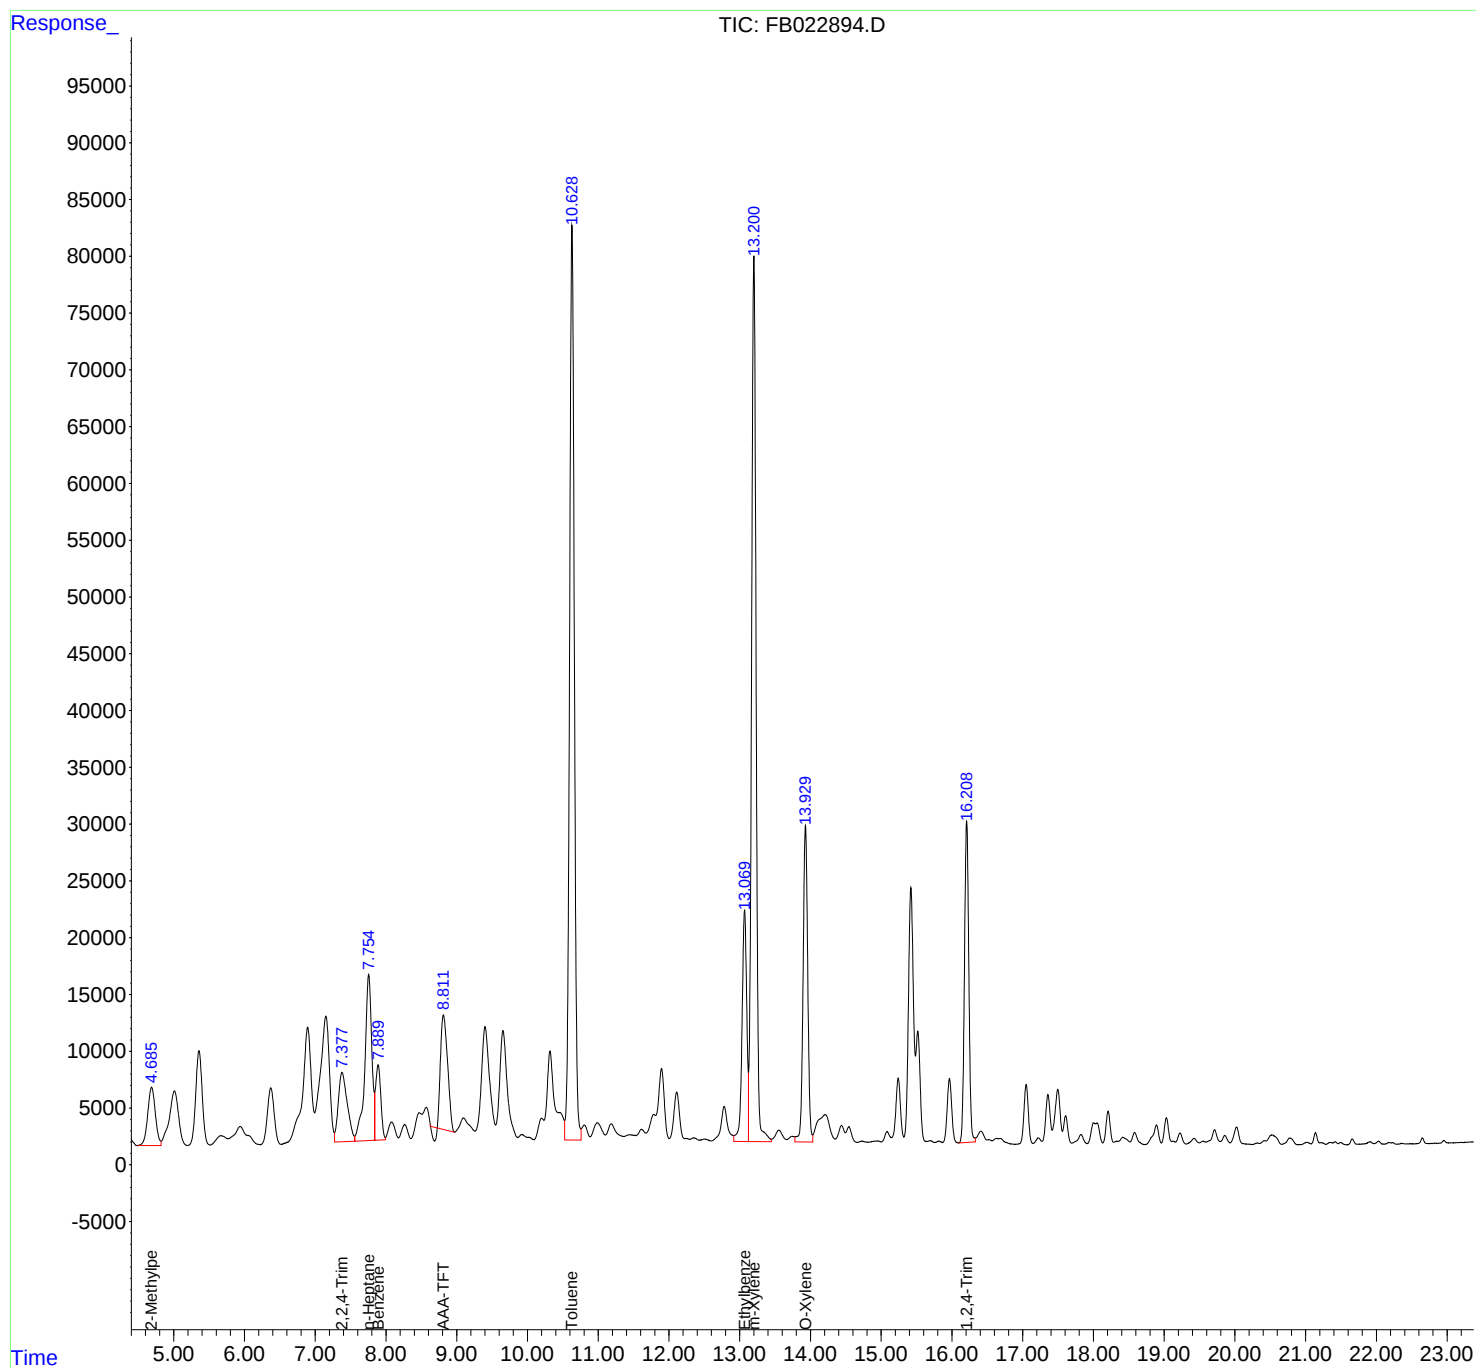


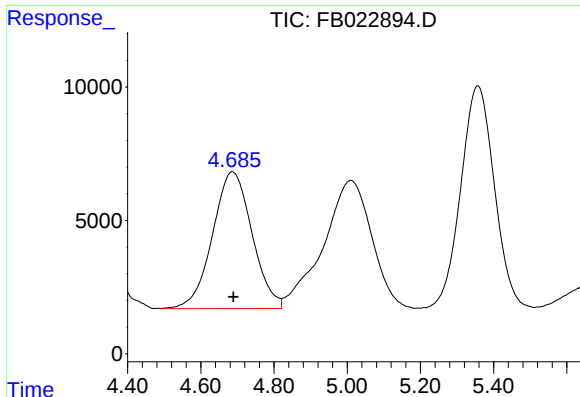

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 385687
Conc: 11.99 ng/ml

Instrument :
FID_B
ClientSampleId :

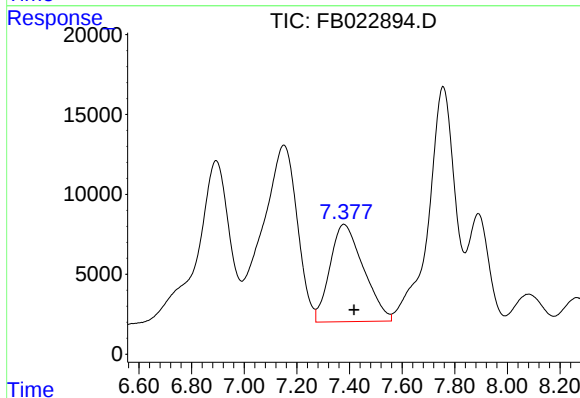


#2 2,2,4-Trimethylpentane

R.T.: 7.379 min
Delta R.T.: -0.039 min
Response: 539521
Conc: 15.28 ng/ml

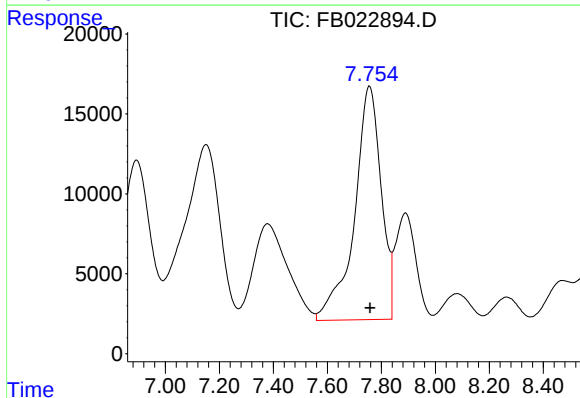


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 1004703
Conc: 28.88 ng/ml

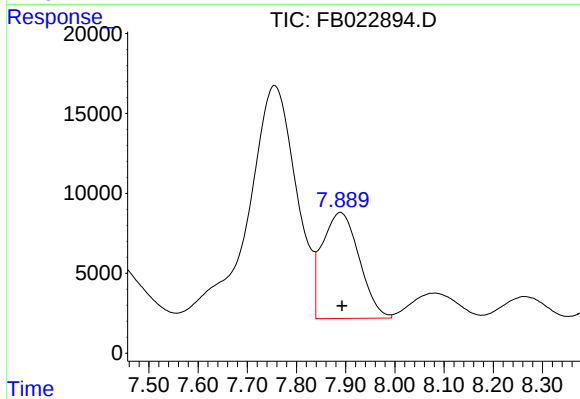

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 345762
Conc: 7.98 ng/ml

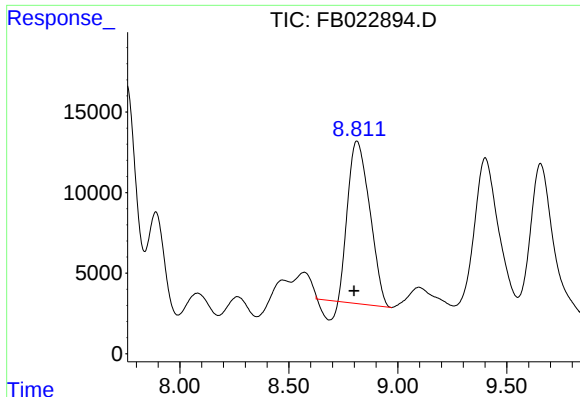

#5 AAA-TFT


R.T.: 8.812 min
Delta R.T.: 0.013 min
Response: 669698
Conc: 29.75 ng/ml

Instrument :
FID_B
ClientSampleId :

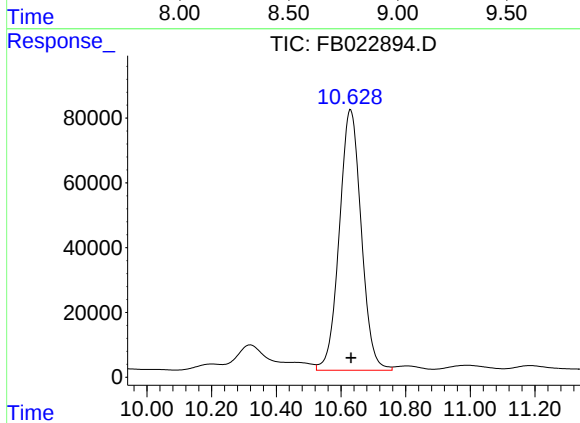


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 3782478
Conc: 87.74 ng/ml

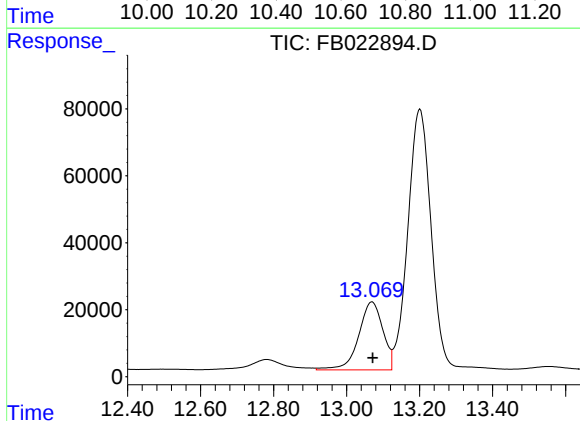


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 933777
Conc: 23.39 ng/ml

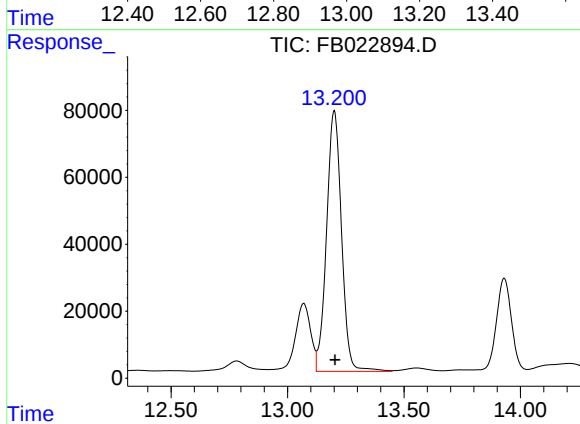

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 3484172
Conc: 92.25 ng/ml

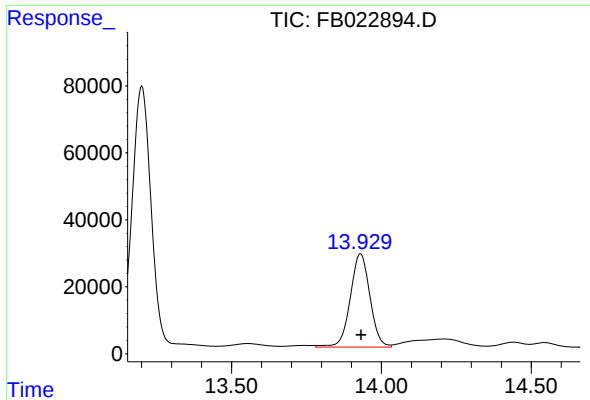

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 1268889
Conc: 35.60 ng/ml

Instrument :
FID_B
ClientSampleId :

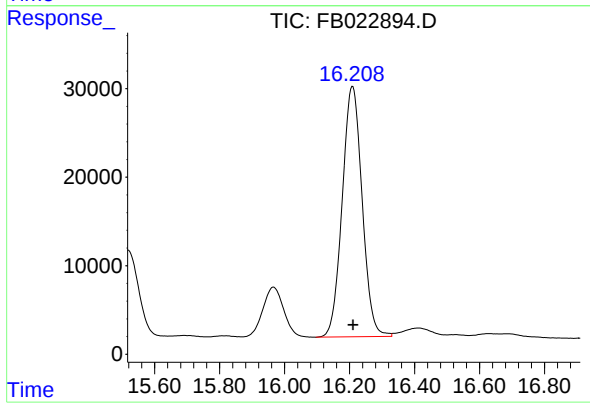

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 1206003
Conc: 42.53 ng/ml