

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022895.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 18:21
 Operator : DD/AJ
 Sample : K5609-15 300X SP
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 07:49:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.812	685894	30.468 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	395289	12.288 ng/ml
2) t 2,2,4-Trimethylpentane	7.378	556444	15.763 ng/ml
3) t n-Heptane	7.755	1028158	29.557 ng/ml
4) t Benzene	7.889	357754	8.259 ng/ml
6) t Toluene	10.629	3840790	89.092 ng/ml
7) t Ethylbenzene	13.069	952042	23.847 ng/ml
8) t m-Xylene	13.200	3534028	93.574 ng/ml
9) t O-Xylene	13.930	1282625	35.988 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	1216871	42.910 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022895.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 18:21
Operator : DD/AJ
Sample : K5609-15 300X SP
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 07:49:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

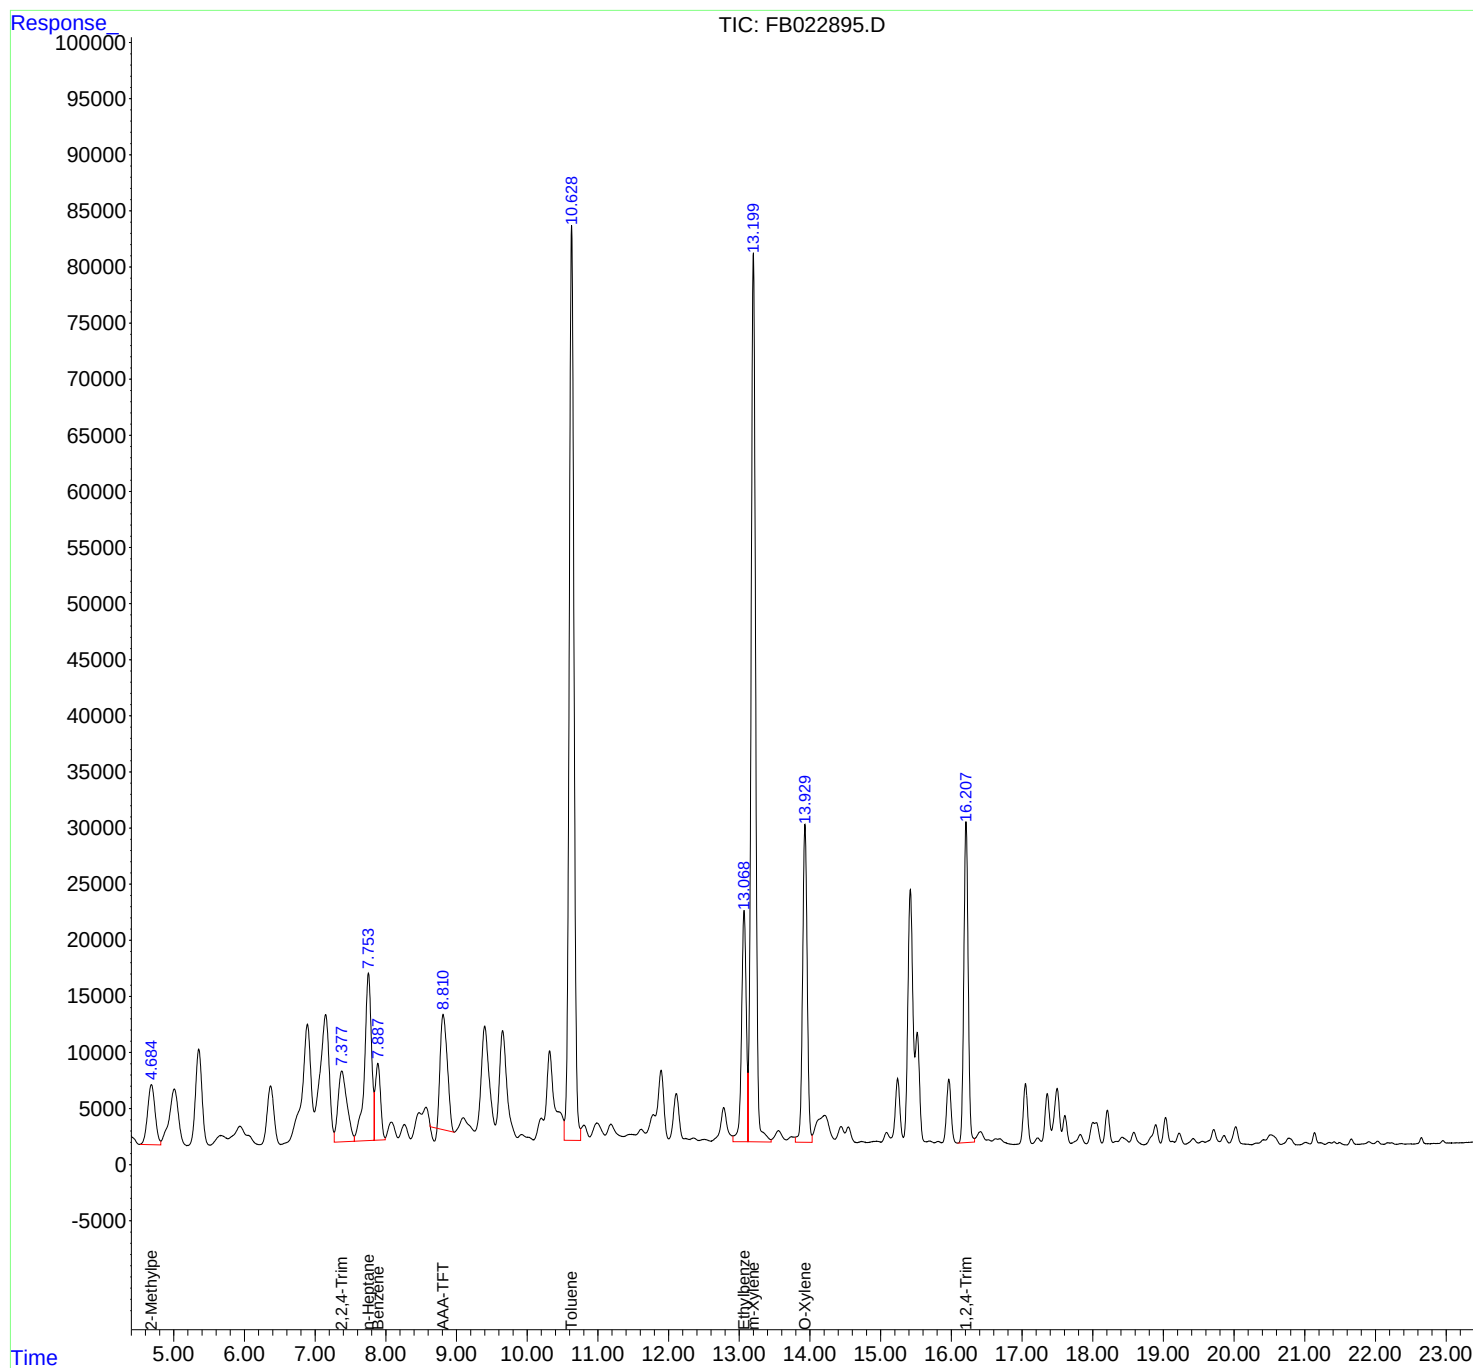


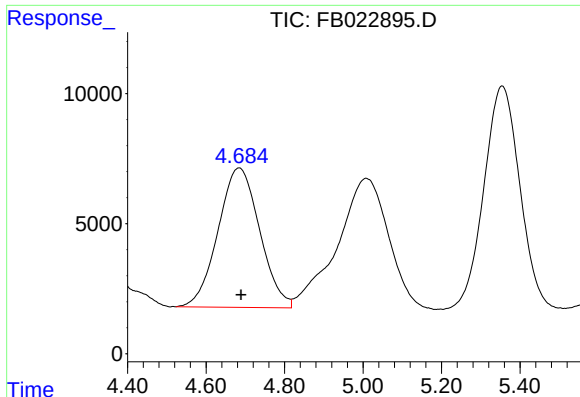

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 395289
Conc: 12.29 ng/ml

Instrument :
FID_B
ClientSampleId :

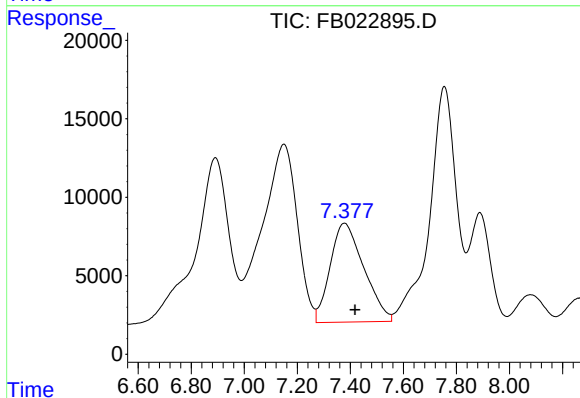


#2 2,2,4-Trimethylpentane

R.T.: 7.378 min
Delta R.T.: -0.040 min
Response: 556444
Conc: 15.76 ng/ml

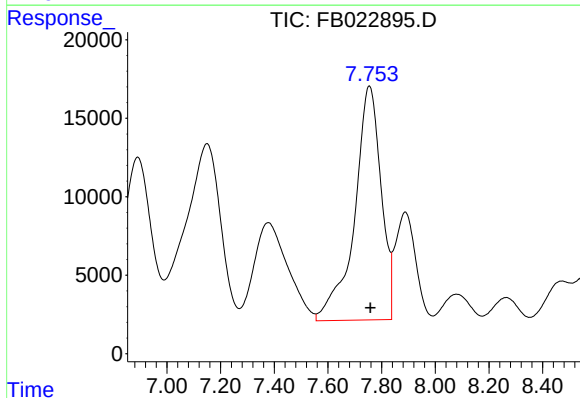


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 1028158
Conc: 29.56 ng/ml

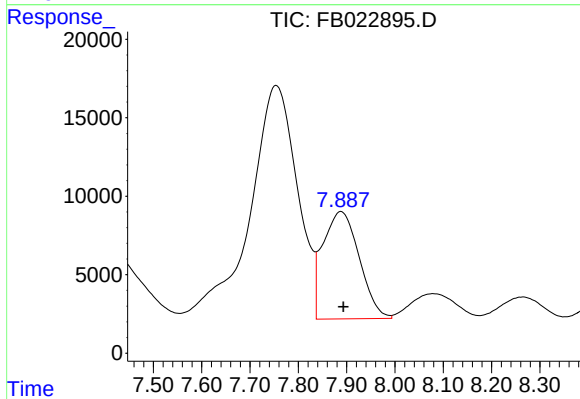

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 357754
Conc: 8.26 ng/ml

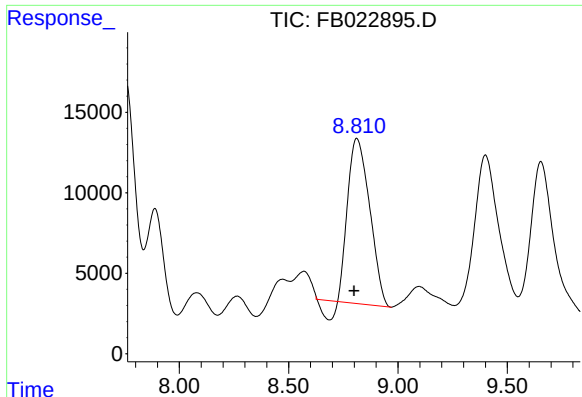

#5 AAA-TFT


R.T.: 8.812 min
Delta R.T.: 0.012 min
Response: 685894
Conc: 30.47 ng/ml

Instrument :
FID_B
ClientSampleId :

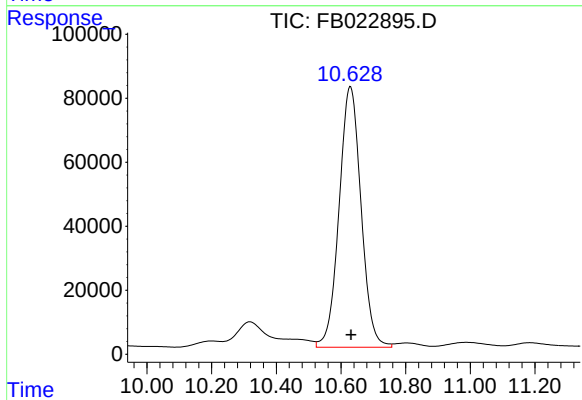


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 3840790
Conc: 89.09 ng/ml

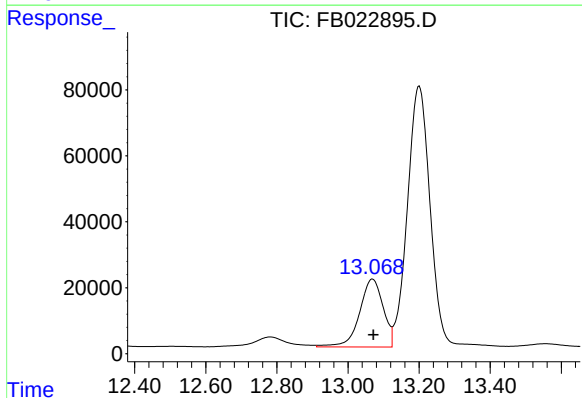


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 952042
Conc: 23.85 ng/ml

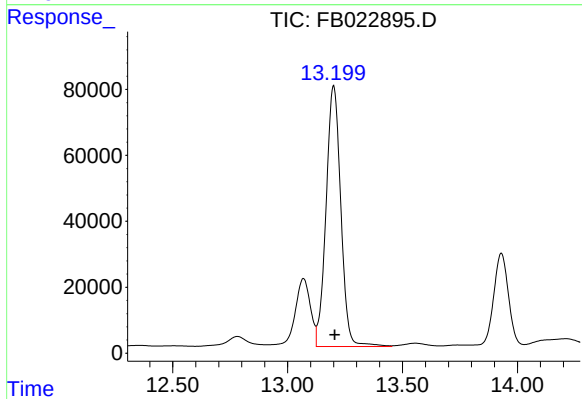

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.004 min
Response: 3534028
Conc: 93.57 ng/ml

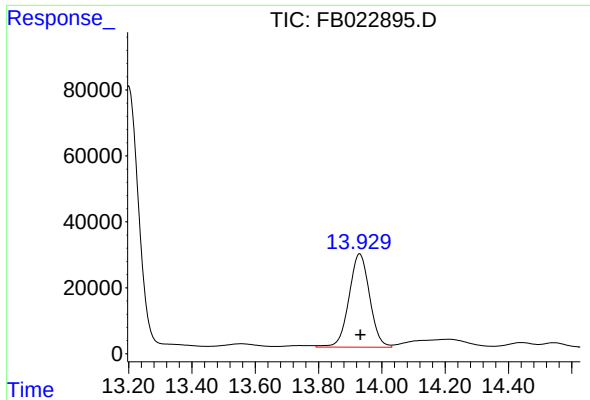

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 1282625
Conc: 35.99 ng/ml

Instrument :
FID_B
ClientSampleId :

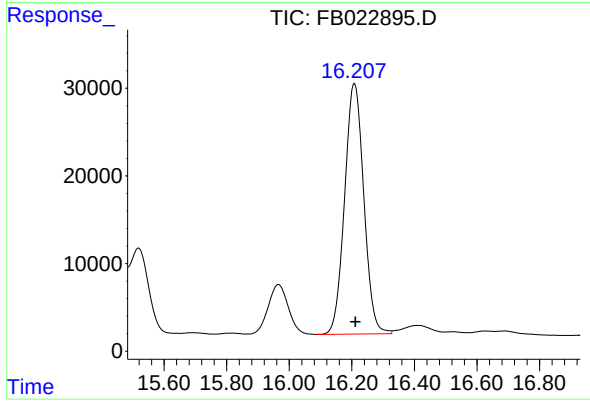

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 1216871
Conc: 42.91 ng/ml