

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022886.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 9:56
 Operator : DD/AJ
 Sample : BSF1105S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1105S1

Integration File: Calibration.e
 Quant Time: Nov 06 00:31:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	439289	19.514 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	997606	31.013 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1128272	31.962 ng/ml
3) t n-Heptane	7.754	367822	10.574 ng/ml
4) t Benzene	7.888	436869	10.086 ng/ml
6) t Toluene	10.627	1306187	30.299 ng/ml
7) t Ethylbenzene	13.067	409183	10.249 ng/ml
8) t m-Xylene	13.200	771428	20.426 ng/ml
9) t O-Xylene	13.928	723734	20.306 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	598170	21.093 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022886.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 9:56
Operator : DD/AJ
Sample : BSF1105S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1105S1

Integration File: Calibration.e
Quant Time: Nov 06 00:31:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

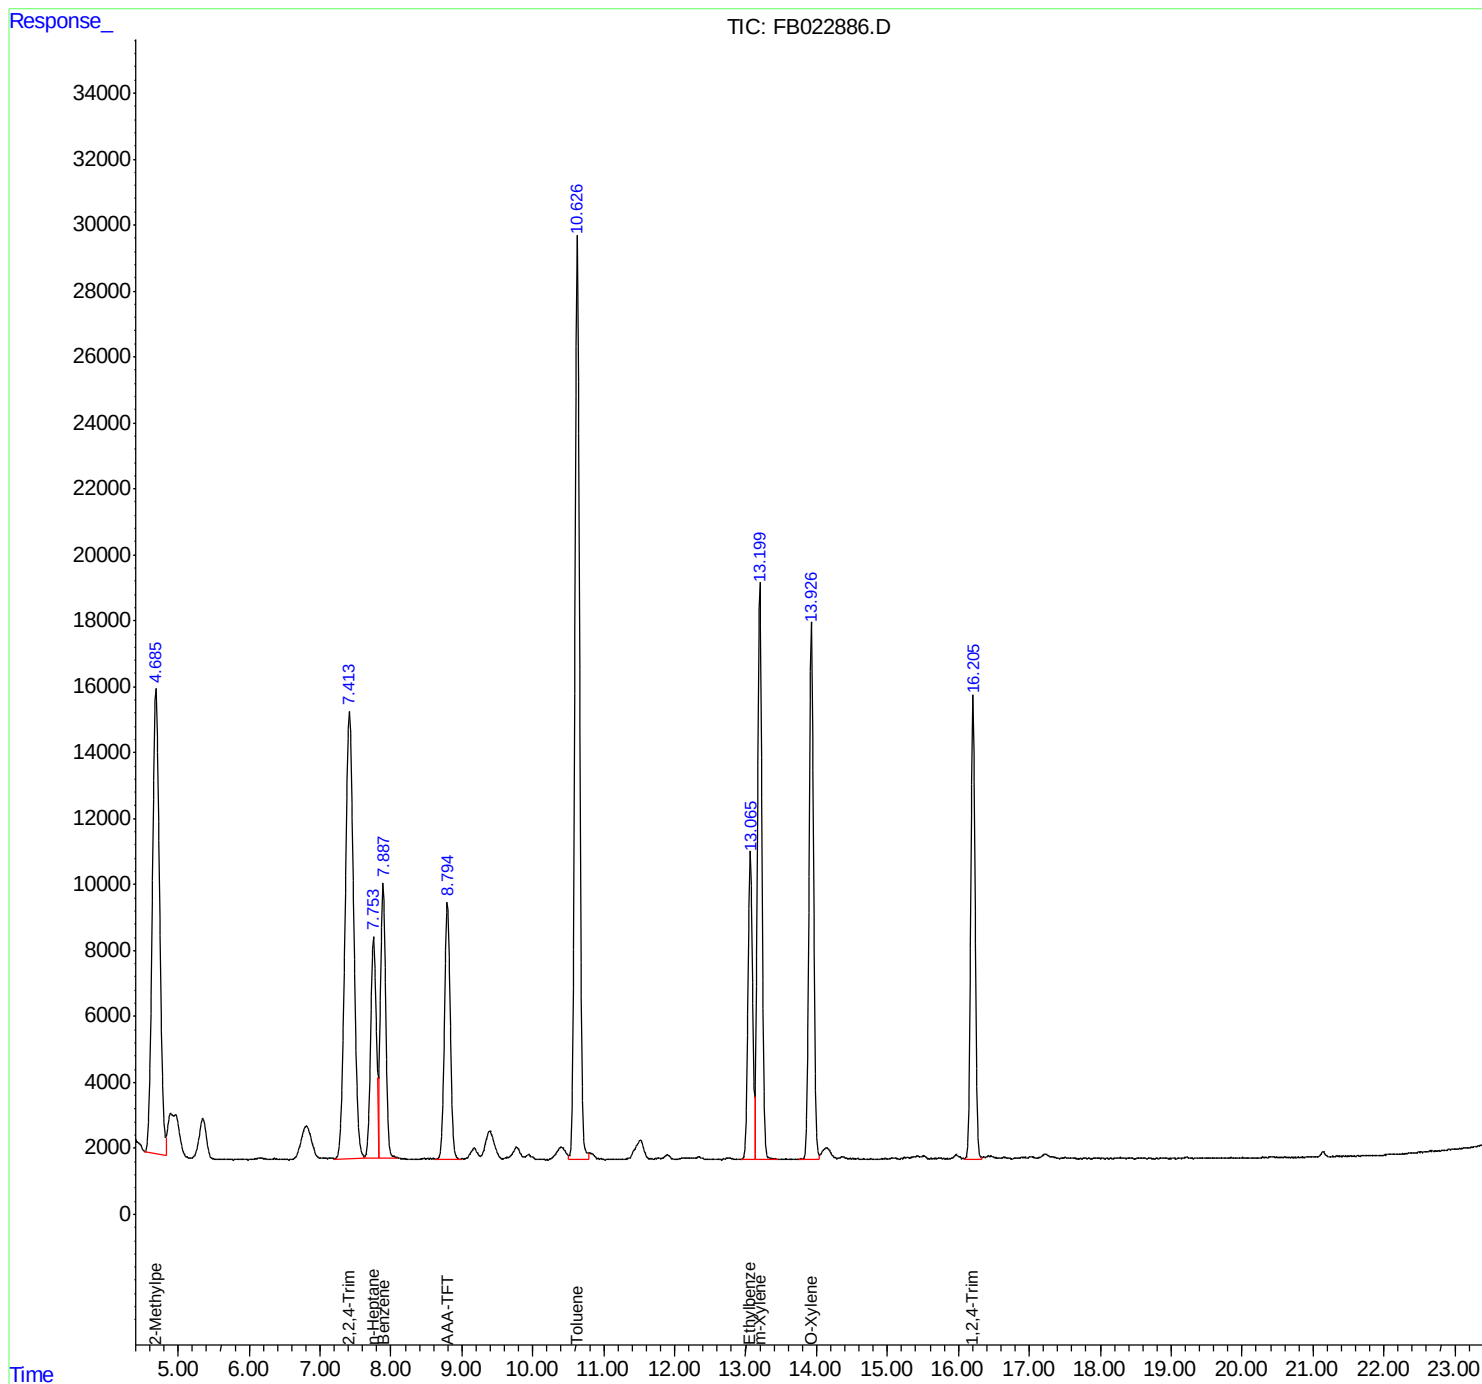


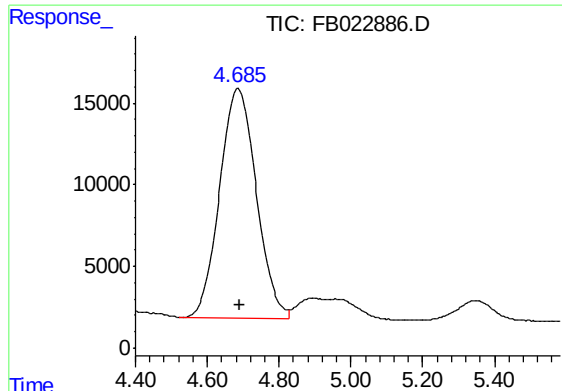

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 997606
Conc: 31.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

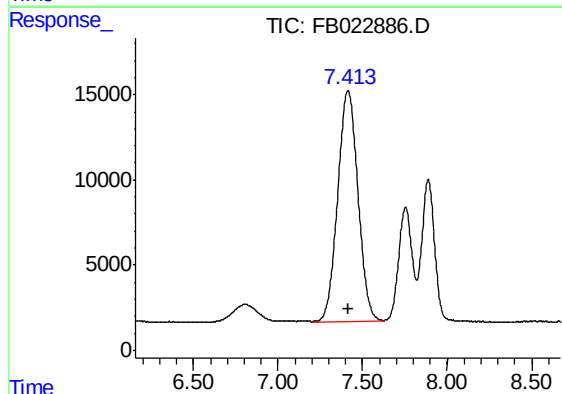


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1128272
Conc: 31.96 ng/ml

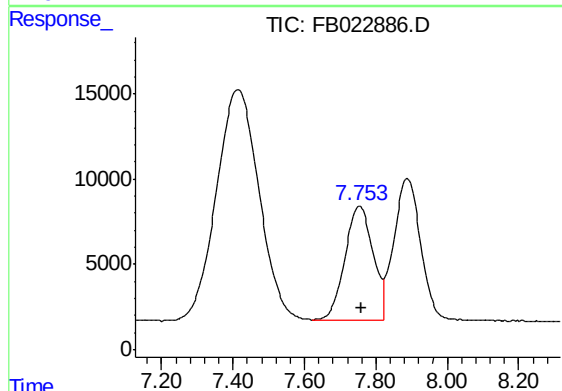


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 367822
Conc: 10.57 ng/ml

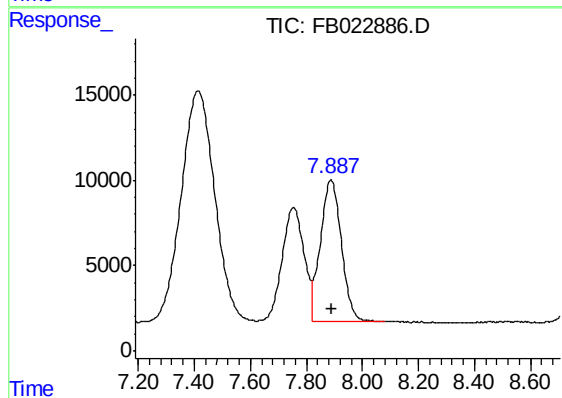

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 436869
Conc: 10.09 ng/ml

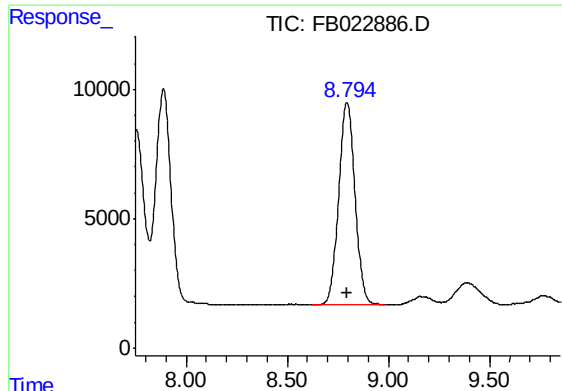

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 439289
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

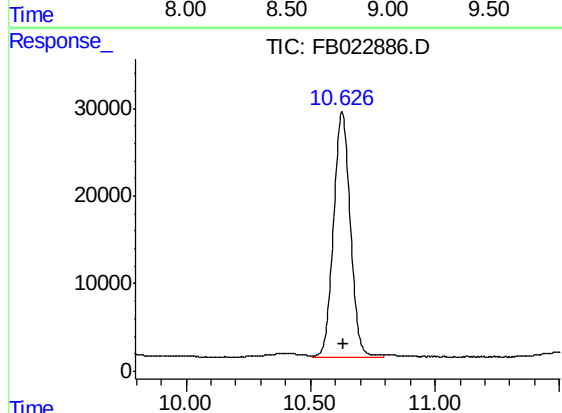


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1306187
Conc: 30.30 ng/ml

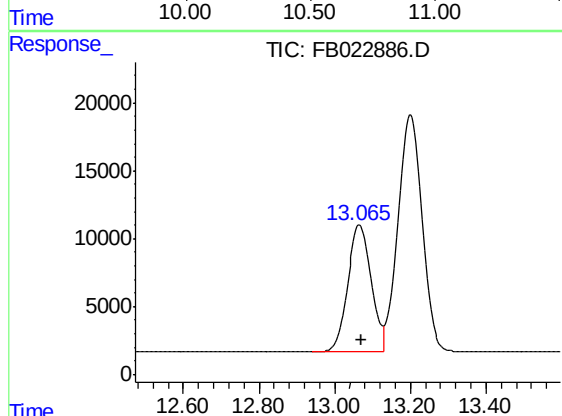


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 409183
Conc: 10.25 ng/ml

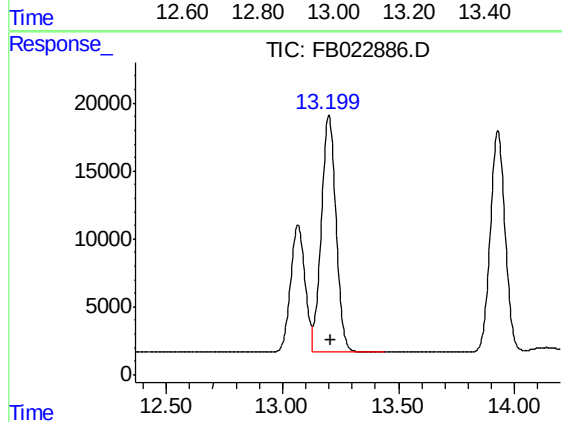

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 771428
Conc: 20.43 ng/ml

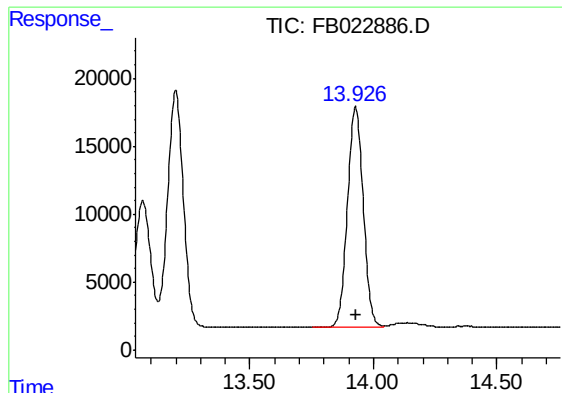

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.005 min
Response: 723734
Conc: 20.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

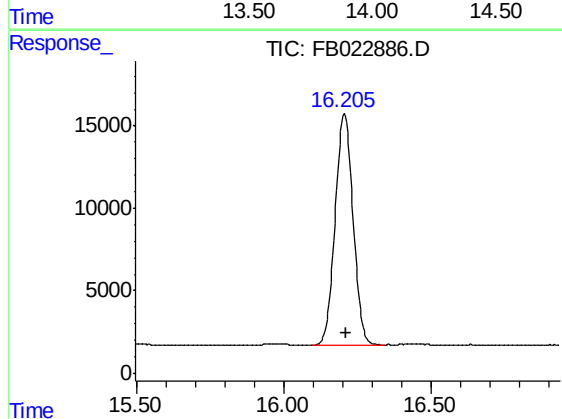

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 598170
Conc: 21.09 ng/ml