

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022887.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 11:52
 Operator : DD/AJ
 Sample : BSF1105S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1105S2

Integration File: Calibration.e
 Quant Time: Nov 06 00:32:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	445676	19.797 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	973414	30.261 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1101076	31.192 ng/ml
3) t n-Heptane	7.752	359591	10.337 ng/ml
4) t Benzene	7.886	428484	9.892 ng/ml
6) t Toluene	10.624	1285423	29.817 ng/ml
7) t Ethylbenzene	13.065	400129	10.023 ng/ml
8) t m-Xylene	13.197	756724	20.037 ng/ml
9) t O-Xylene	13.926	709277	19.901 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	581846	20.517 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022887.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 11:52
Operator : DD/AJ
Sample : BSF1105S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1105S2

Integration File: Calibration.e
Quant Time: Nov 06 00:32:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

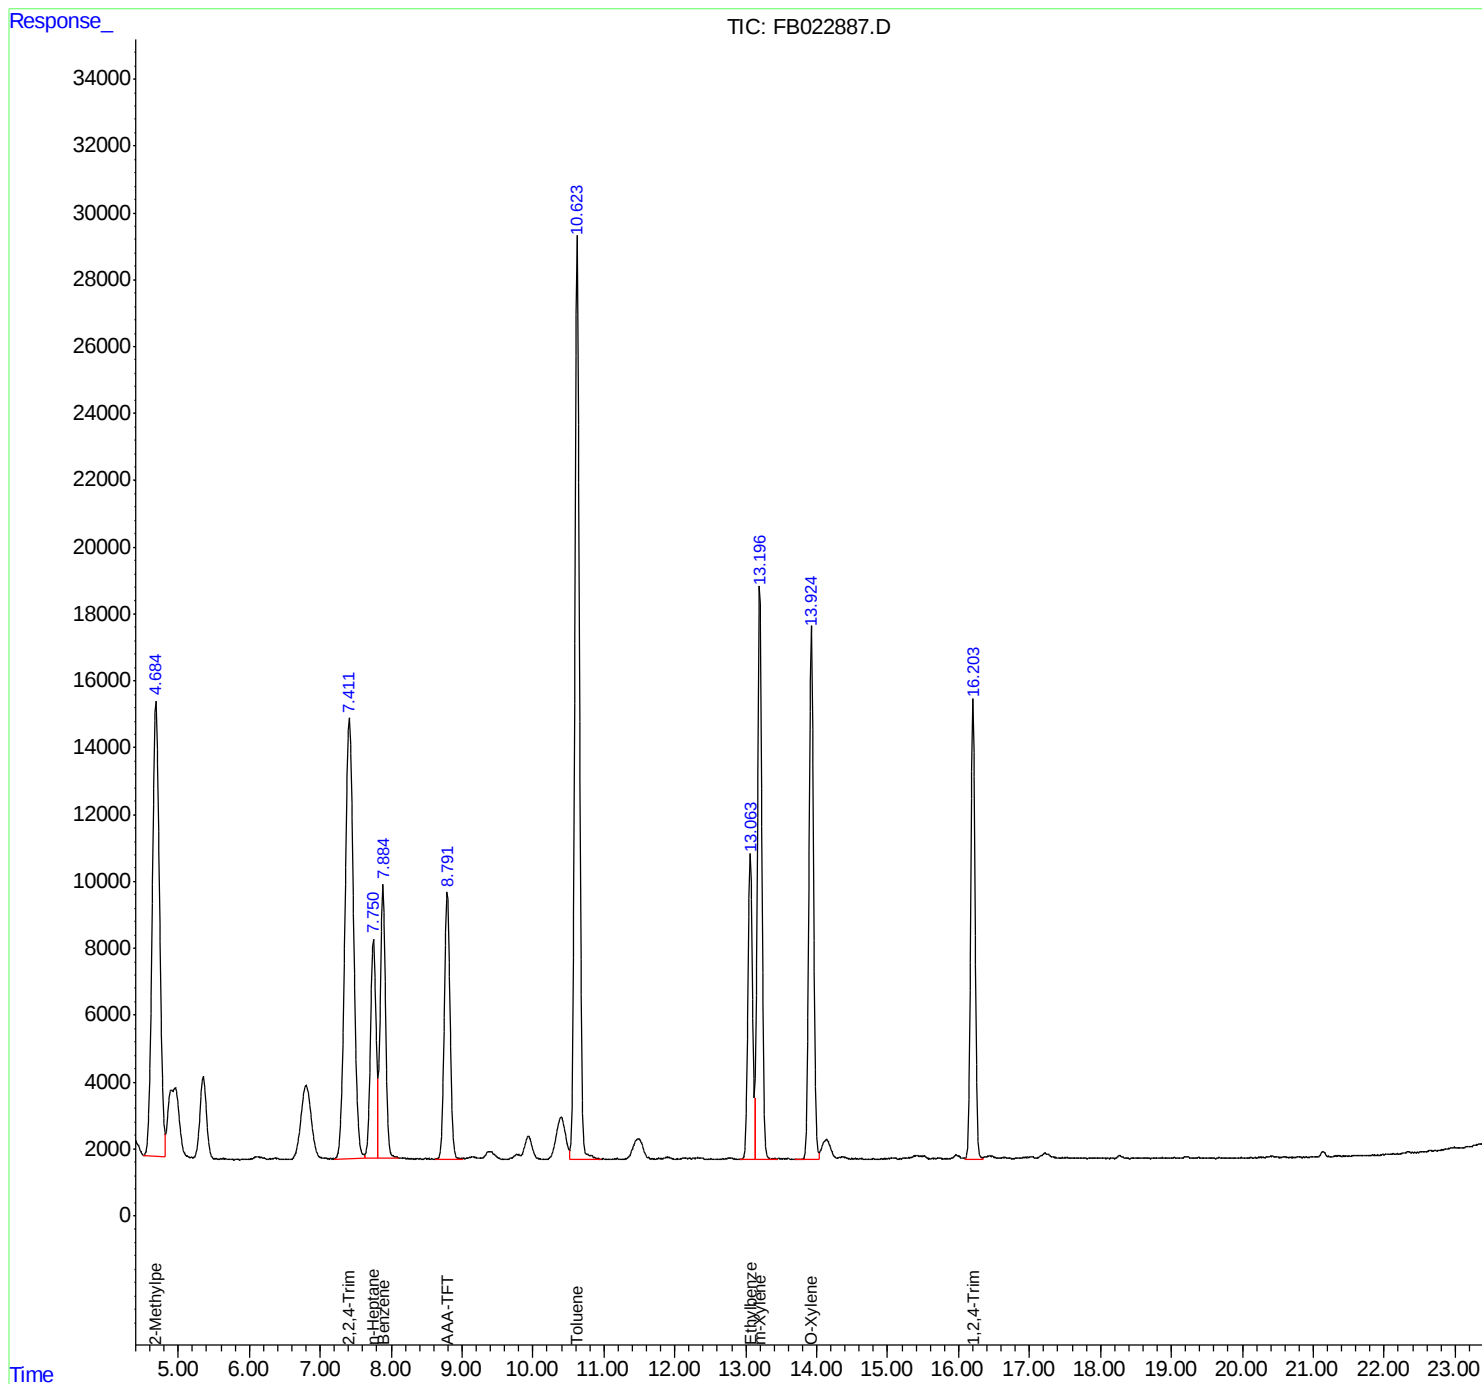


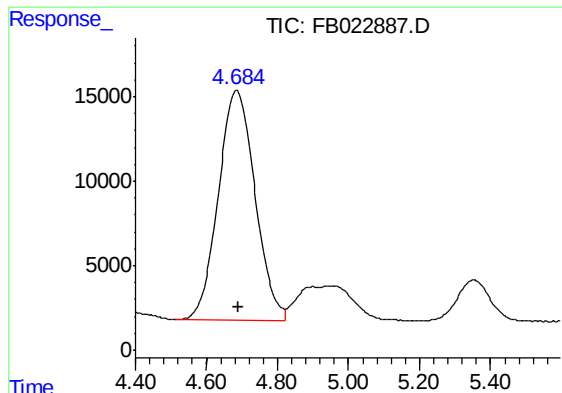

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 973414
Conc: 30.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S2

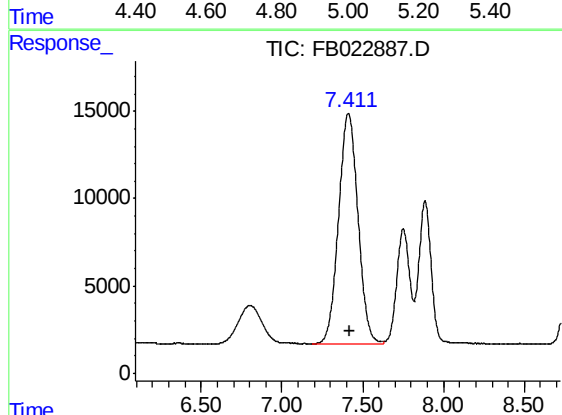


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1101076
Conc: 31.19 ng/ml

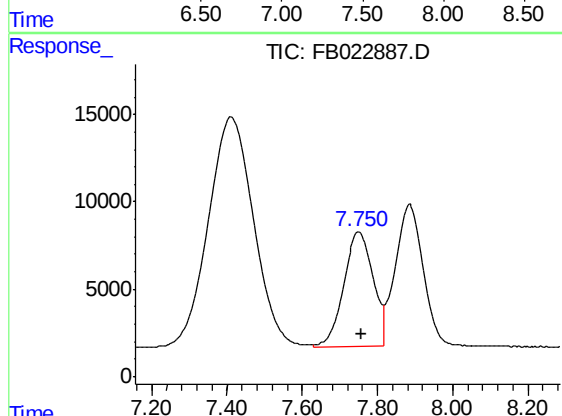


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.007 min
Response: 359591
Conc: 10.34 ng/ml

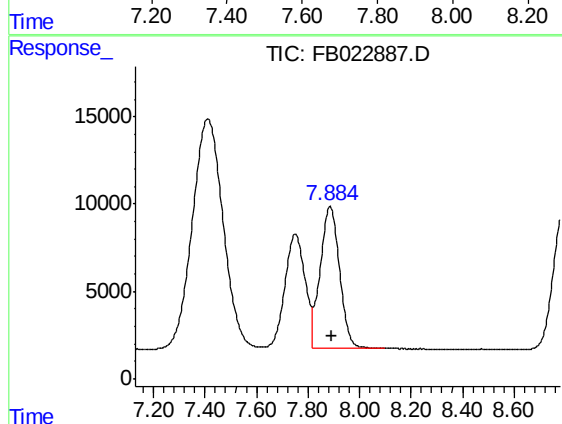

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 428484
Conc: 9.89 ng/ml

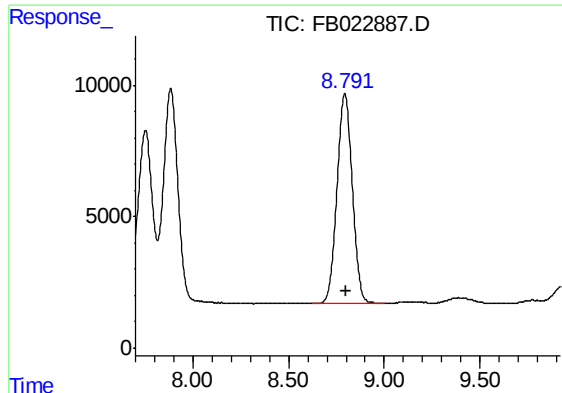

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 445676
Conc: 19.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S2

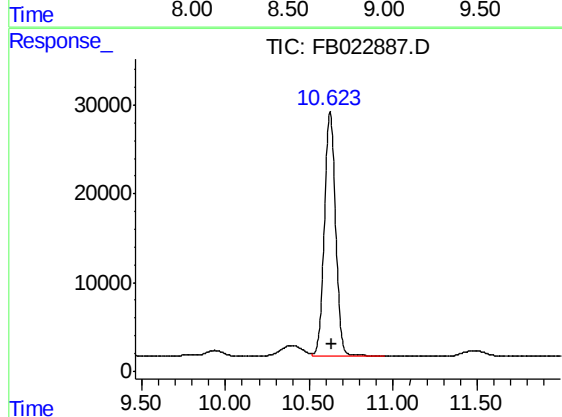


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.008 min
Response: 1285423
Conc: 29.82 ng/ml

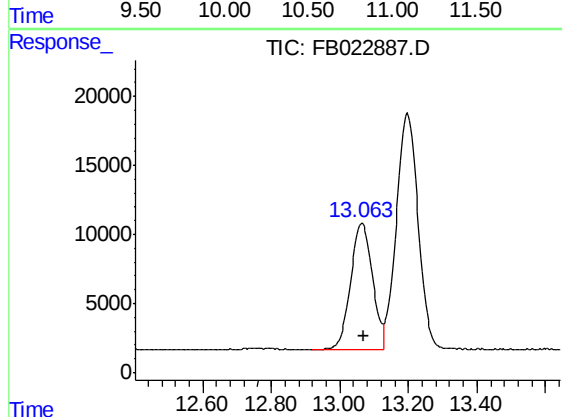


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.007 min
Response: 400129
Conc: 10.02 ng/ml

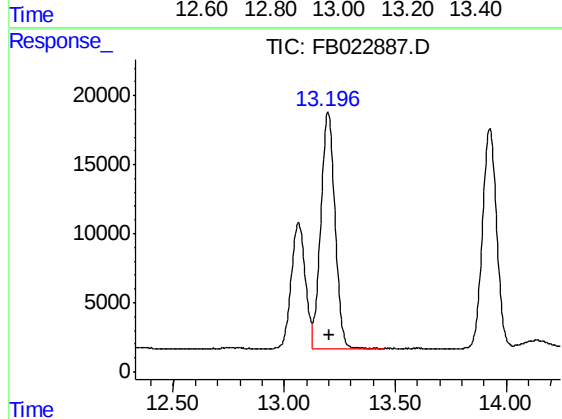

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: -0.008 min
Response: 756724
Conc: 20.04 ng/ml

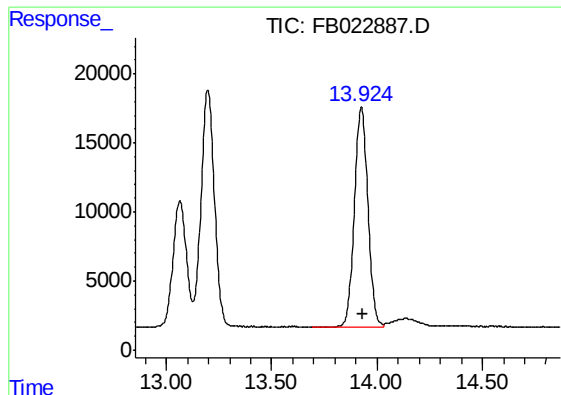

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.007 min
Response: 709277
Conc: 19.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S2

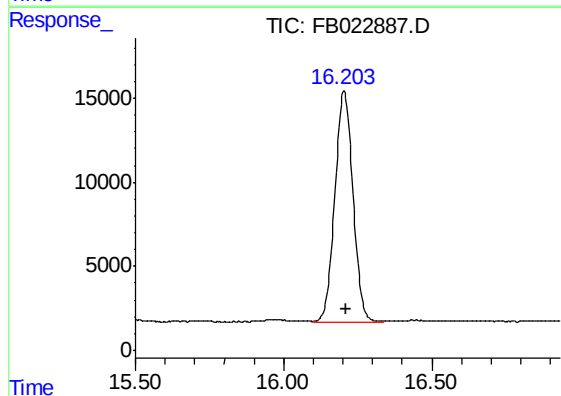

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.007 min
Response: 581846
Conc: 20.52 ng/ml