

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
 Data File : FB022896.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2019 19:21
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 06 07:49:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	440812	19.581 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	984957	30.620 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1040133	29.465 ng/ml
3) t n-Heptane	7.756	343631	9.879 ng/ml
4) t Benzene	7.890	440530	10.171 ng/ml
6) t Toluene	10.628	1292117	29.972 ng/ml
7) t Ethylbenzene	13.069	405281	10.152 ng/ml
8) t m-Xylene	13.202	765109	20.259 ng/ml
9) t O-Xylene	13.930	717346	20.127 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	577497	20.364 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110519\
Data File : FB022896.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2019 19:21
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 06 07:49:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

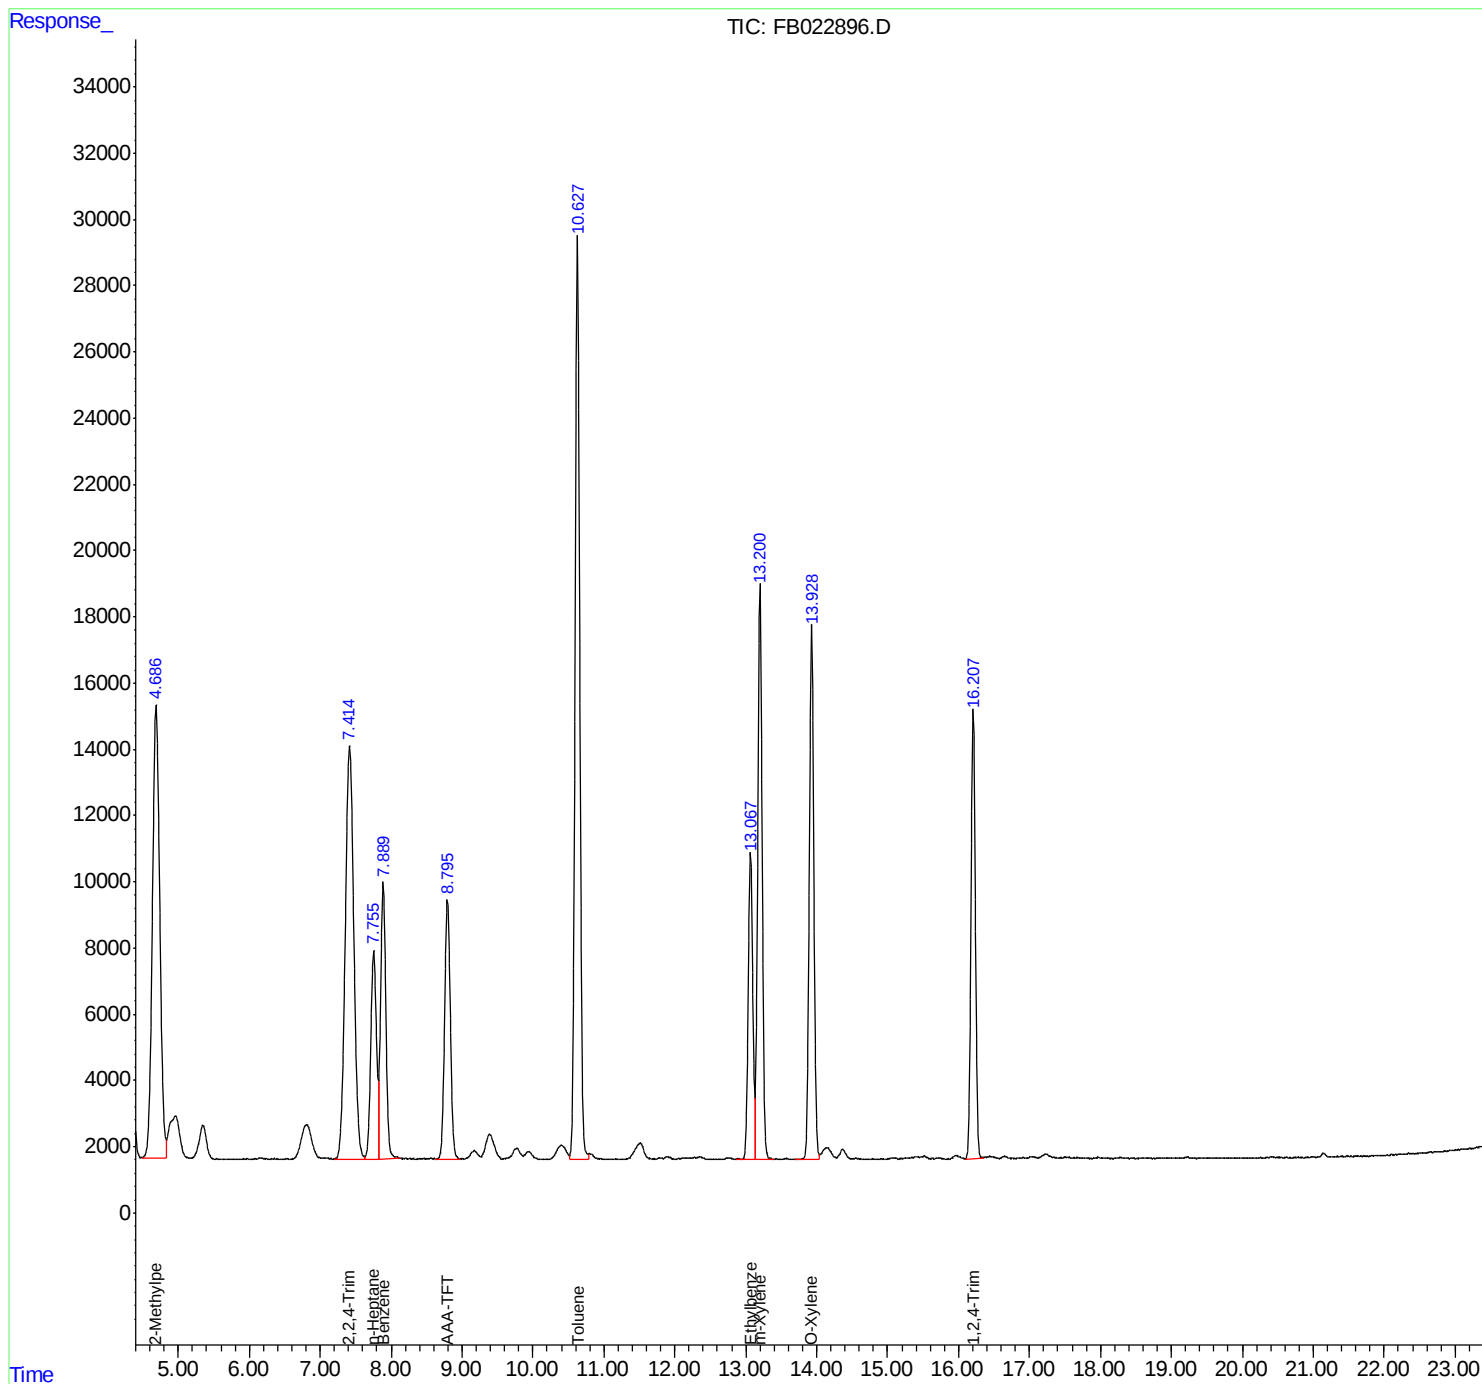


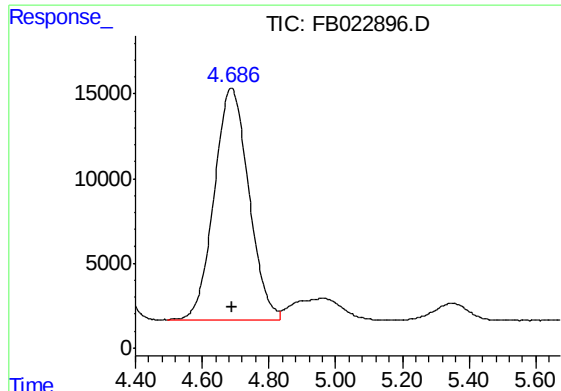

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 984957
Conc: 30.62 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

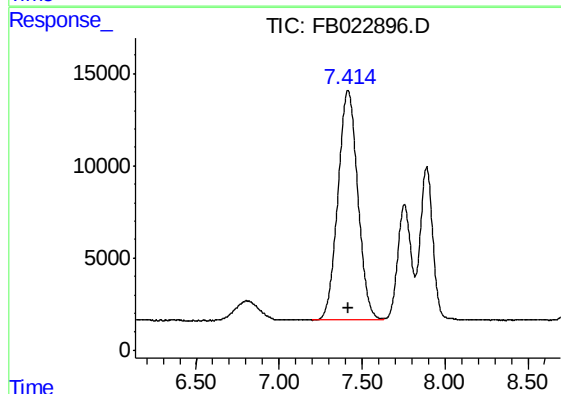


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1040133
Conc: 29.47 ng/ml

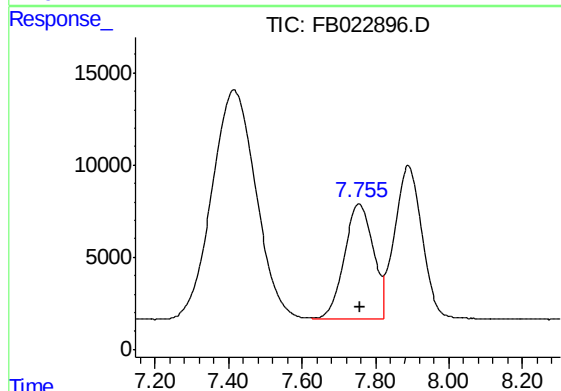


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 343631
Conc: 9.88 ng/ml

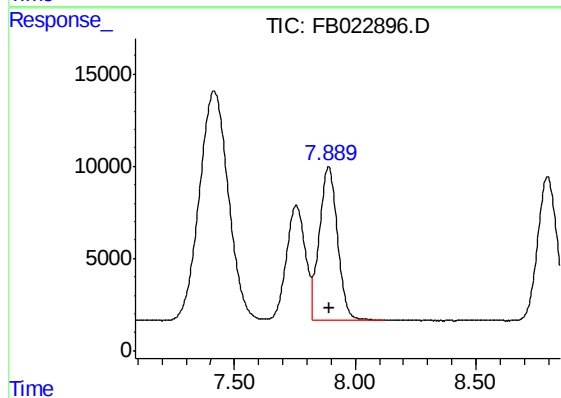

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 440530
Conc: 10.17 ng/ml

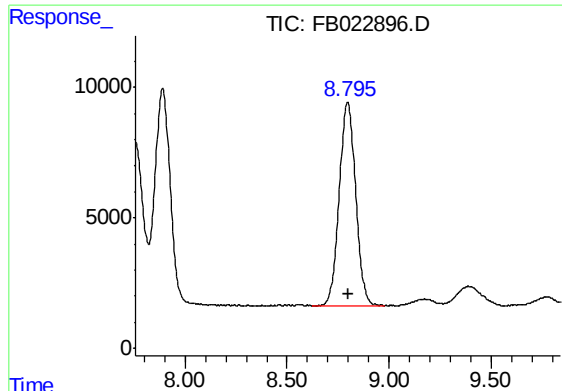

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 440812
Conc: 19.58 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

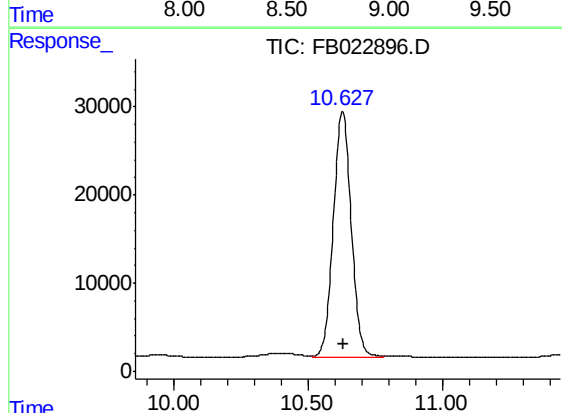


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1292117
Conc: 29.97 ng/ml

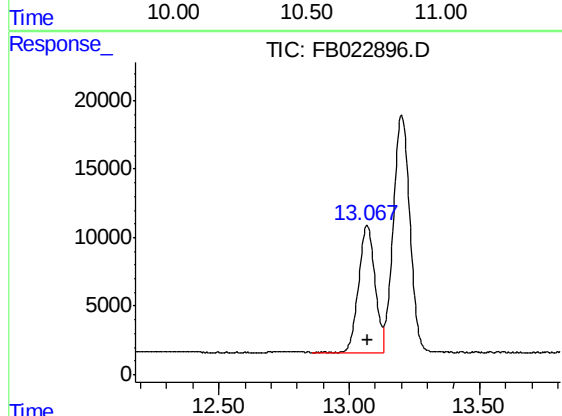


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 405281
Conc: 10.15 ng/ml

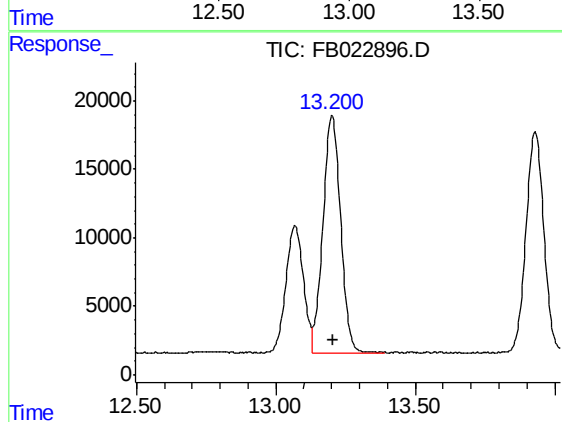

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 765109
Conc: 20.26 ng/ml

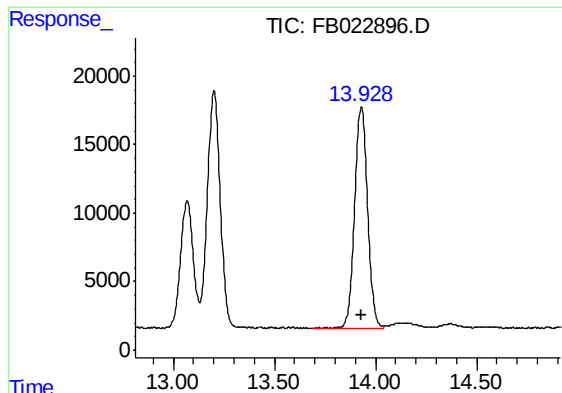

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 717346
Conc: 20.13 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

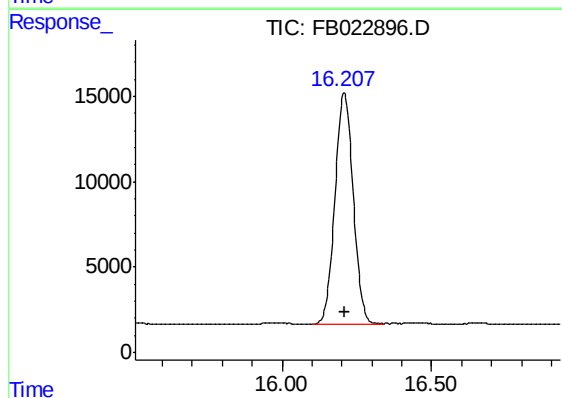

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 577497
Conc: 20.36 ng/ml