

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
 Data File : FB025193.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2020 11:04
 Operator : DD/AJ
 Sample : VBF1105S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 15:20:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	393053	17.408 ng/ml
Target Compounds			
6) t Toluene	10.631	29577	0.791 ng/ml
8) t m-Xylene	13.200	31013	0.919 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
Data File : FB025193.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2020 11:04
Operator : DD/AJ
Sample : VBF1105S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 15:20:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

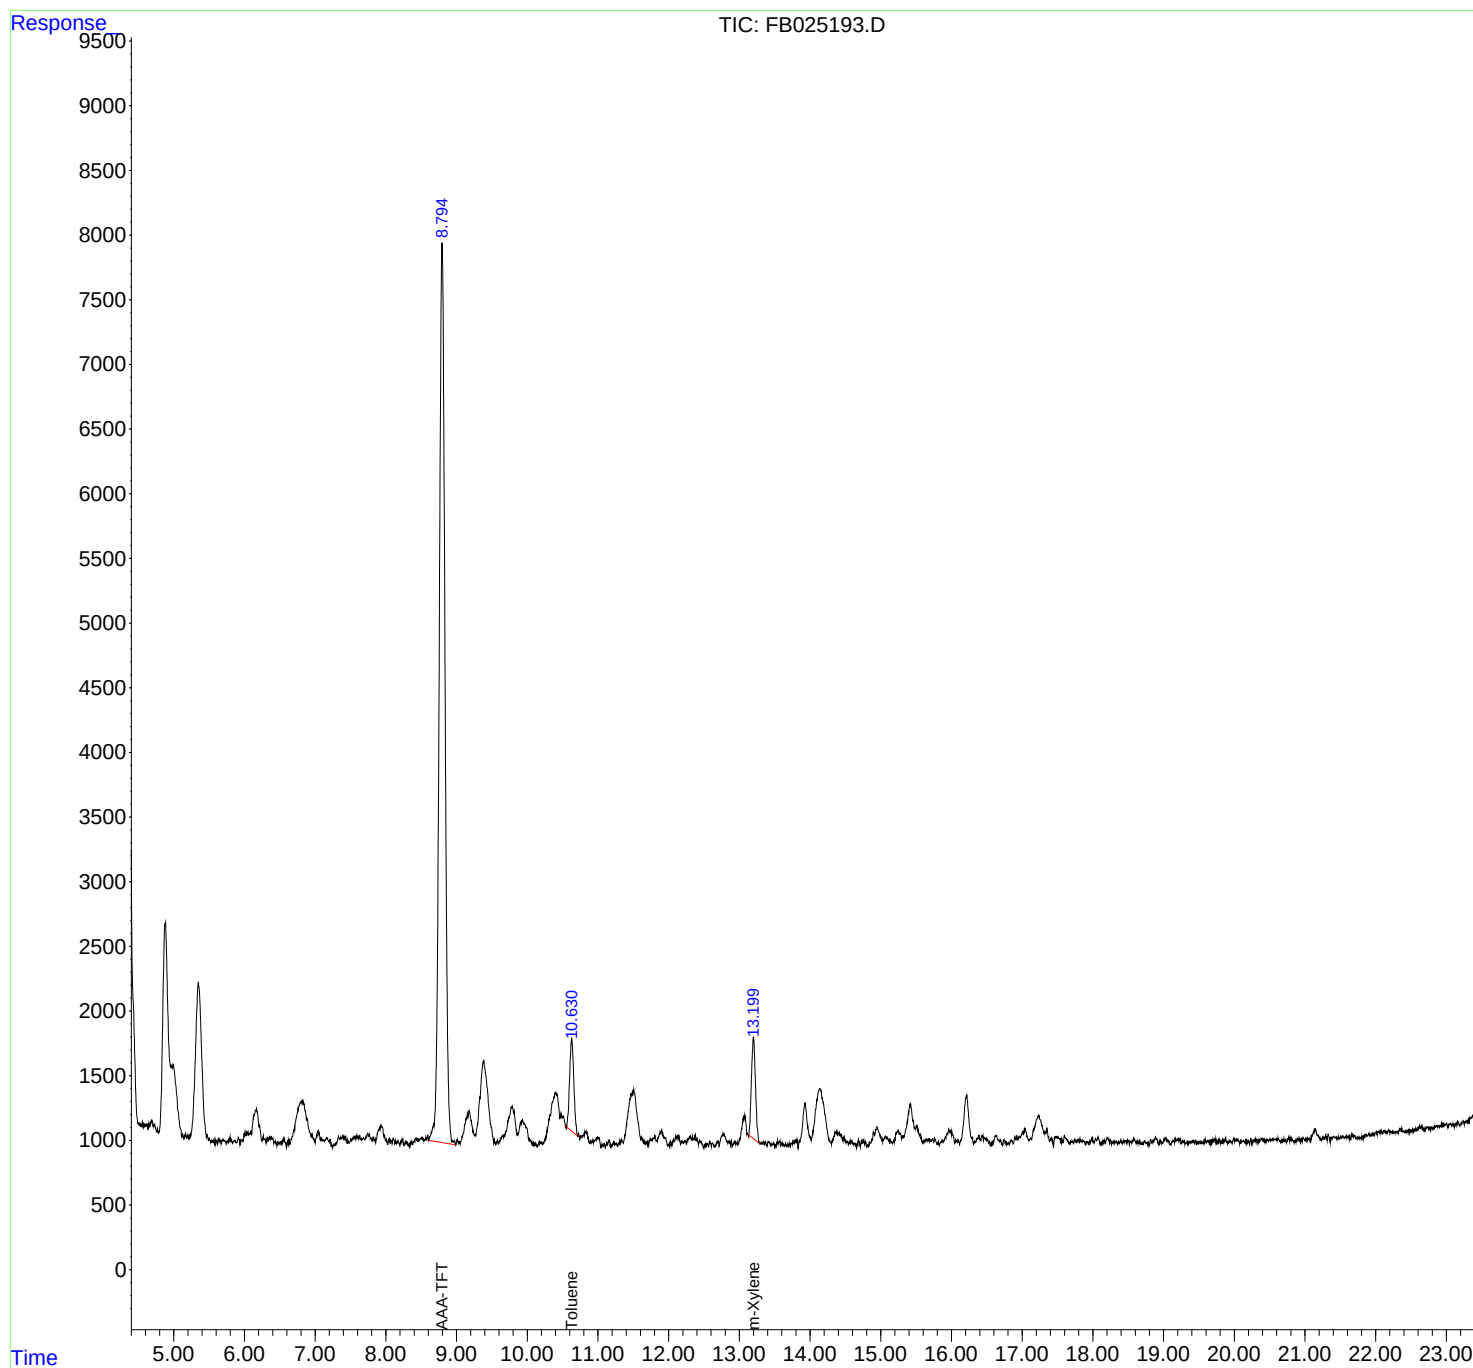


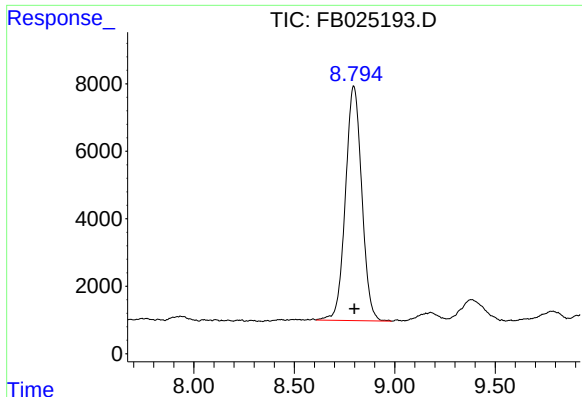

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 393053
Conc: 17.41 ng/ml

Instrument :
FID_B
ClientSampleId :

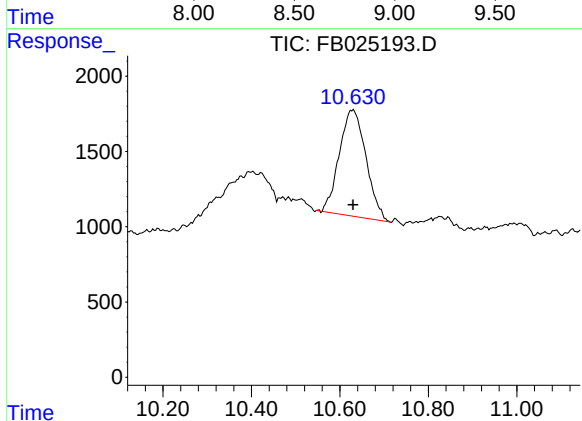

#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 29577
Conc: 0.79 ng/ml

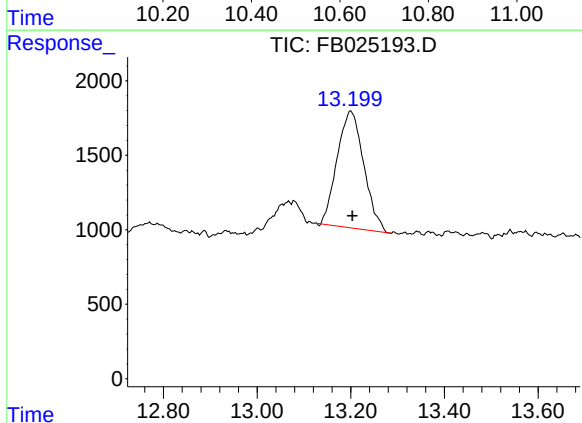

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 31013
Conc: 0.92 ng/ml