

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
 Data File : FB025195.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2020 12:42
 Operator : DD/AJ
 Sample : L4548-15 1000X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 15:20:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.820	989959	43.843 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	290205	8.991 ng/ml
2) t 2,2,4-Trimethylpentane	7.383	622389	18.759 ng/ml
3) t n-Heptane	7.756	913686	27.818 ng/ml
4) t Benzene	7.883	147975	3.722 ng/ml
6) t Toluene	10.630	2105523	56.311 ng/ml
7) t Ethylbenzene	13.068	679161	19.777 ng/ml
8) t m-Xylene	13.200	1912658	56.647 ng/ml
9) t O-Xylene	13.930	773993	23.672 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	768180	27.919 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
Data File : FB025195.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2020 12:42
Operator : DD/AJ
Sample : L4548-15 1000X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 15:20:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

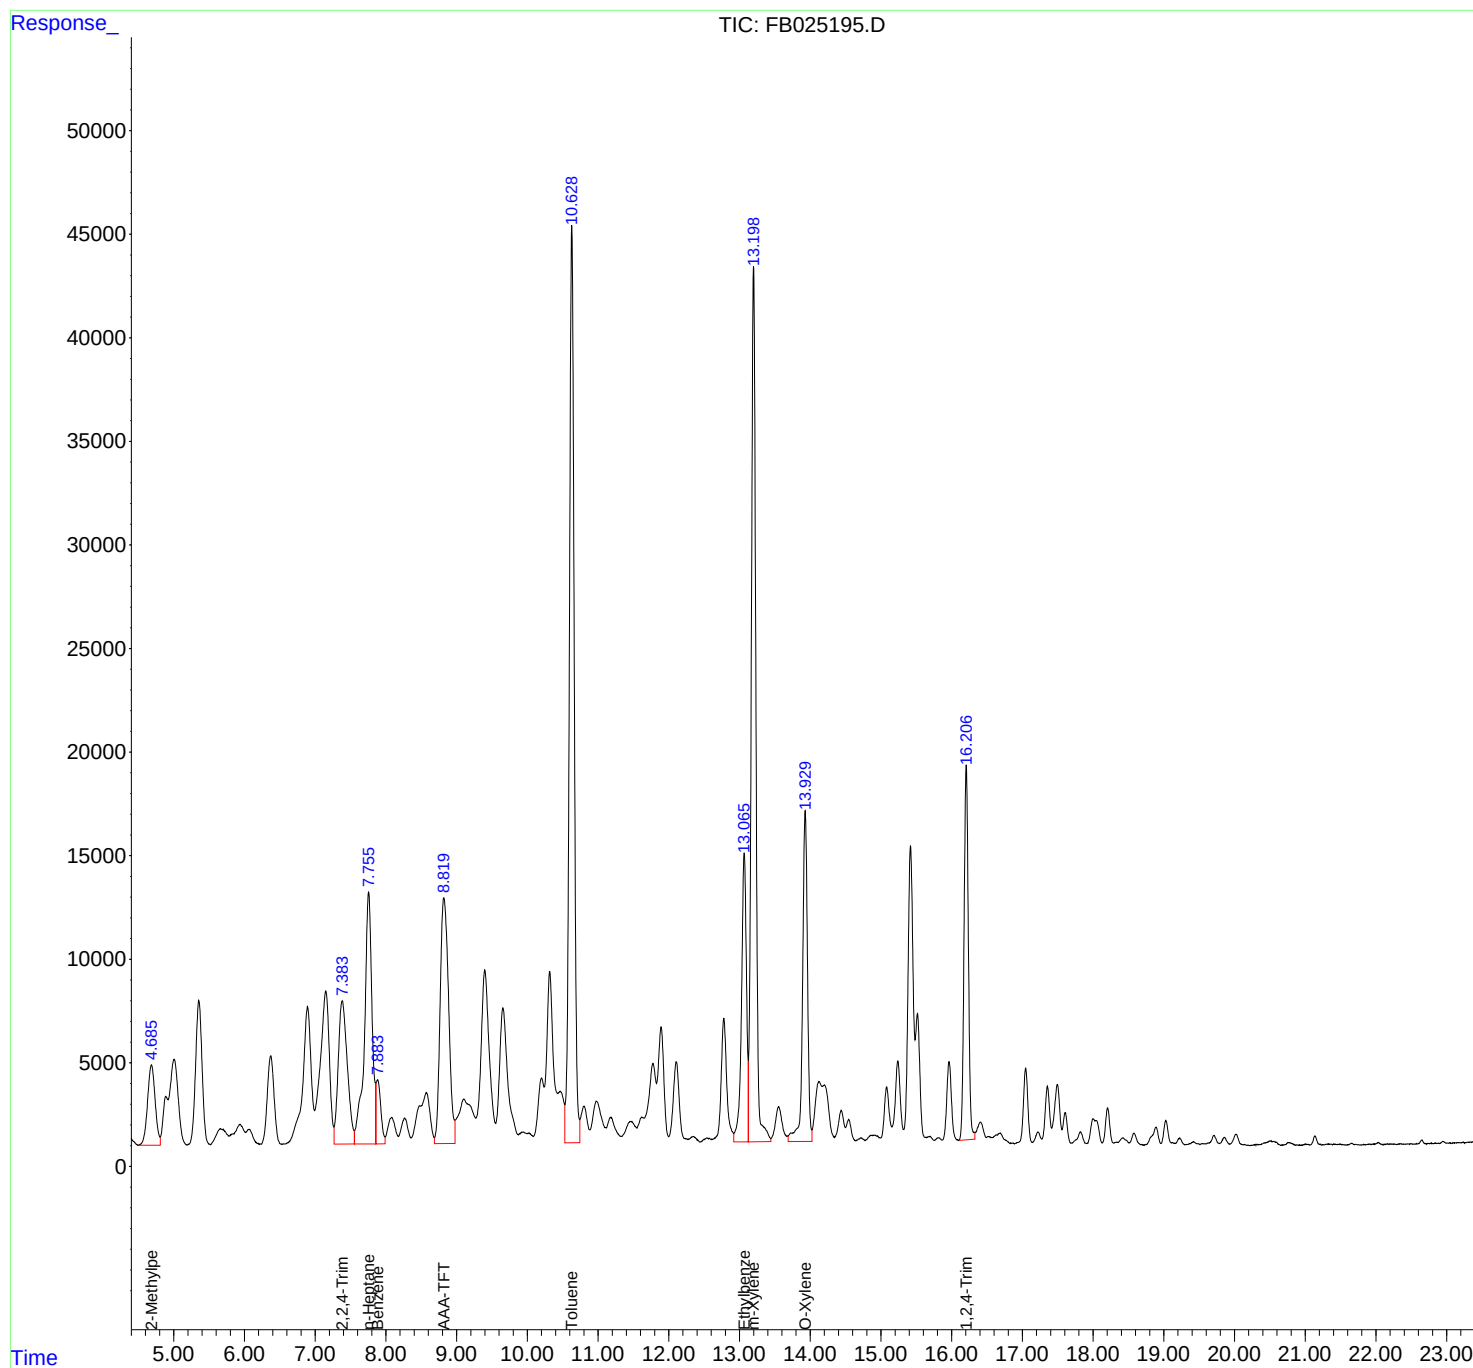


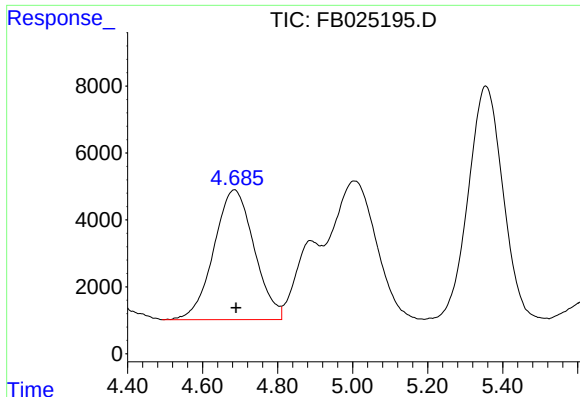

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 290205
Conc: 8.99 ng/ml

Instrument :
FID_B
ClientSampleId :

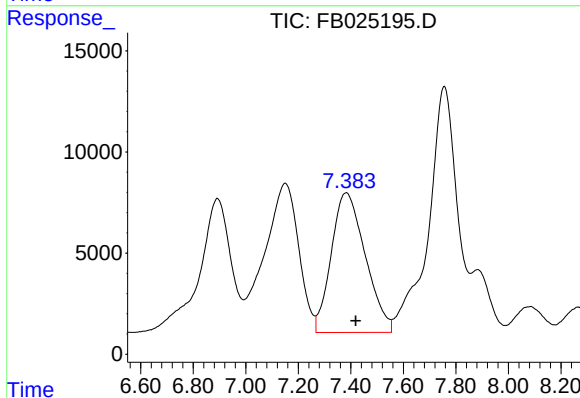


#2 2,2,4-Trimethylpentane

R.T.: 7.383 min
Delta R.T.: -0.035 min
Response: 622389
Conc: 18.76 ng/ml

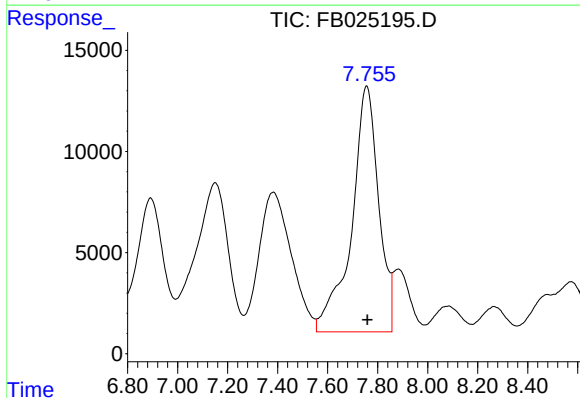


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 913686
Conc: 27.82 ng/ml

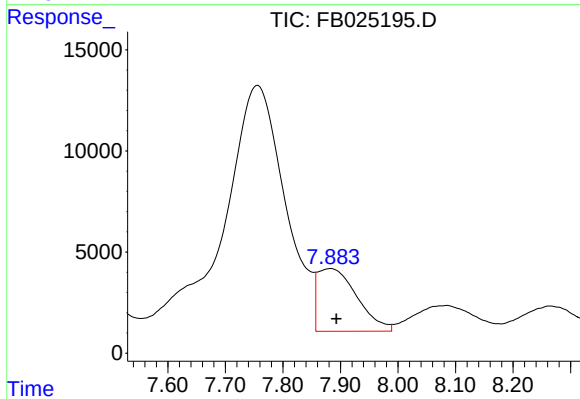

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.010 min
Response: 147975
Conc: 3.72 ng/ml

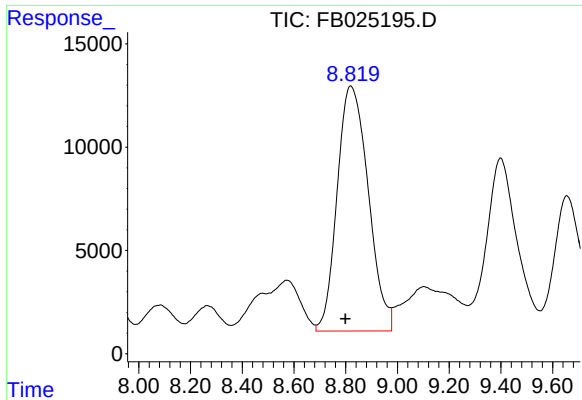

#5 AAA-TFT


R.T.: 8.820 min
Delta R.T.: 0.021 min
Response: 989959
Conc: 43.84 ng/ml

Instrument :
FID_B
ClientSampleId :

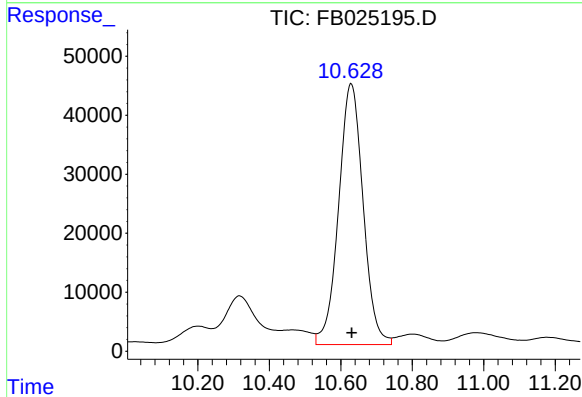


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 2105523
Conc: 56.31 ng/ml

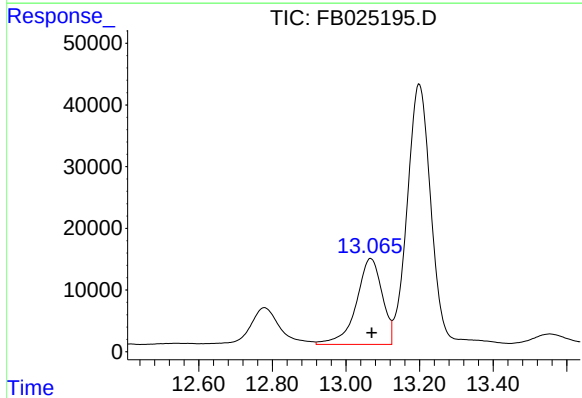


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 679161
Conc: 19.78 ng/ml

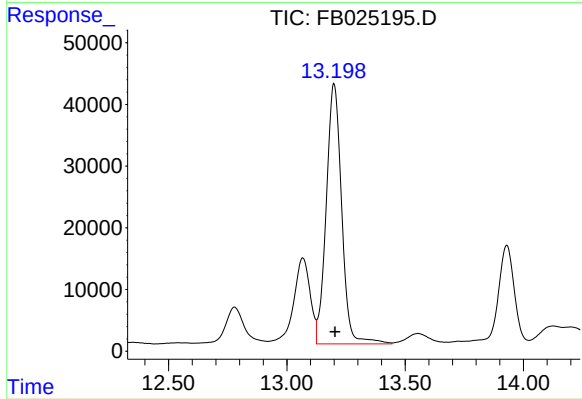

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 1912658
Conc: 56.65 ng/ml

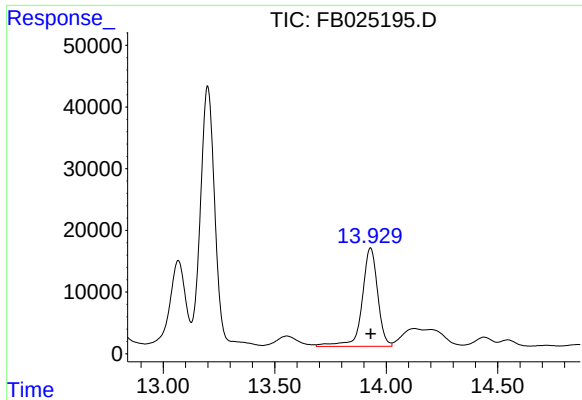

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 773993
Conc: 23.67 ng/ml

Instrument :
FID_B
ClientSampleId :

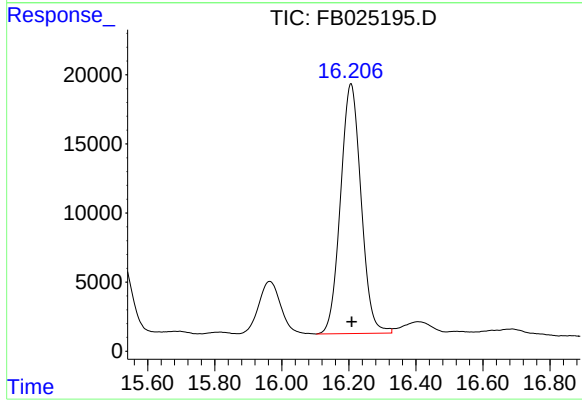

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 768180
Conc: 27.92 ng/ml