

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
 Data File : FB025197.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2020 14:18
 Operator : DD/AJ
 Sample : L4621-03MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 05 15:20:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	465344	20.609 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	972046	30.115 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	996998	30.050 ng/ml
3) t n-Heptane	7.758	330086	10.050 ng/ml
4) t Benzene	7.893	407631	10.252 ng/ml
6) t Toluene	10.630	1150589	30.772 ng/ml
7) t Ethylbenzene	13.070	353165	10.284 ng/ml
8) t m-Xylene	13.202	701407	20.774 ng/ml
9) t O-Xylene	13.930	670660	20.512 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	559806	20.345 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
Data File : FB025197.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2020 14:18
Operator : DD/AJ
Sample : L4621-03MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 05 15:20:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

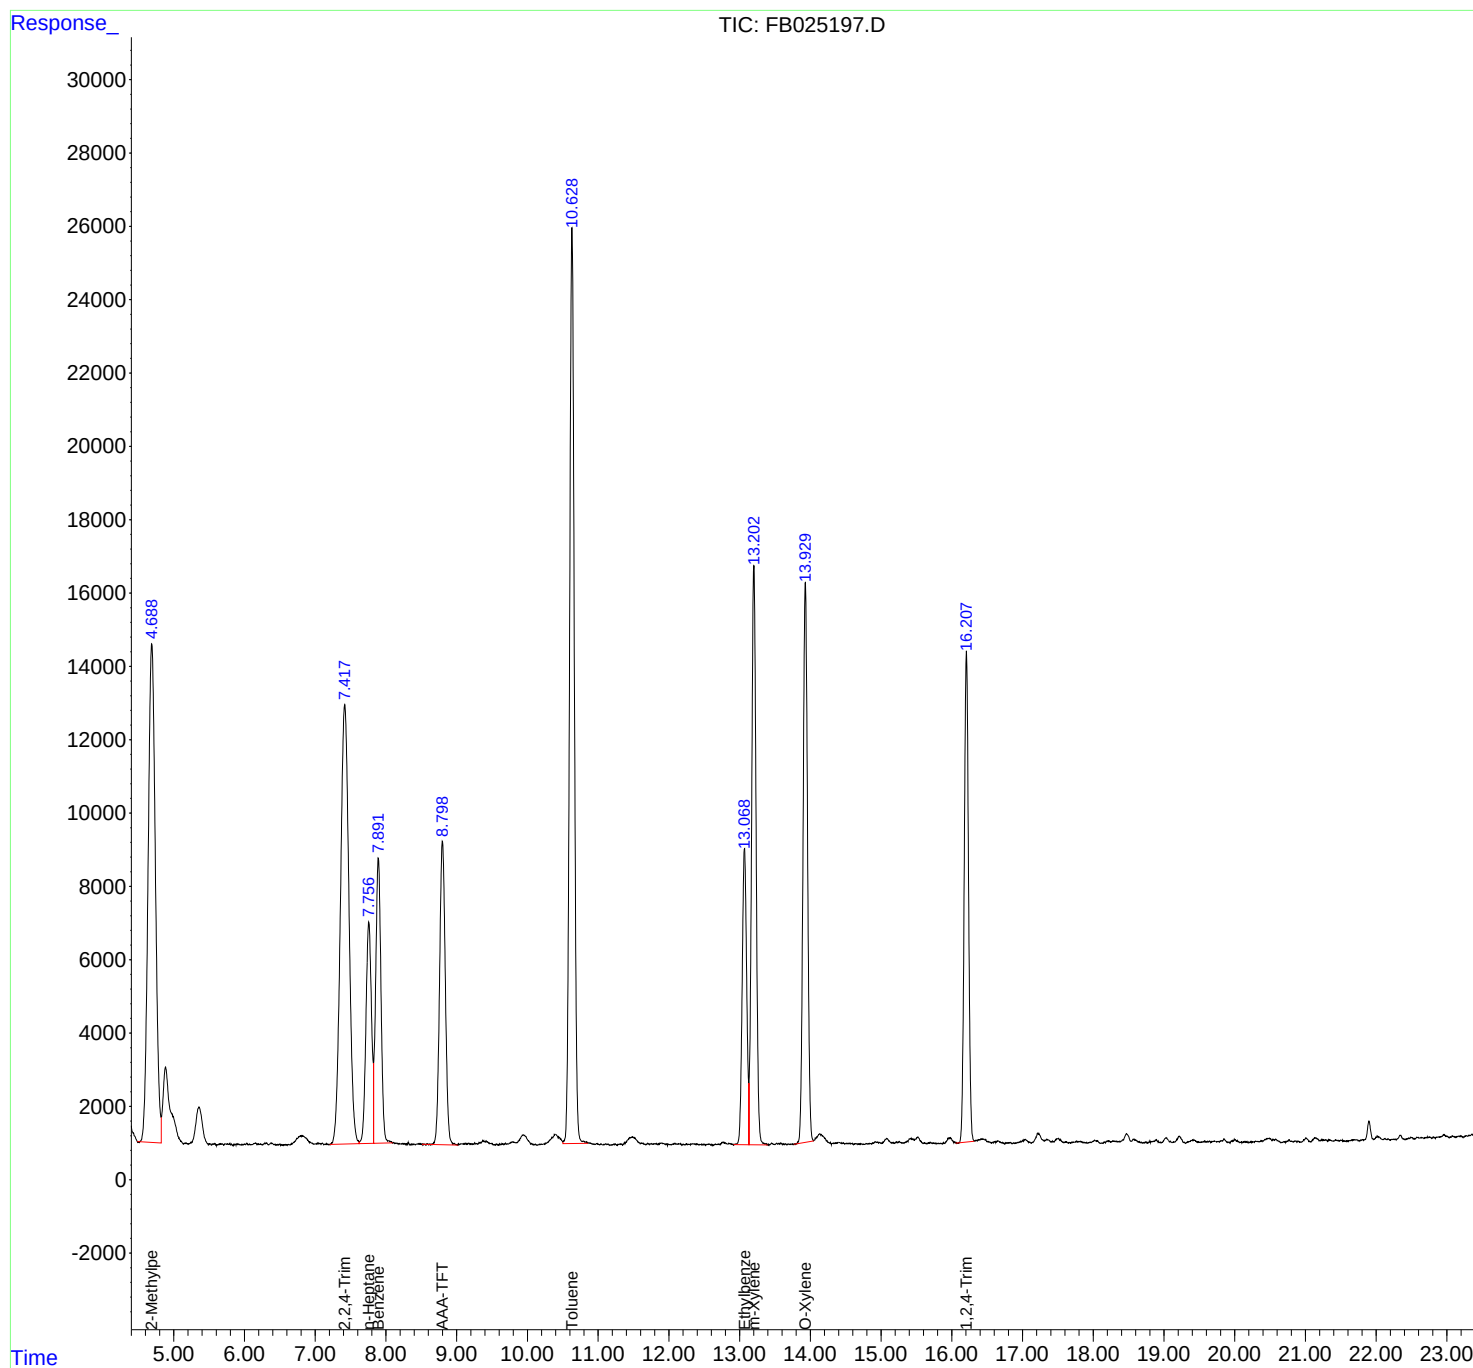


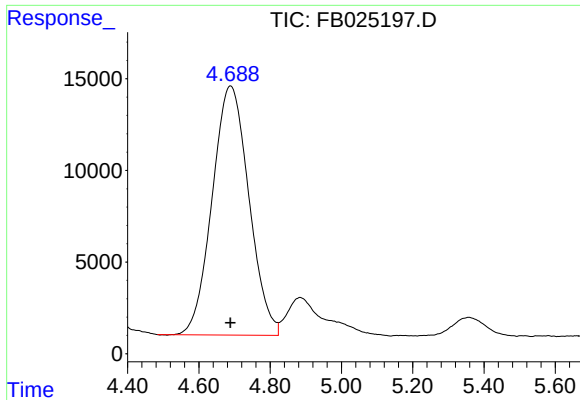

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 972046
Conc: 30.12 ng/ml

Instrument :
FID_B
ClientSampleId :

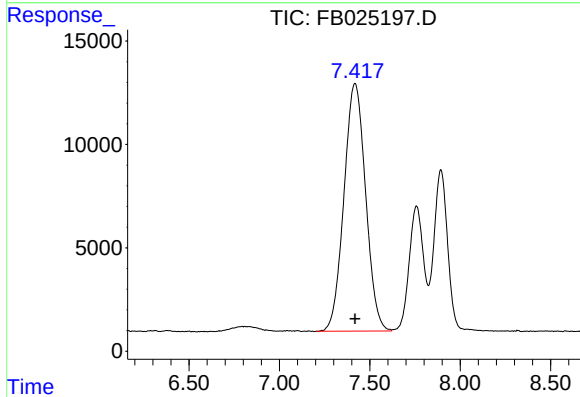


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 996998
Conc: 30.05 ng/ml

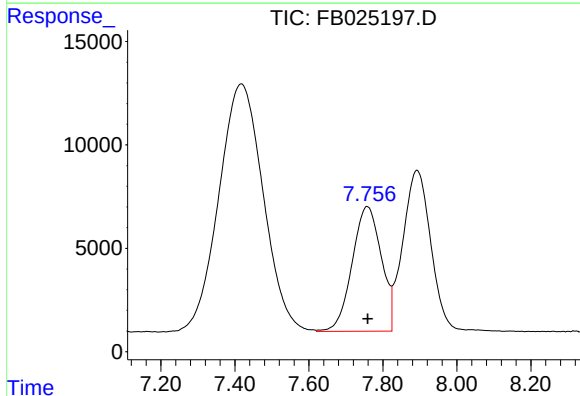


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 330086
Conc: 10.05 ng/ml

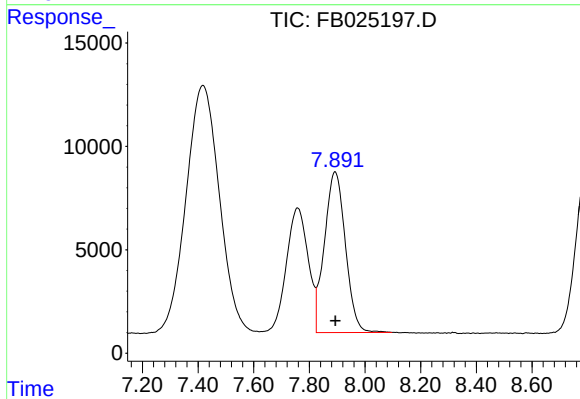

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 407631
Conc: 10.25 ng/ml

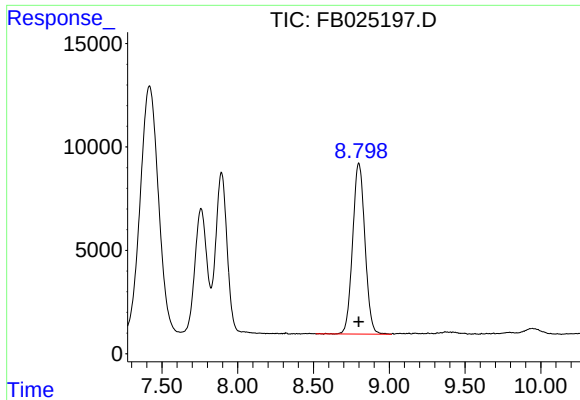

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 465344
Conc: 20.61 ng/ml

Instrument :
FID_B
ClientSampleId :

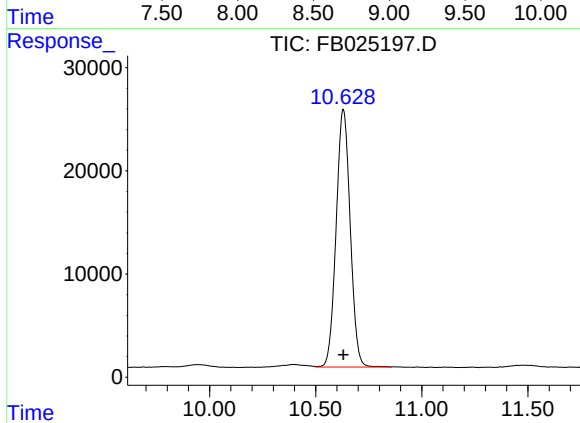


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1150589
Conc: 30.77 ng/ml

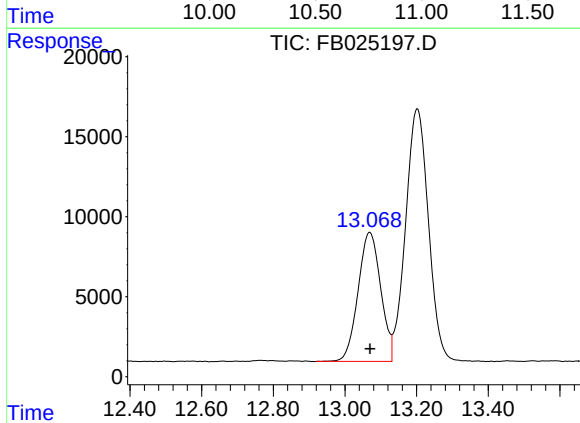


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 353165
Conc: 10.28 ng/ml

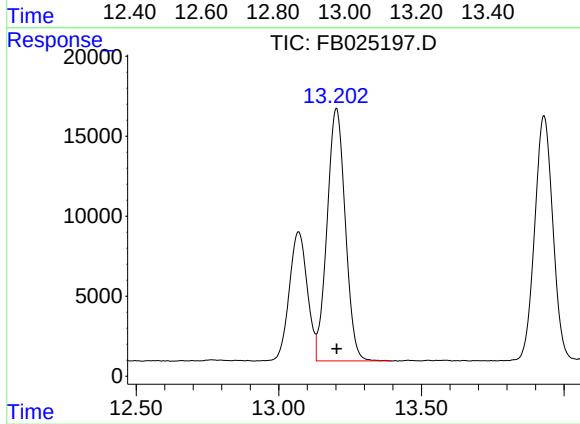

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 701407
Conc: 20.77 ng/ml

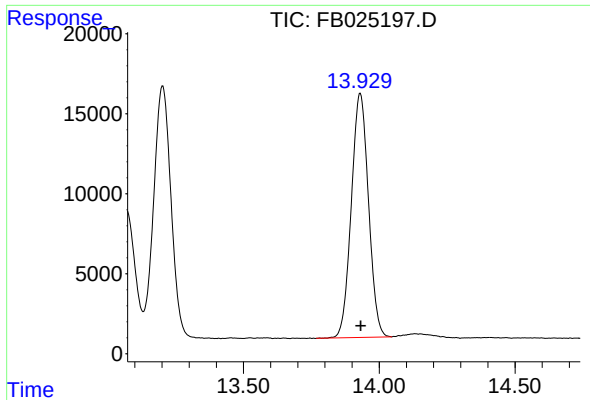

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 670660
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :

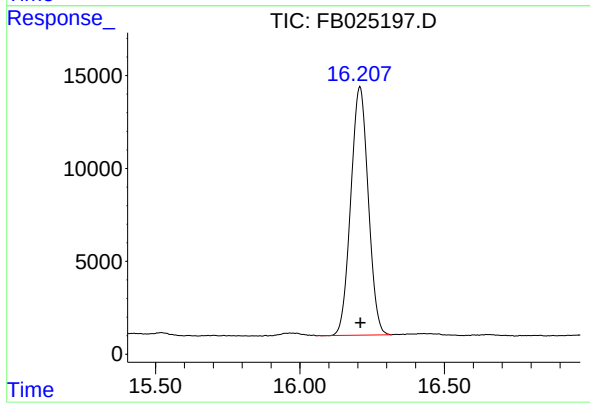

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 559806
Conc: 20.35 ng/ml