

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
 Data File : FB025190.D
 Signal(s) : FID2B.CH
 Acq On : 5 Nov 2020 9:31
 Operator : DD/AJ
 Sample : BSF1105S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1105S1

Integration File: Calibration.e
 Quant Time: Nov 05 15:19:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	416213	18.433 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	943990	29.246 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1000643	30.160 ng/ml
3) t n-Heptane	7.758	329008	10.017 ng/ml
4) t Benzene	7.893	392143	9.863 ng/ml
6) t Toluene	10.630	1113513	29.780 ng/ml
7) t Ethylbenzene	13.069	327121	9.526 ng/ml
8) t m-Xylene	13.202	659642	19.537 ng/ml
9) t O-Xylene	13.929	637301	19.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	515289	18.728 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110520\
Data File : FB025190.D
Signal(s) : FID2B.CH
Acq On : 5 Nov 2020 9:31
Operator : DD/AJ
Sample : BSF1105S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1105S1

Integration File: Calibration.e
Quant Time: Nov 05 15:19:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

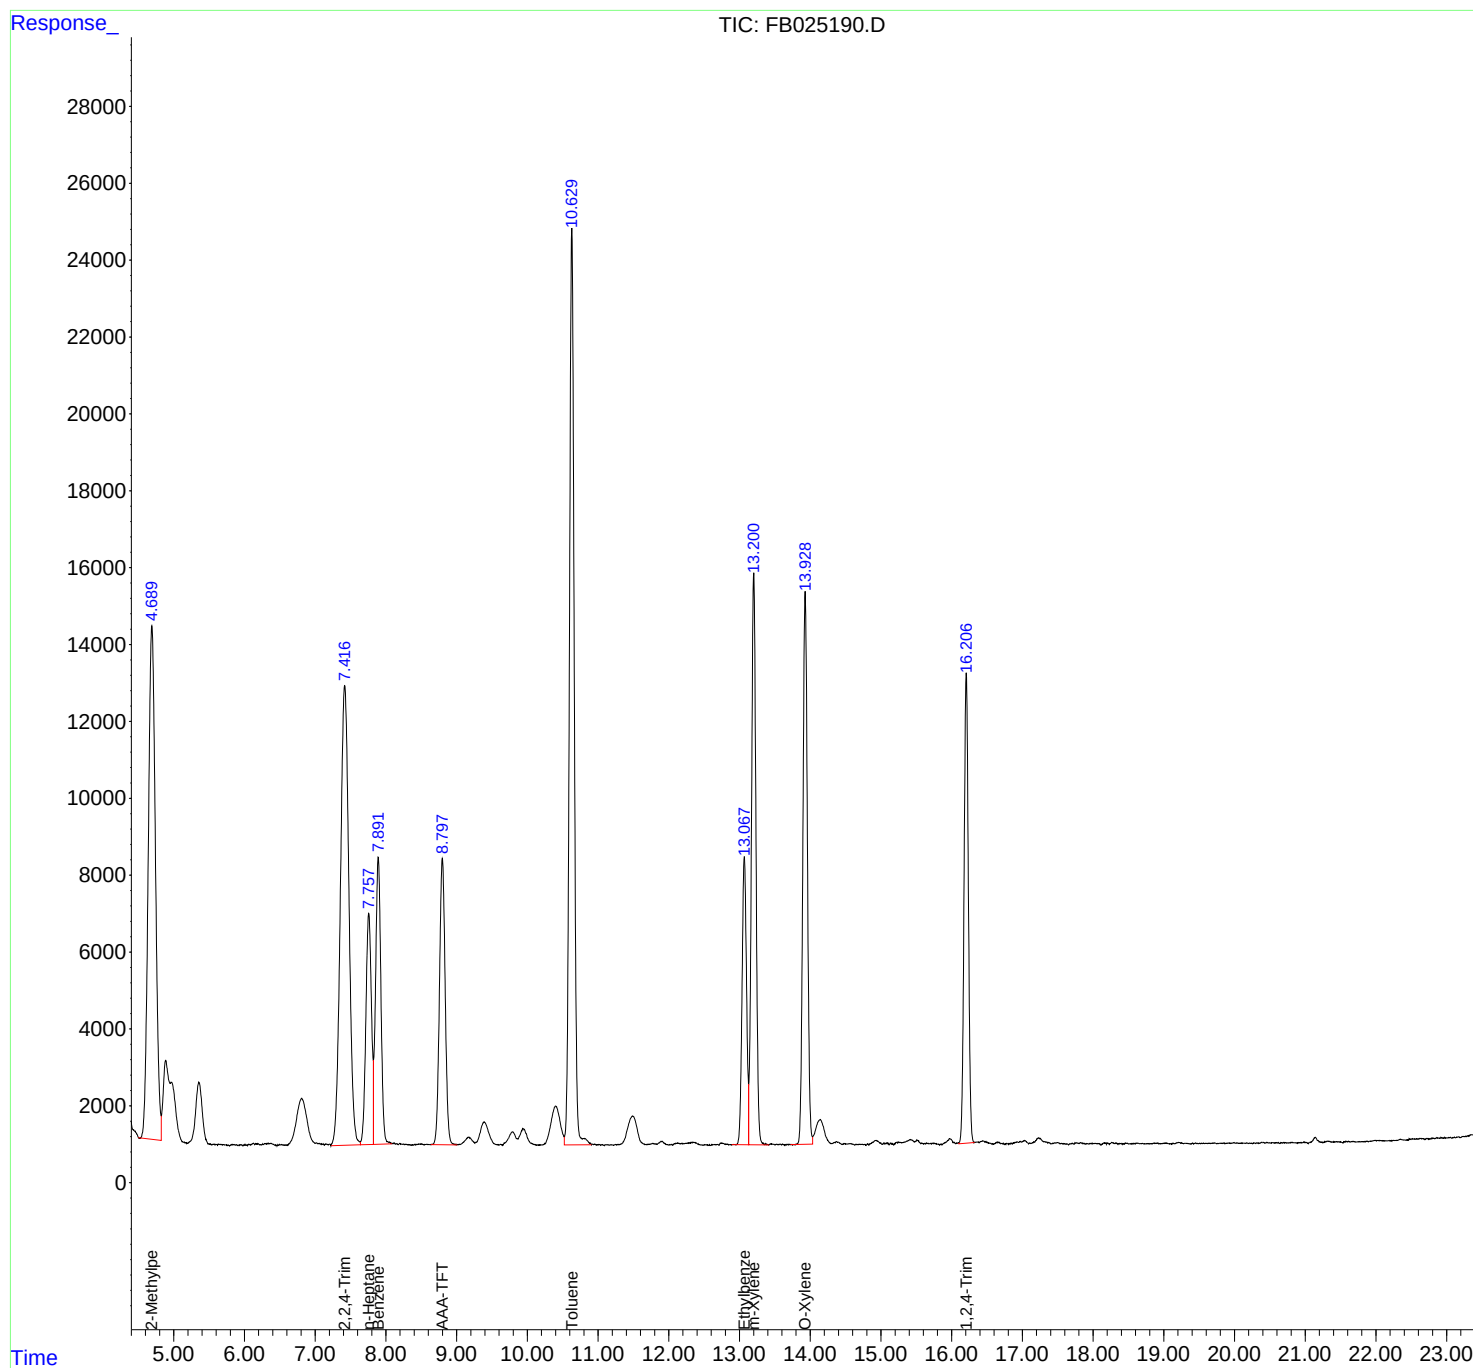


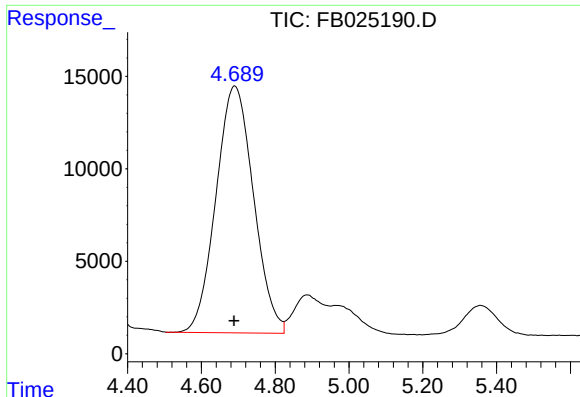

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 943990
Conc: 29.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

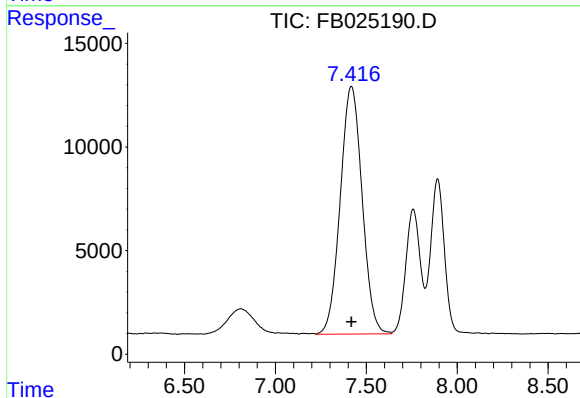


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1000643
Conc: 30.16 ng/ml

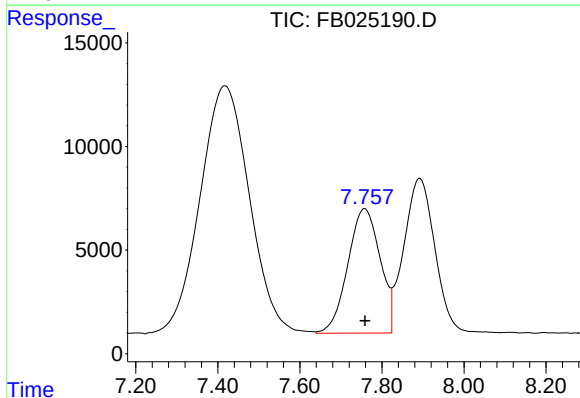


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 329008
Conc: 10.02 ng/ml

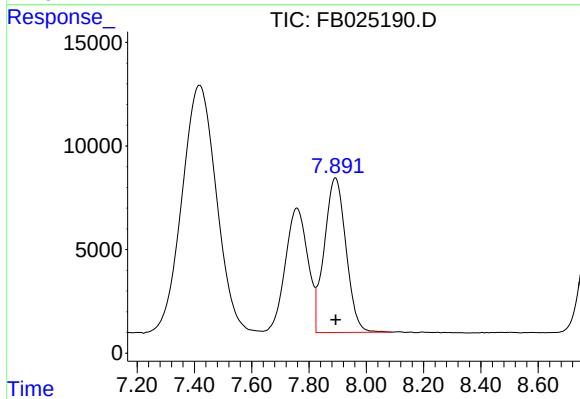

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 392143
Conc: 9.86 ng/ml

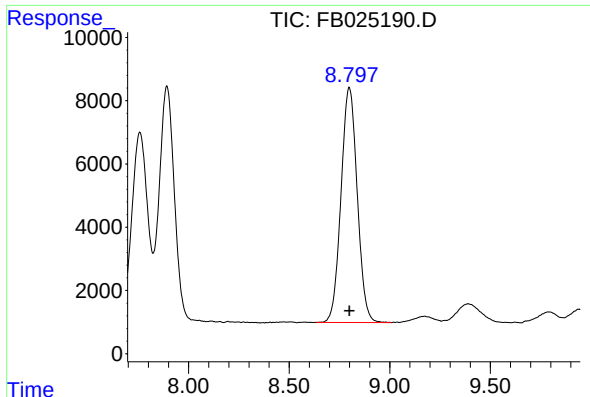

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 416213
Conc: 18.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

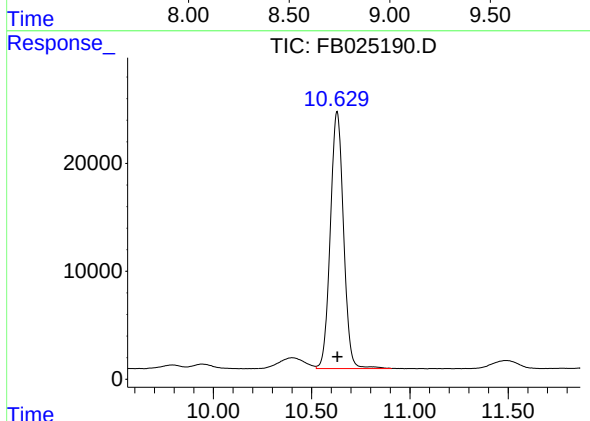


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1113513
Conc: 29.78 ng/ml

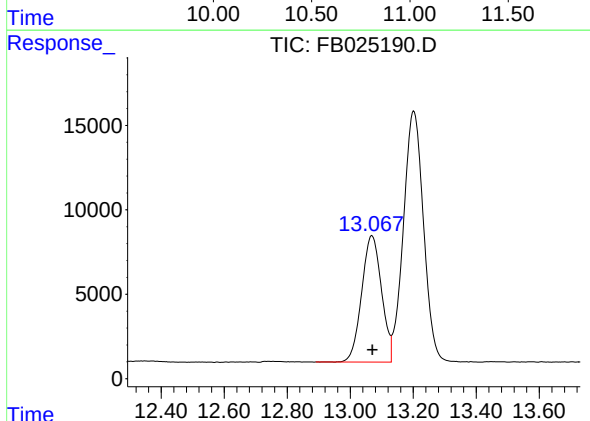


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 327121
Conc: 9.53 ng/ml

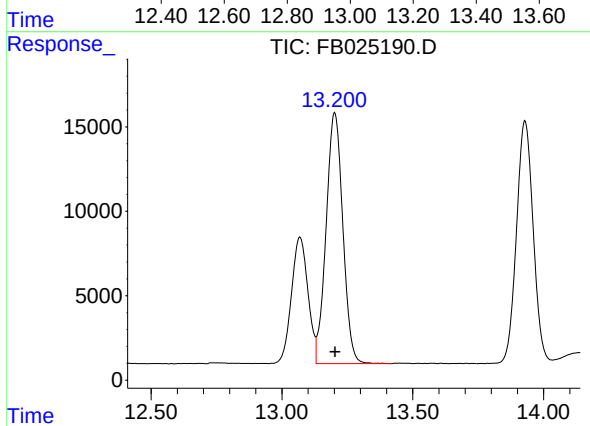

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 659642
Conc: 19.54 ng/ml

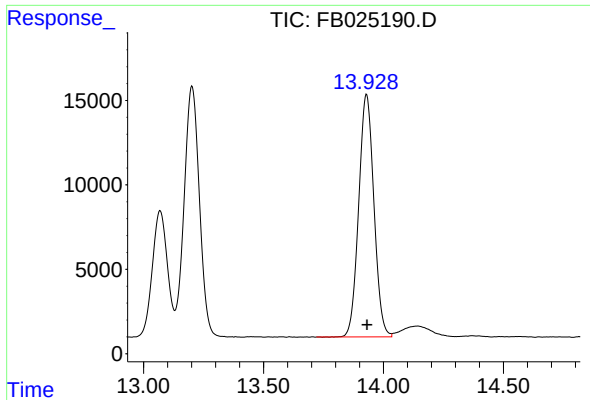

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 637301
Conc: 19.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1105S1

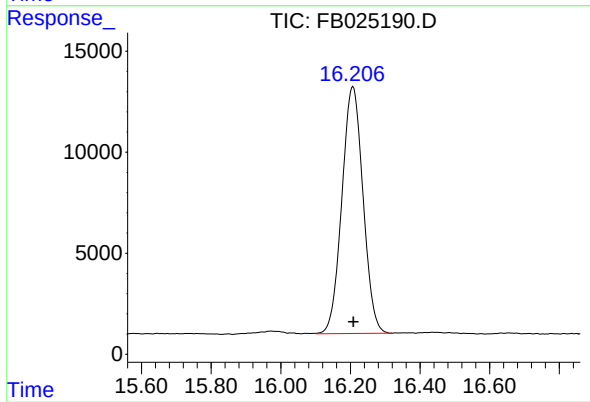

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 515289
Conc: 18.73 ng/ml