

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110618\
 Data File : FB018573.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2018 1:34
 Operator : MJ/SJ
 Sample : J5826-10MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 07 07:49:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	168438	19.557 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	352010	23.016 ng/ml
2) t 2,2,4-Trimethylpentane	7.724	368041	24.907 ng/ml
3) t n-Heptane	8.065	113307	7.996 ng/ml
4) t Benzene	8.203	148975	7.997 ng/ml
6) t Toluene	10.958	387378	25.417 ng/ml
7) t Ethylbenzene	13.407	126084	7.947 ng/ml
8) t m-Xylene	13.540	268552	16.140 ng/ml
9) t O-Xylene	14.272	282239	15.830 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	334585	16.447 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110618\
Data File : FB018573.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2018 1:34
Operator : MJ/SJ
Sample : J5826-10MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 07 07:49:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

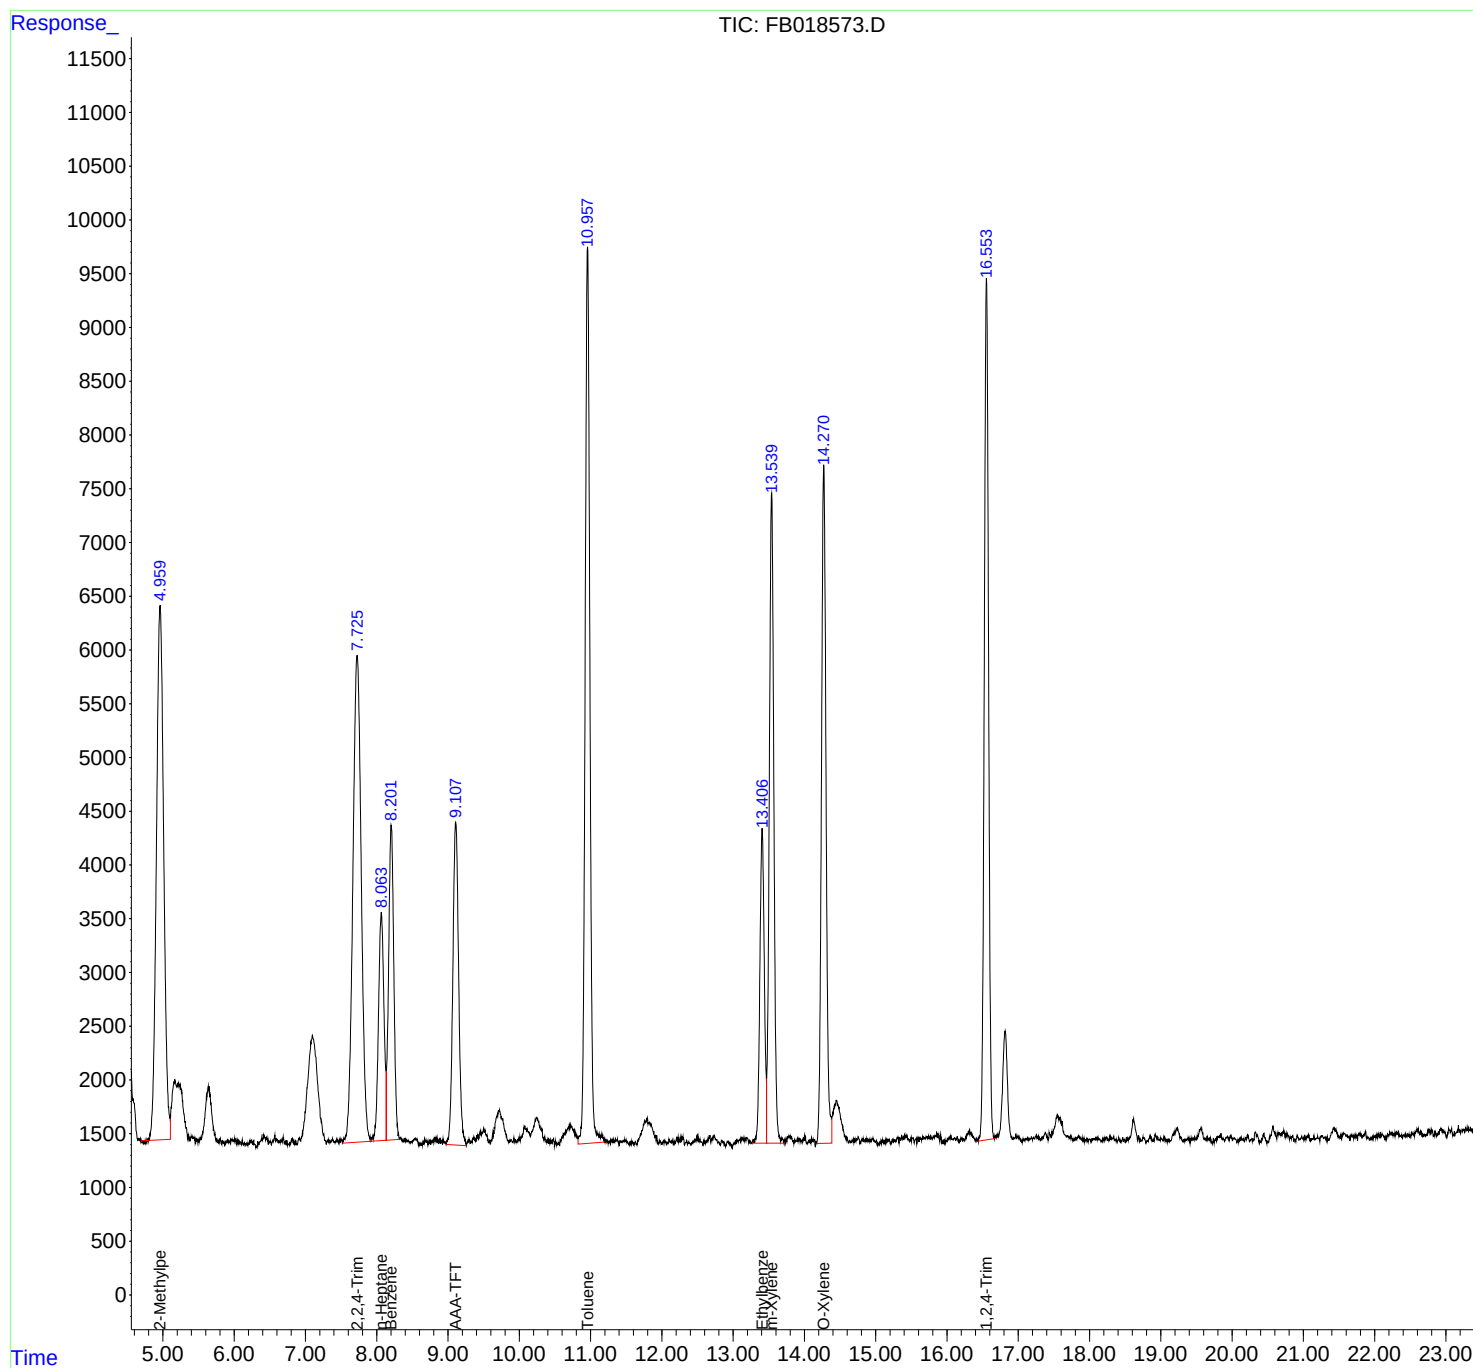

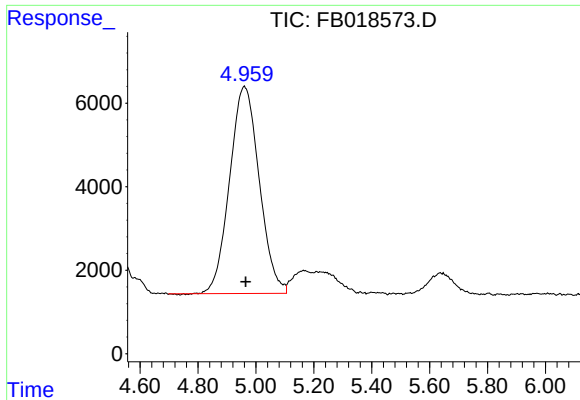


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 352010
Conc: 23.02 ng/ml

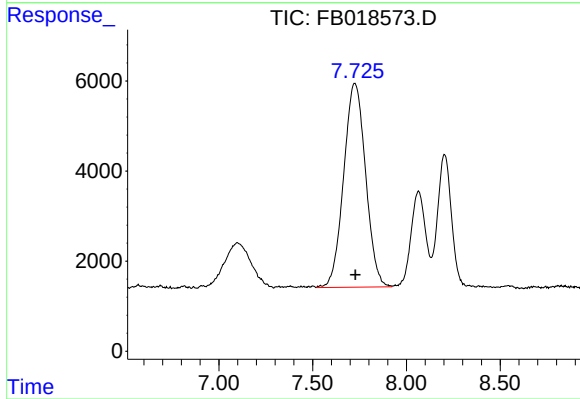


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: -0.004 min
Response: 368041
Conc: 24.91 ng/ml

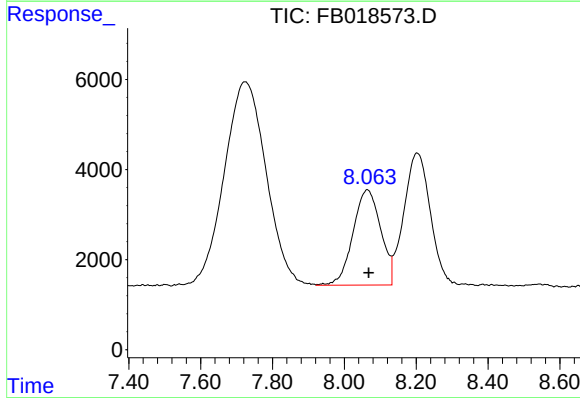


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 113307
Conc: 8.00 ng/ml

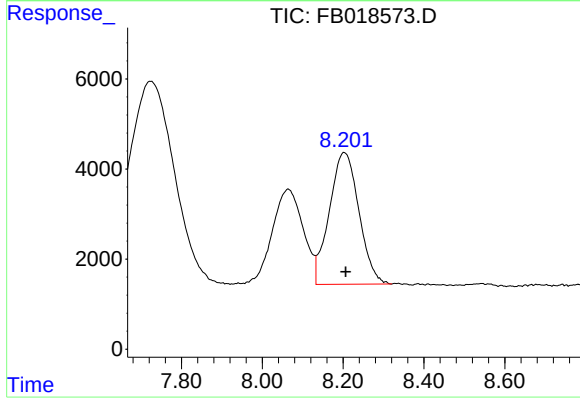


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 148975
Conc: 8.00 ng/ml

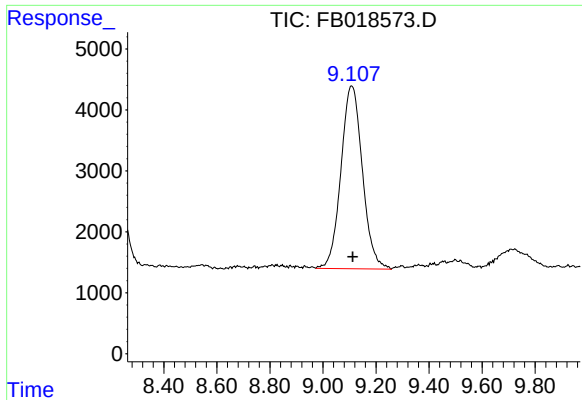


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 168438
Conc: 19.56 ng/ml

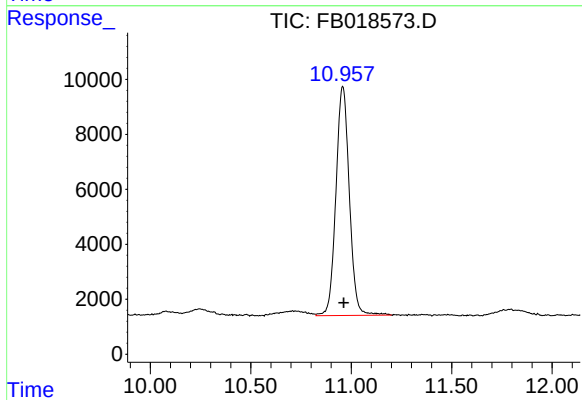


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.004 min
Response: 387378
Conc: 25.42 ng/ml

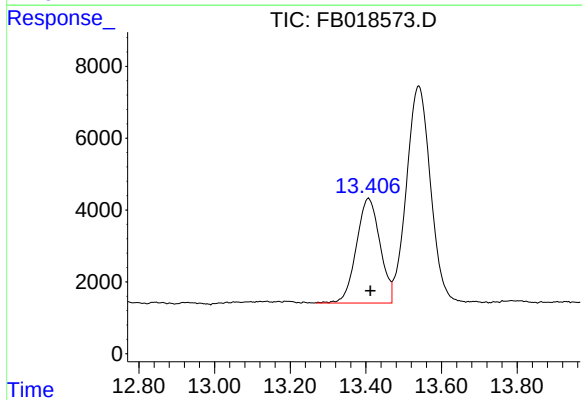


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.005 min
Response: 126084
Conc: 7.95 ng/ml

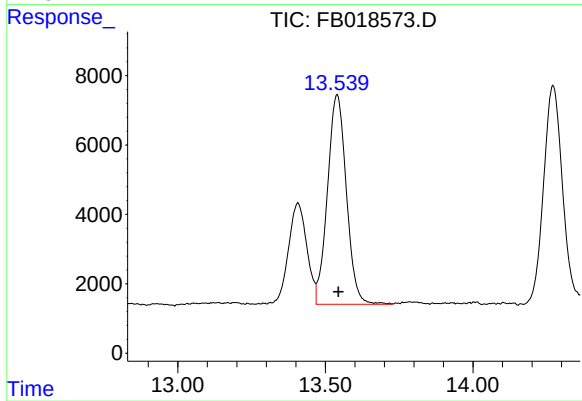


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.004 min
Response: 268552
Conc: 16.14 ng/ml

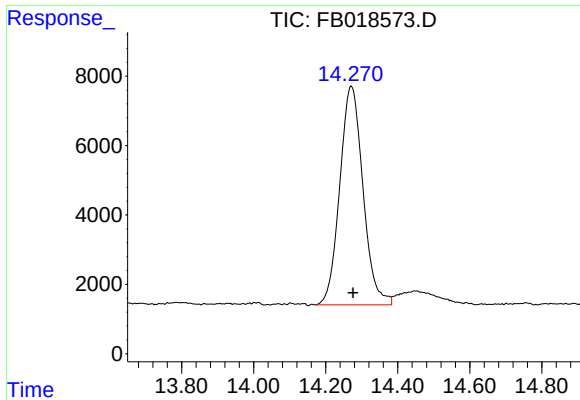

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.005 min
Response: 282239
Conc: 15.83 ng/ml

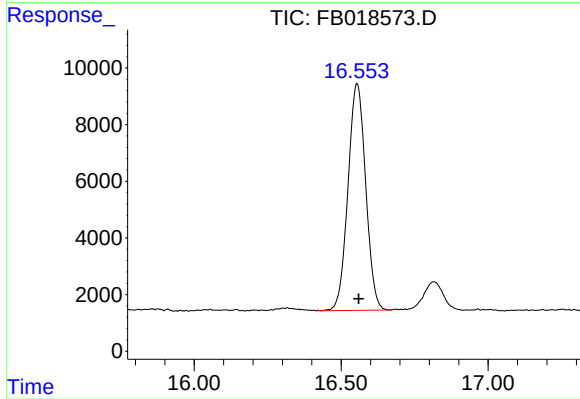

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.005 min
Response: 334585
Conc: 16.45 ng/ml