

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110618\
 Data File : FB018574.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2018 2:04
 Operator : MJ/SJ
 Sample : J5826-10MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 07 07:49:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	156605	18.183 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	350105	22.891 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	375965	25.443 ng/ml
3) t n-Heptane	8.065	117714	8.306 ng/ml
4) t Benzene	8.204	152274	8.174 ng/ml
6) t Toluene	10.958	392099	25.727 ng/ml
7) t Ethylbenzene	13.408	130457	8.223 ng/ml
8) t m-Xylene	13.540	276200	16.600 ng/ml
9) t O-Xylene	14.272	291060	16.324 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	341063	16.765 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110618\
Data File : FB018574.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2018 2:04
Operator : MJ/SJ
Sample : J5826-10MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 07 07:49:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

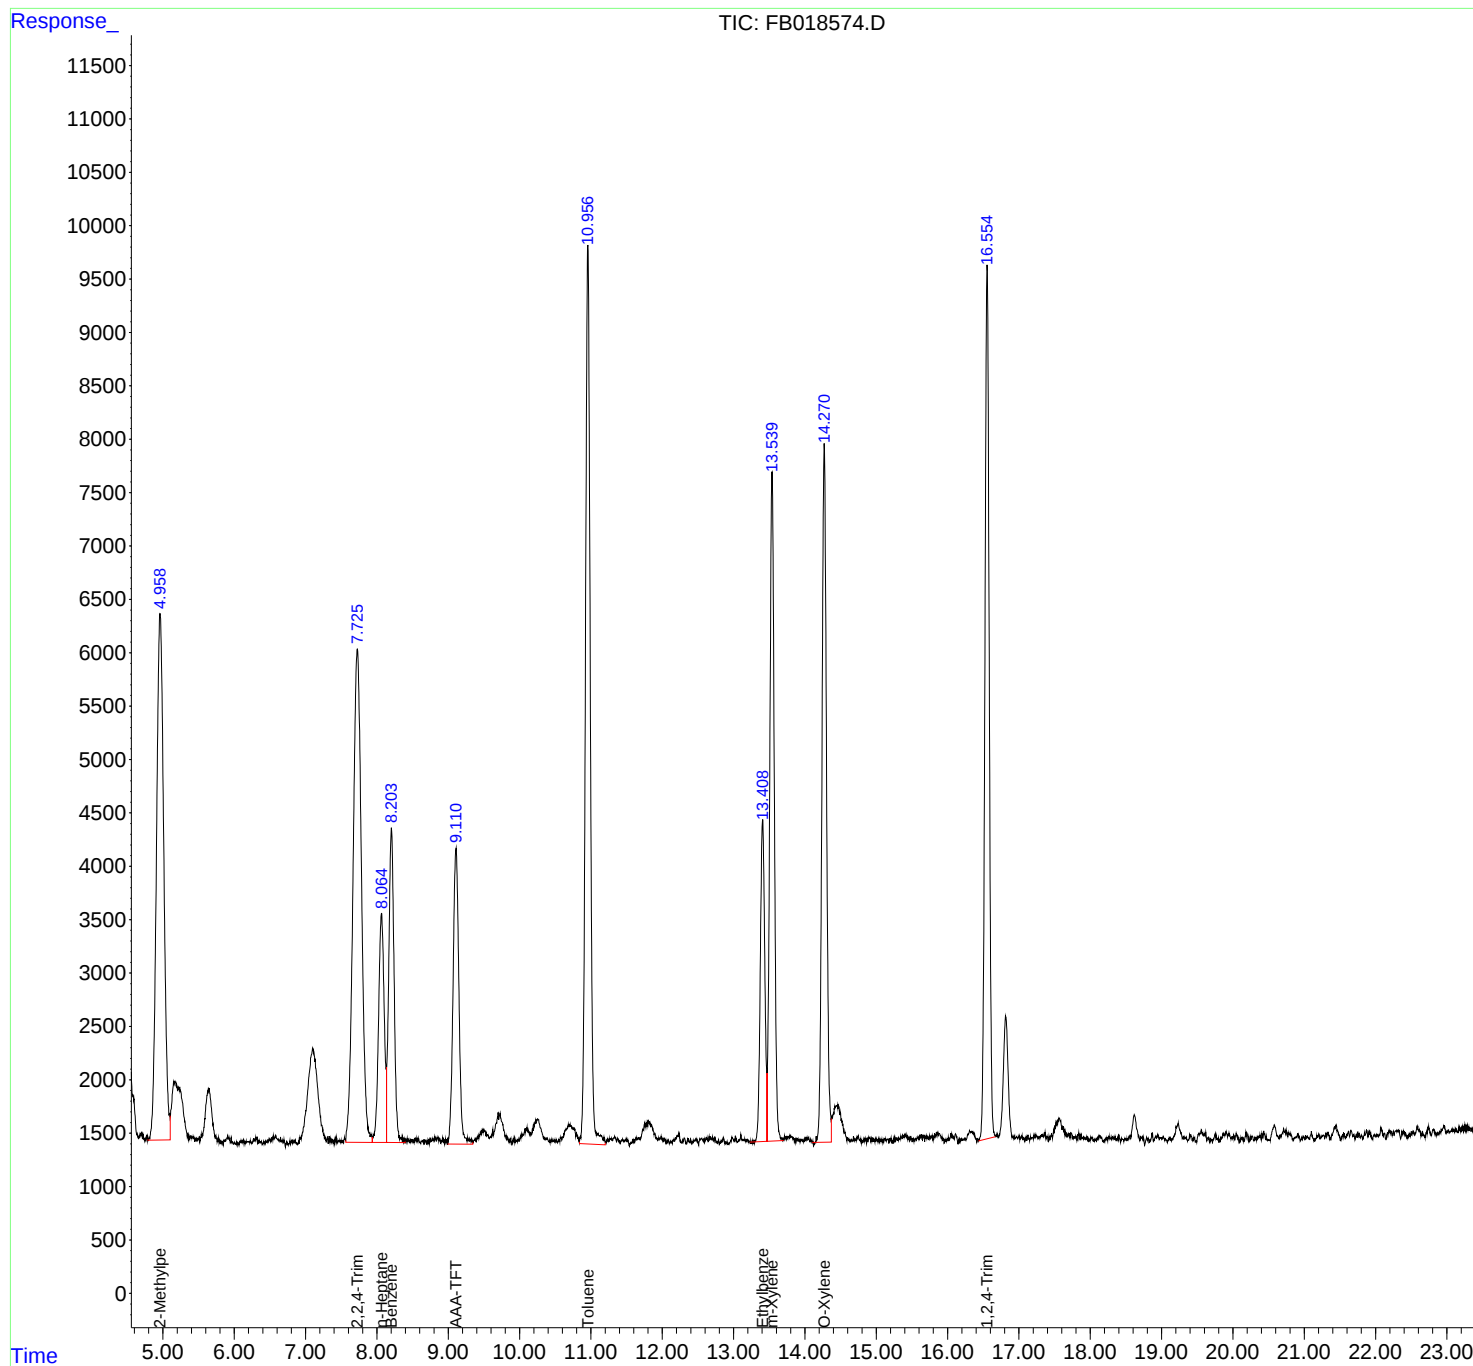

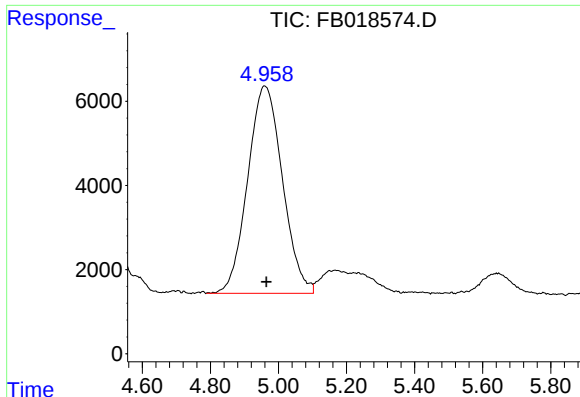


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 350105
Conc: 22.89 ng/ml

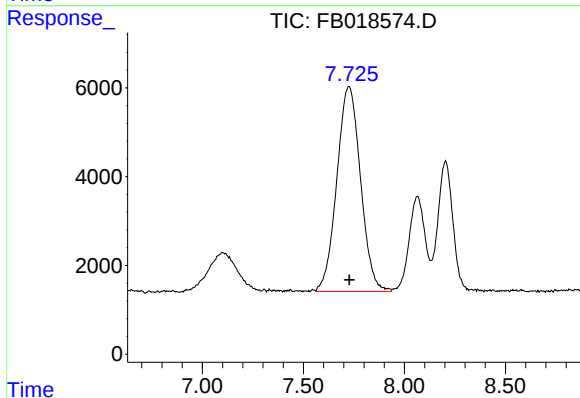


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.002 min
Response: 375965
Conc: 25.44 ng/ml

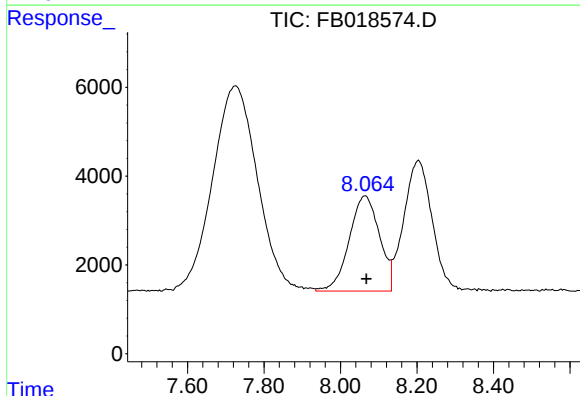


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 117714
Conc: 8.31 ng/ml

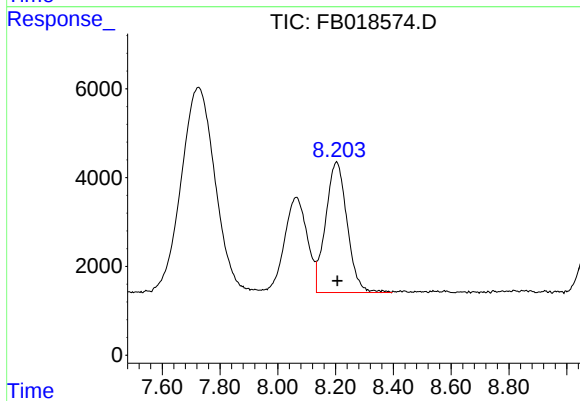


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 152274
Conc: 8.17 ng/ml

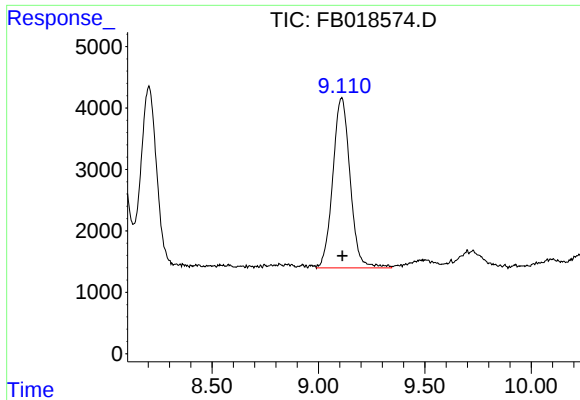


#5 AAA-TFT

R.T.: 9.109 min
 Delta R.T.: -0.003 min
 Response: 156605
 Conc: 18.18 ng/ml

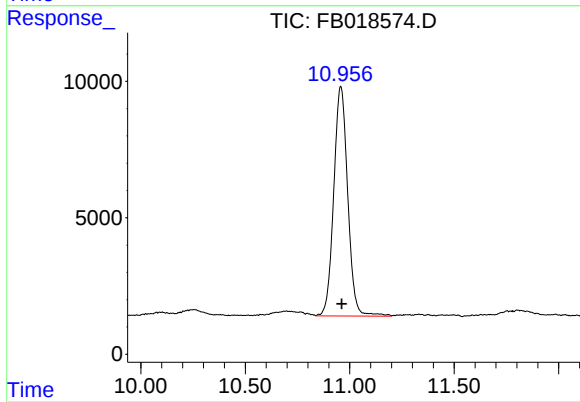


#6 Toluene

R.T.: 10.958 min
 Delta R.T.: -0.005 min
 Response: 392099
 Conc: 25.73 ng/ml

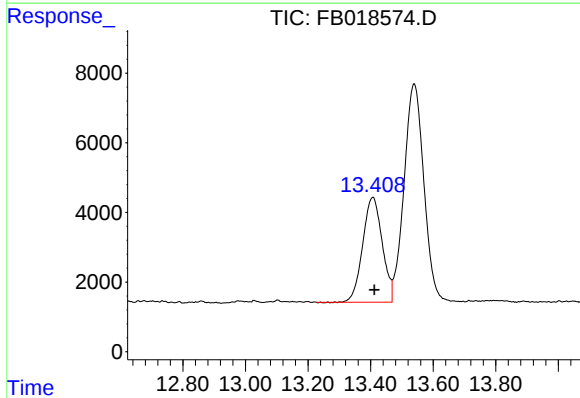


#7 Ethylbenzene

R.T.: 13.408 min
 Delta R.T.: -0.005 min
 Response: 130457
 Conc: 8.22 ng/ml

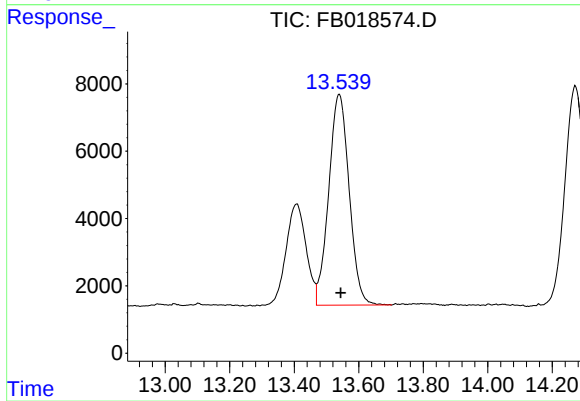


#8 m-Xylene

R.T.: 13.540 min
 Delta R.T.: -0.005 min
 Response: 276200
 Conc: 16.60 ng/ml

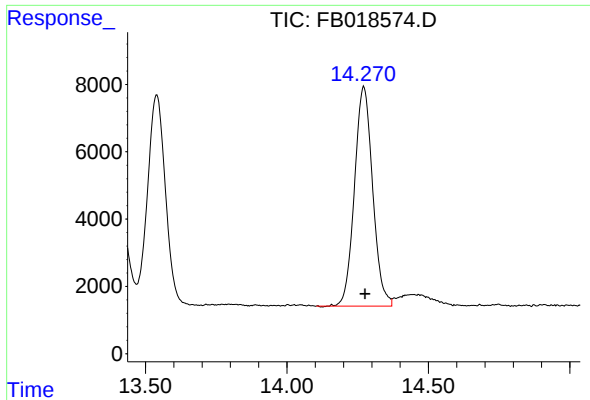

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.005 min
Response: 291060
Conc: 16.32 ng/ml

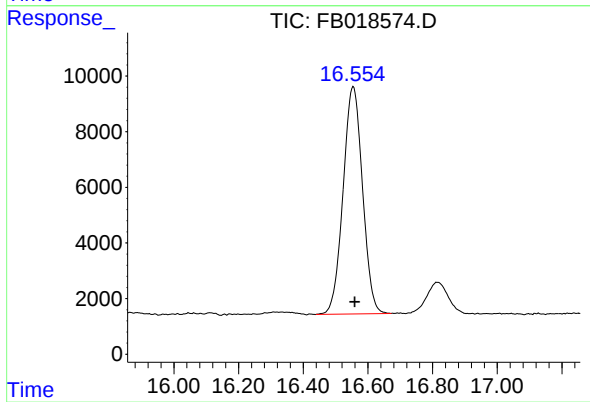

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.005 min
Response: 341063
Conc: 16.77 ng/ml