

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110718\
 Data File : FE029053.D
 Signal(s) : FID1B.CH
 Acq On : 07 Nov 2018 8:59
 Operator : DD\SJ
 Sample : J5827-02MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 15:54:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
 Quant Title :
 QLast Update : Wed Oct 24 08:22:18 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.892	3013813	17.938 ug/ml
Target Compounds			
1) N-OCTANE	2.516	1896089	16.370 ug/ml
3) N-DECANE	4.592	3061017	17.047 ug/ml
5) N-DODECANE	6.615	3286396	25.465 ug/ml
6) N-TETRADECANE	8.486	890736	6.722 ug/ml
8) N-OCTADECANE	11.472	3313745	22.552 ug/ml
10) N-TETRACOSANE	15.142	60379	0.423 ug/ml
11) N-OCTACOSANE	17.124	746247	5.484 ug/ml
12) N-DOTRIACONTANE	18.803	3315404	27.819 ug/ml
14) N-HEXATRIACONTANE	20.331	2628645	27.239 ug/ml
15) N-TETRACONTANE	22.102	2891685	33.501 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110718\
Data File : FE029053.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2018 8:59
Operator : DD\SJ
Sample : J5827-02MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 15:54:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

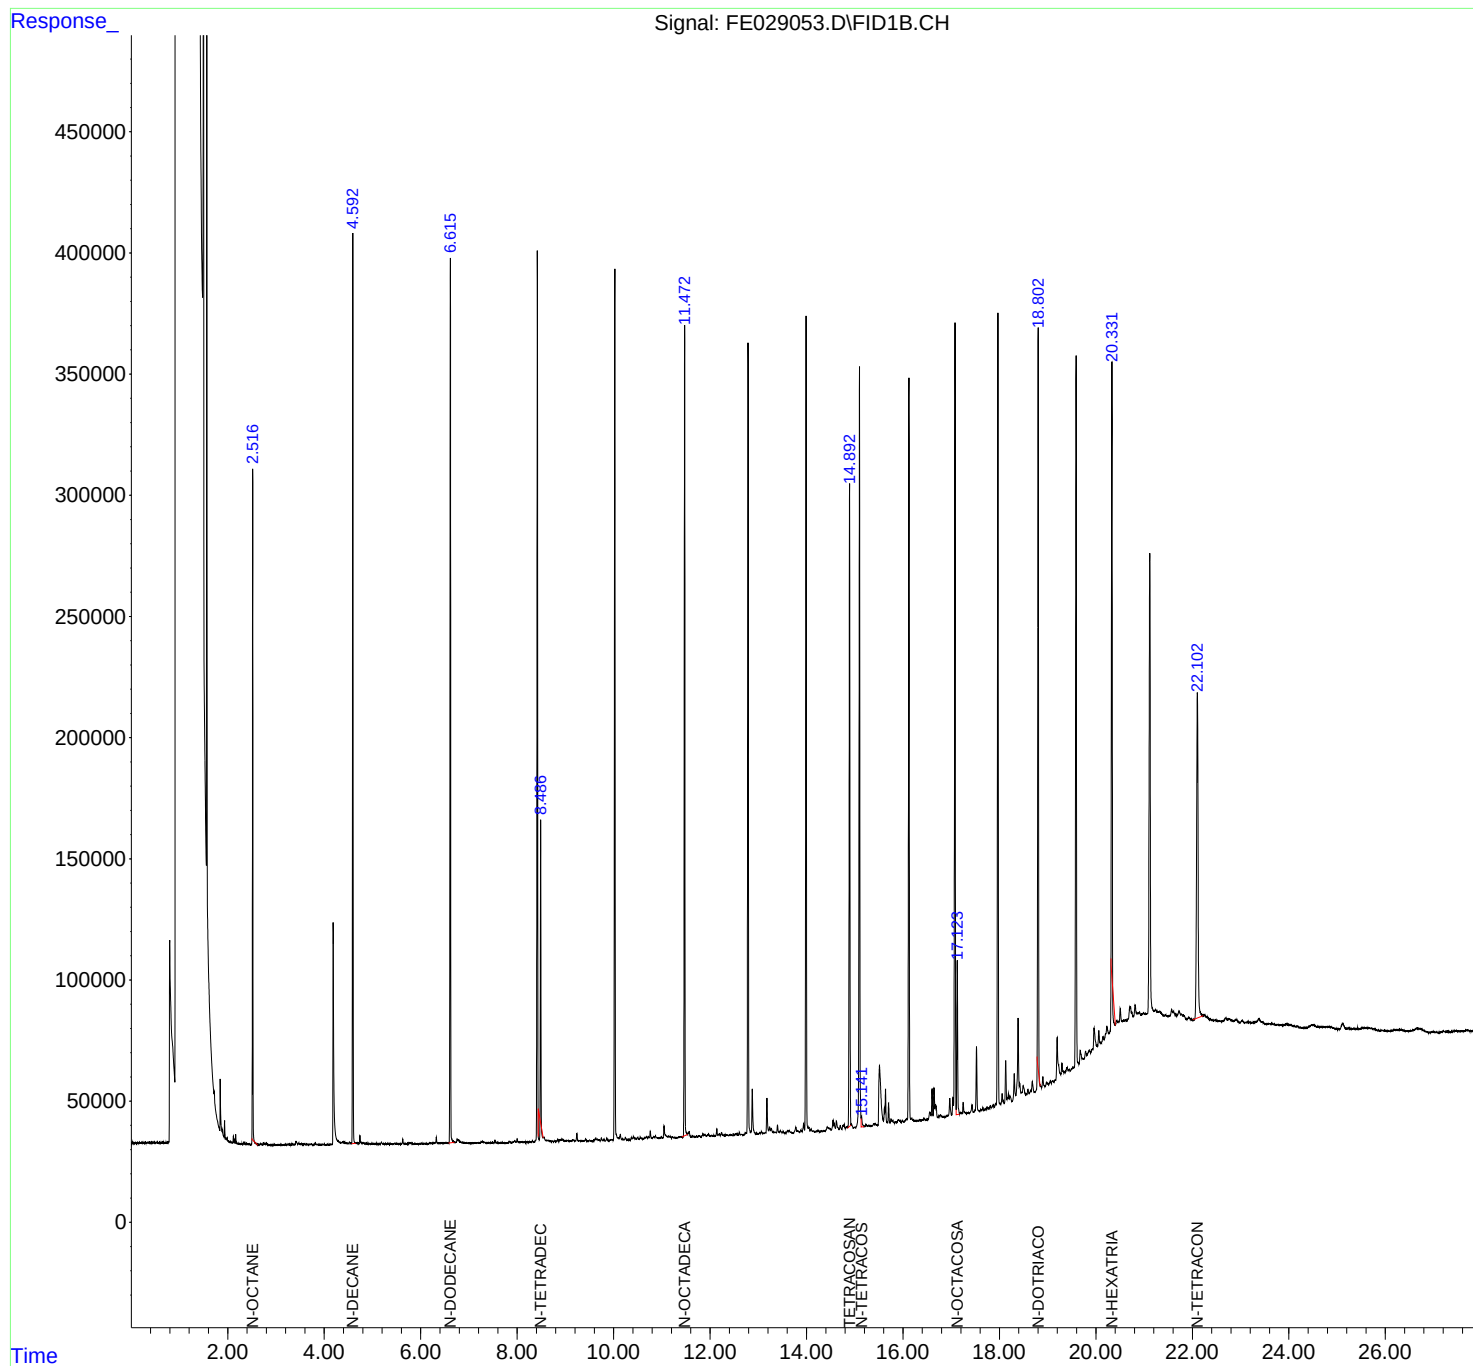

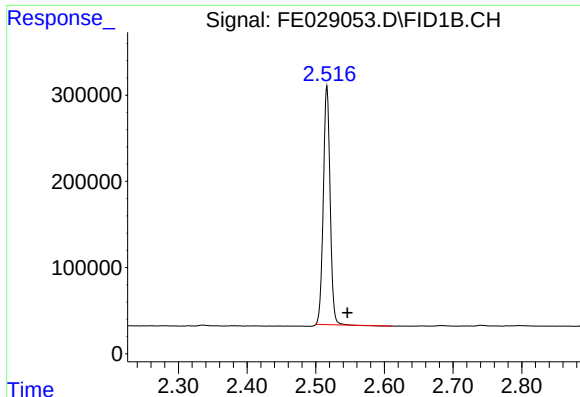


#1 N-OCTANE

R.T.: 2.516 min
Delta R.T.: -0.030 min
Response: 1896089
Conc: 16.37 ug/ml

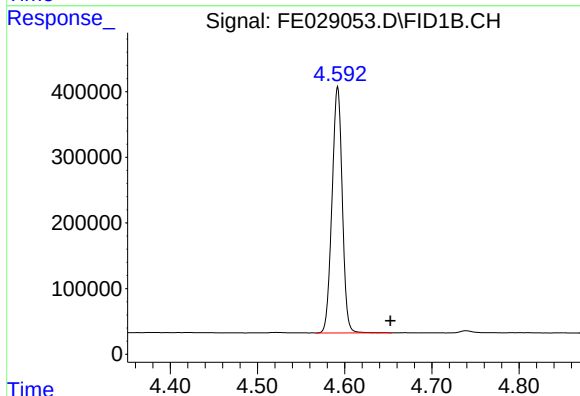


#3 N-DECANE

R.T.: 4.592 min
Delta R.T.: -0.060 min
Response: 3061017
Conc: 17.05 ug/ml

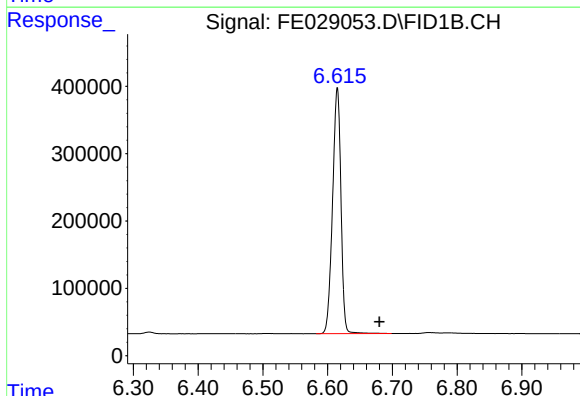


#5 N-DODECANE

R.T.: 6.615 min
Delta R.T.: -0.065 min
Response: 3286396
Conc: 25.46 ug/ml

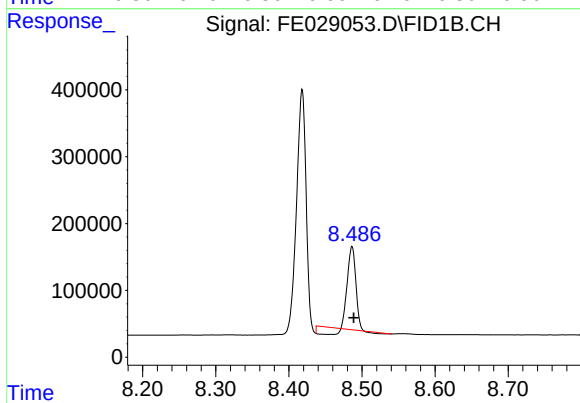


#6 N-TETRADECANE

R.T.: 8.486 min
Delta R.T.: -0.002 min
Response: 890736
Conc: 6.72 ug/ml

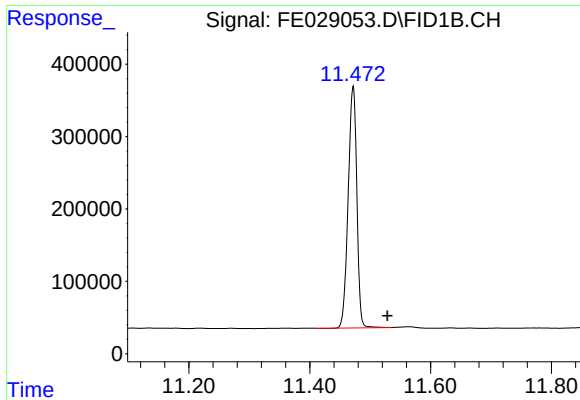


#8 N-OCTADECANE

R.T.: 11.472 min
Delta R.T.: -0.056 min
Response: 3313745
Conc: 22.55 ug/ml

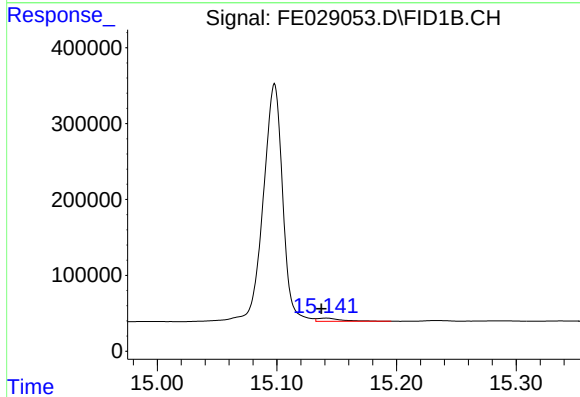


#10 N-TETRACOSANE

R.T.: 15.142 min
Delta R.T.: 0.004 min
Response: 60379
Conc: 0.42 ug/ml

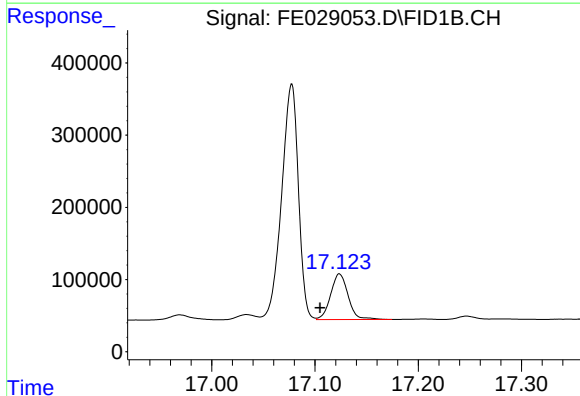


#11 N-OCTACOSANE

R.T.: 17.124 min
Delta R.T.: 0.019 min
Response: 746247
Conc: 5.48 ug/ml

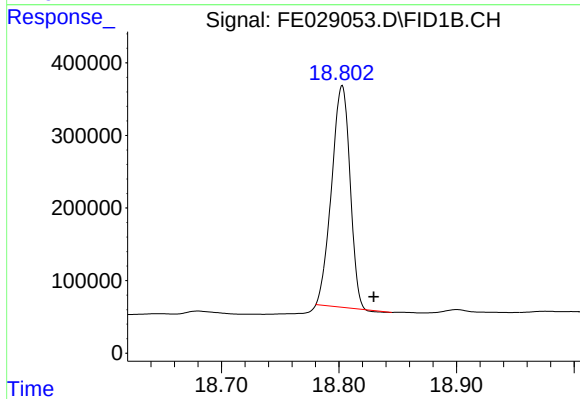


#12 N-DOTRIACONTANE

R.T.: 18.803 min
Delta R.T.: -0.027 min
Response: 3315404
Conc: 27.82 ug/ml

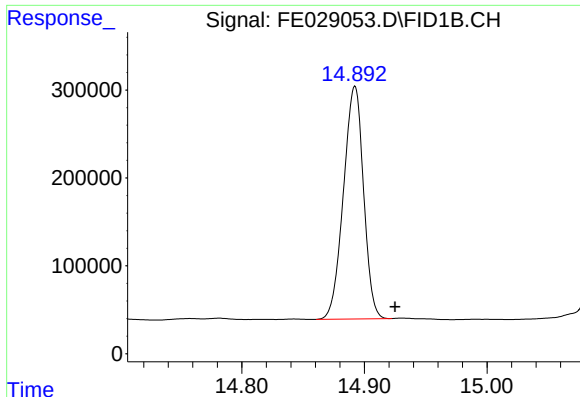


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.892 min
Delta R.T.: -0.033 min
Response: 3013813
Conc: 17.94 ug/ml

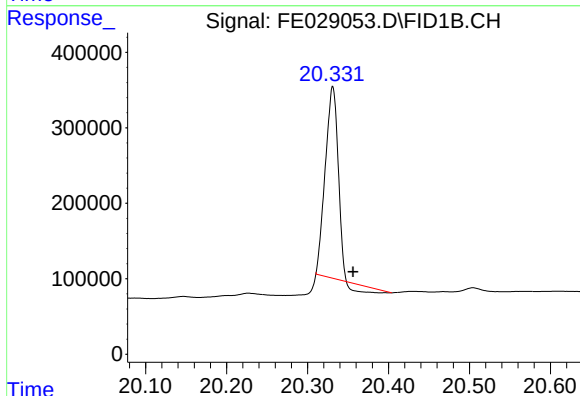

#14 N-HEXATRIACONTANE

R.T.: 20.331 min
Delta R.T.: -0.025 min
Response: 2628645
Conc: 27.24 ug/ml

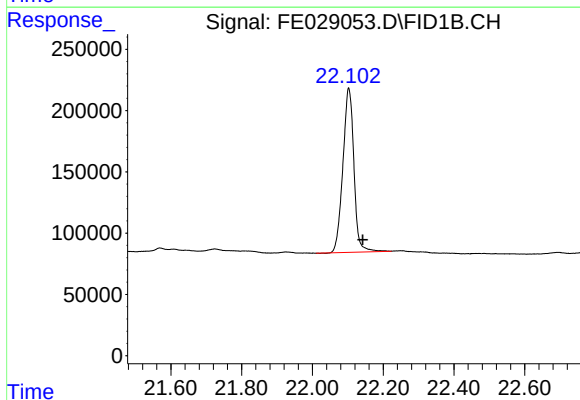

#15 N-TETRACONTANE

R.T.: 22.102 min
Delta R.T.: -0.040 min
Response: 2891685
Conc: 33.50 ug/ml