

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
 Data File : FB022899.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2019 10:08
 Operator : DD/AJ
 Sample : BSF1106S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 06 14:18:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	416330	18.494 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	951012	29.564 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1076204	30.487 ng/ml
3) t n-Heptane	7.754	350703	10.082 ng/ml
4) t Benzene	7.888	422264	9.749 ng/ml
6) t Toluene	10.626	1233461	28.612 ng/ml
7) t Ethylbenzene	13.066	389221	9.749 ng/ml
8) t m-Xylene	13.199	735337	19.470 ng/ml
9) t O-Xylene	13.926	692397	19.427 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	572459	20.186 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
Data File : FB022899.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2019 10:08
Operator : DD/AJ
Sample : BSF1106S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 06 14:18:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

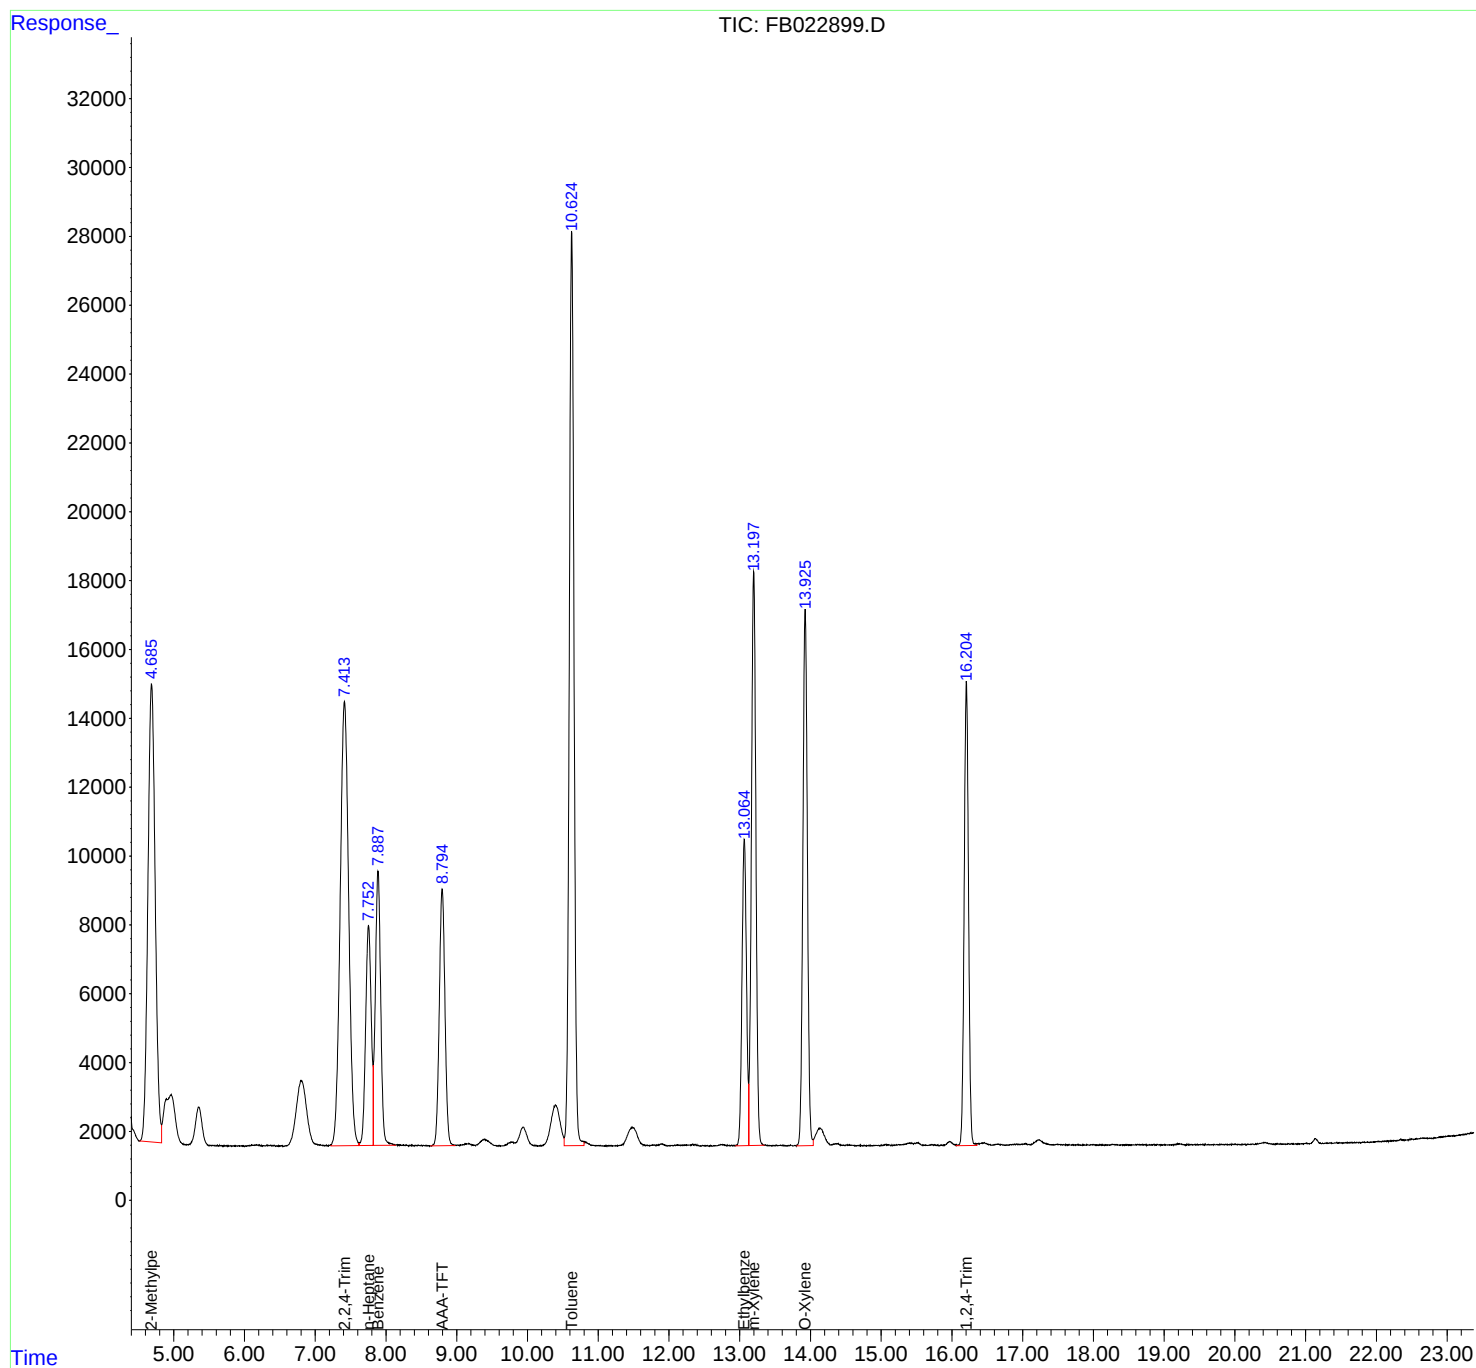

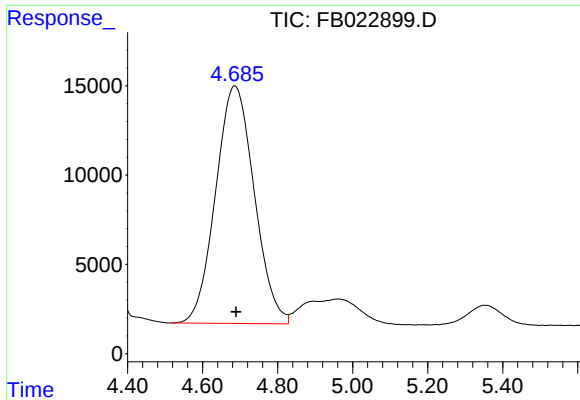


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 951012
Conc: 29.56 ng/ml

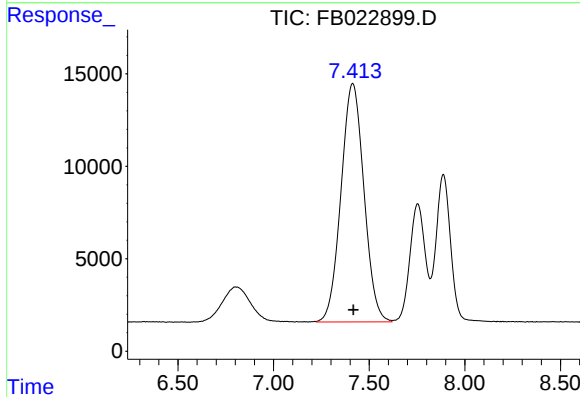


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1076204
Conc: 30.49 ng/ml

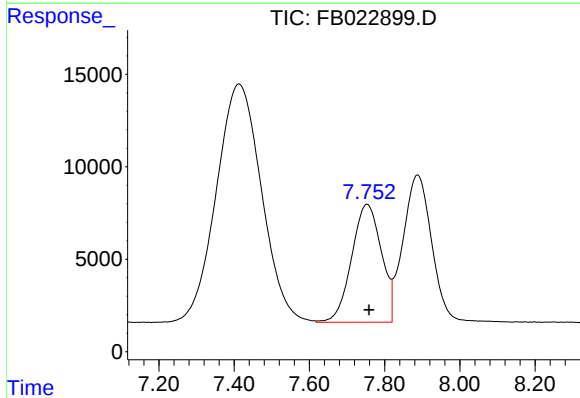


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 350703
Conc: 10.08 ng/ml

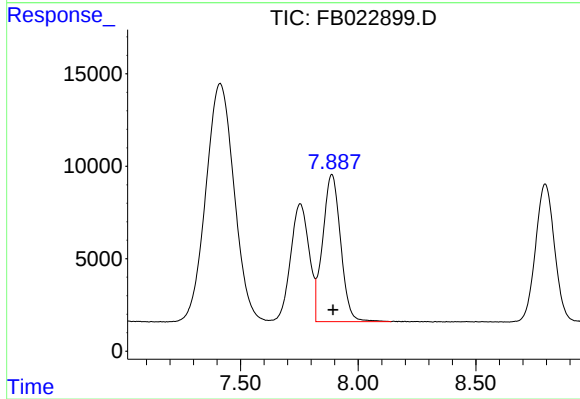


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 422264
Conc: 9.75 ng/ml

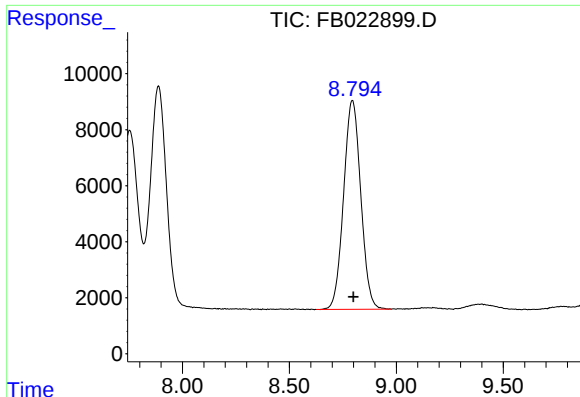


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 416330
Conc: 18.49 ng/ml

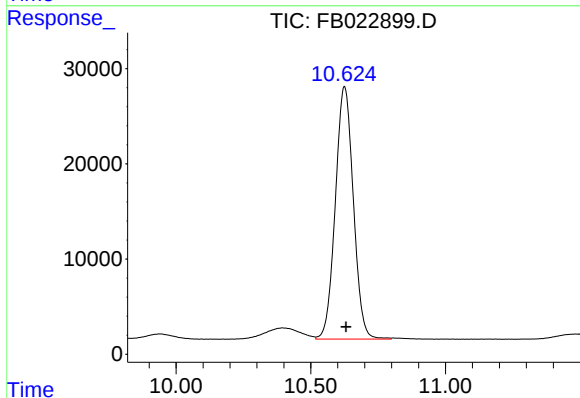


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 1233461
Conc: 28.61 ng/ml

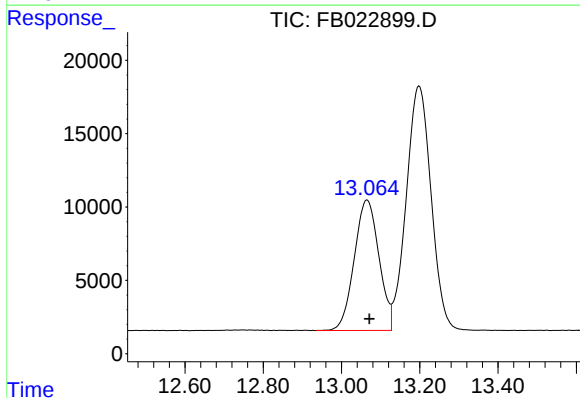


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.006 min
Response: 389221
Conc: 9.75 ng/ml

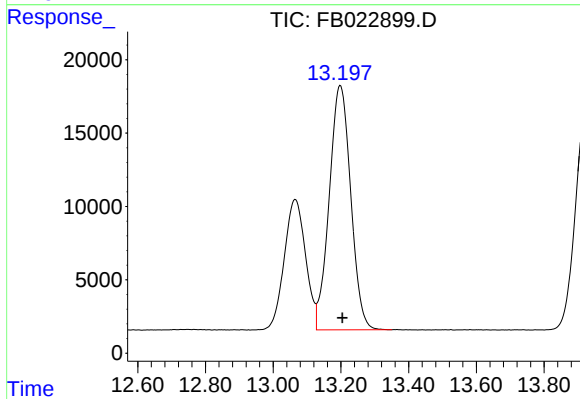


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 735337
Conc: 19.47 ng/ml

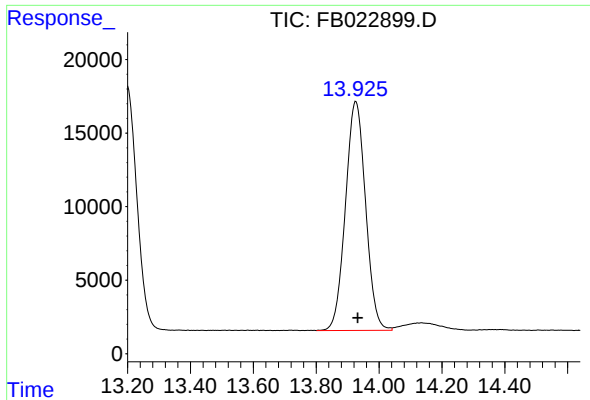

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.006 min
Response: 692397
Conc: 19.43 ng/ml

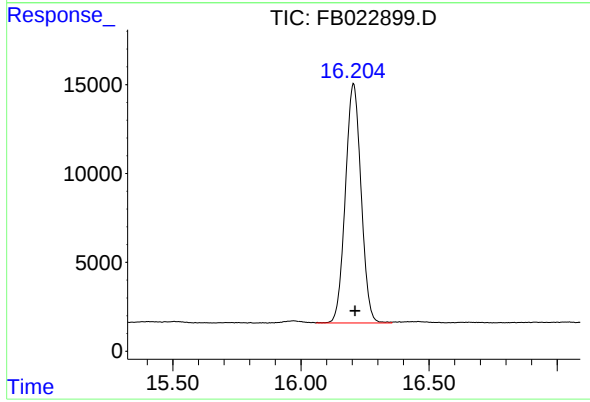

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 572459
Conc: 20.19 ng/ml