

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
 Data File : FB022902.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2019 12:20
 Operator : DD/AJ
 Sample : K5609-15 100X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 06 14:18:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.840	1317075	58.506 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.680	1331534	41.394 ng/ml
2) t 2,2,4-Trimethylpentane	7.373	1818368	51.511 ng/ml
3) t n-Heptane	7.751	3320358	95.453 ng/ml
4) t Benzene	7.885	1152381	26.605 ng/ml
6) t Toluene	10.626	12468375	289.219 ng/ml
7) t Ethylbenzene	13.066	3187108	79.833 ng/ml
8) t m-Xylene	13.197	12267208	324.811 ng/ml
9) t O-Xylene	13.927	4417947	123.958 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	3914302	138.028 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
Data File : FB022902.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2019 12:20
Operator : DD/AJ
Sample : K5609-15 100X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 06 14:18:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

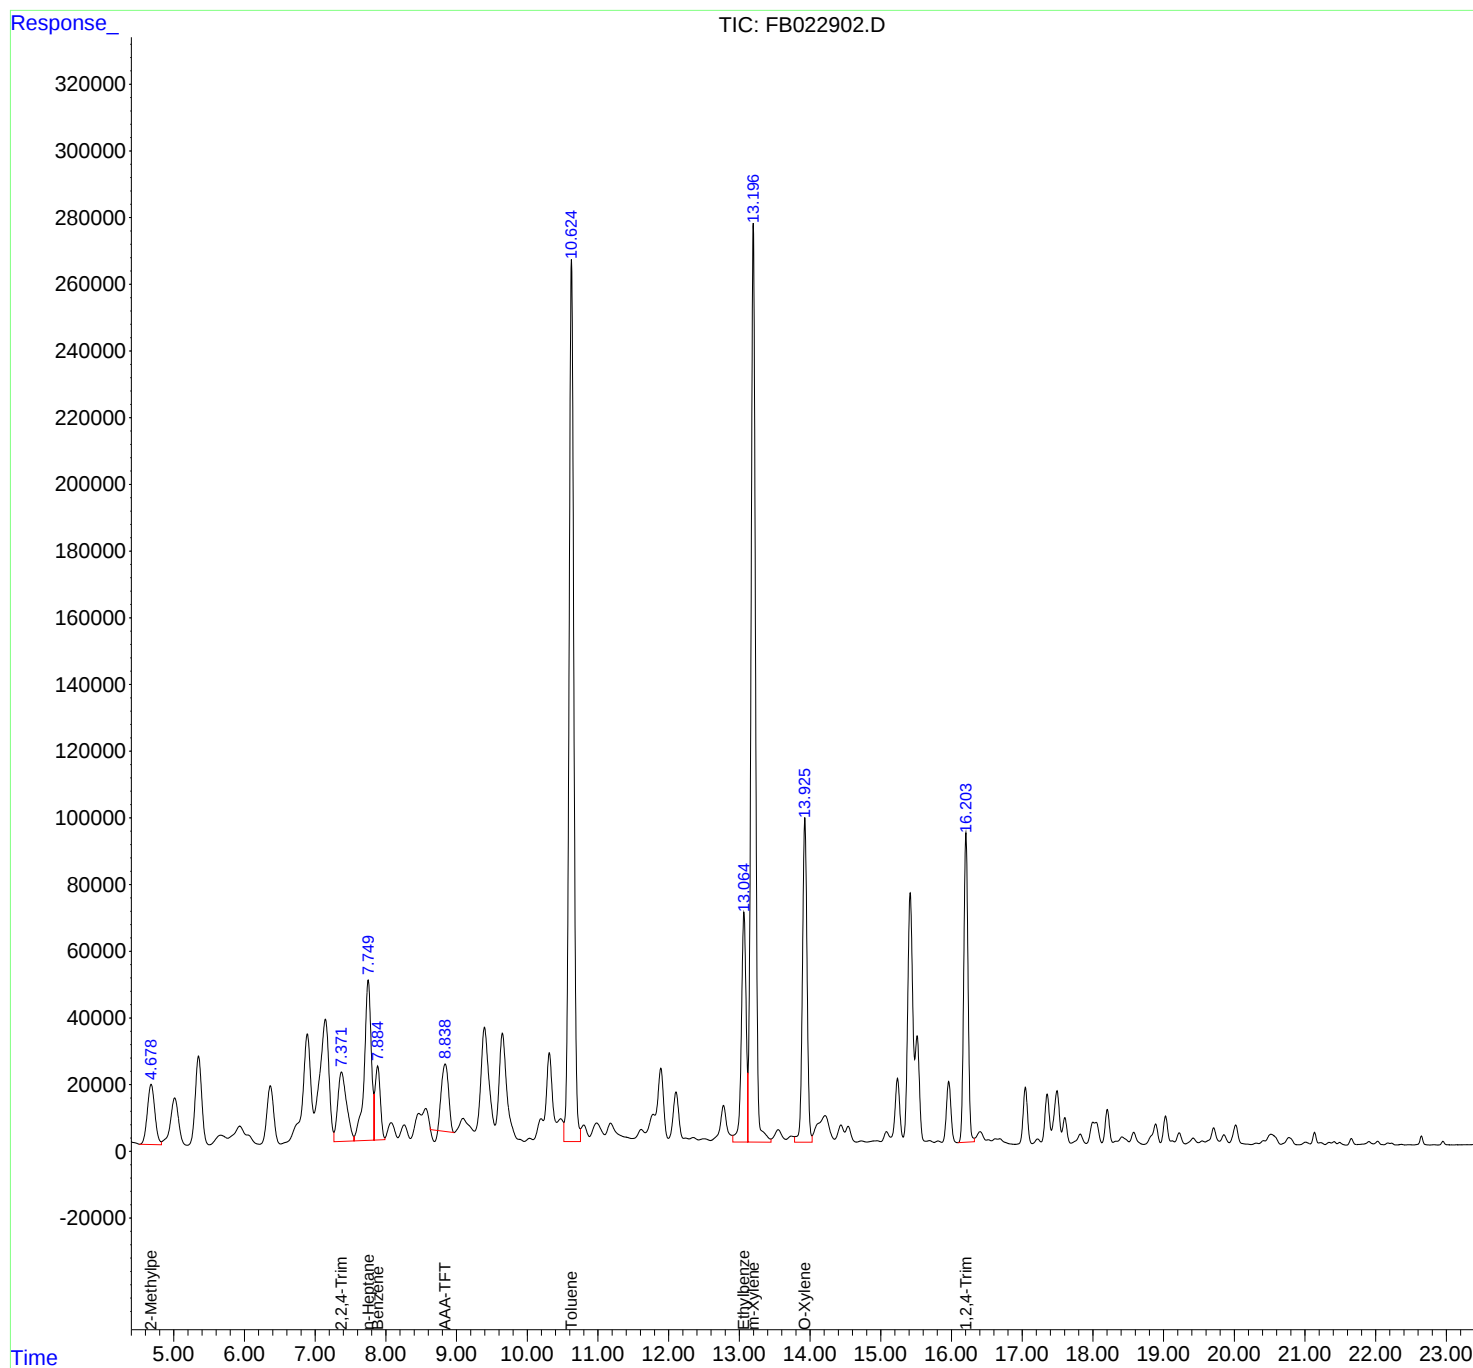

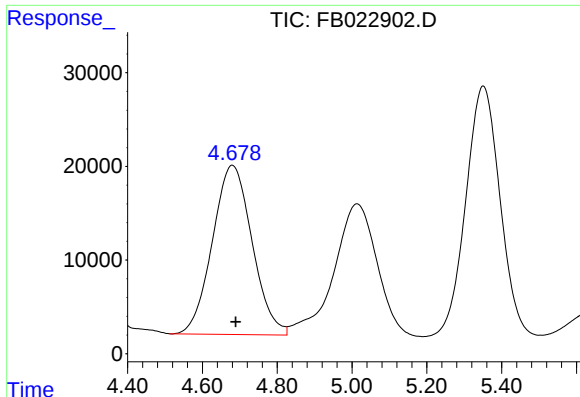


#1 2-Methylpentane

R.T.: 4.680 min
Delta R.T.: -0.009 min
Response: 1331534
Conc: 41.39 ng/ml

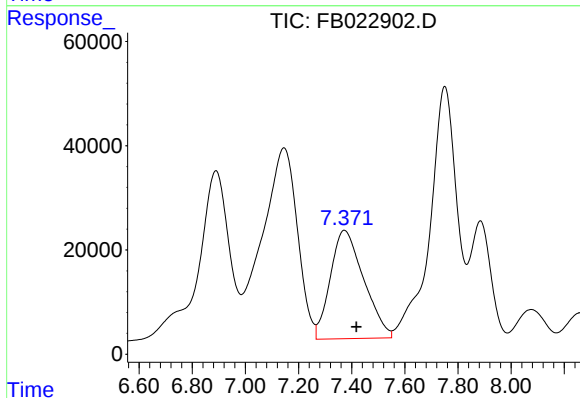


#2 2,2,4-Trimethylpentane

R.T.: 7.373 min
Delta R.T.: -0.045 min
Response: 1818368
Conc: 51.51 ng/ml

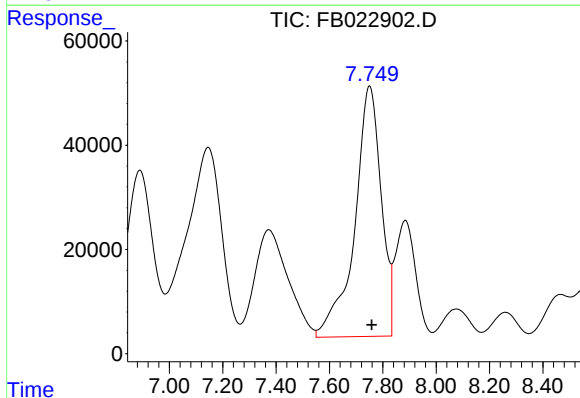


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 3320358
Conc: 95.45 ng/ml

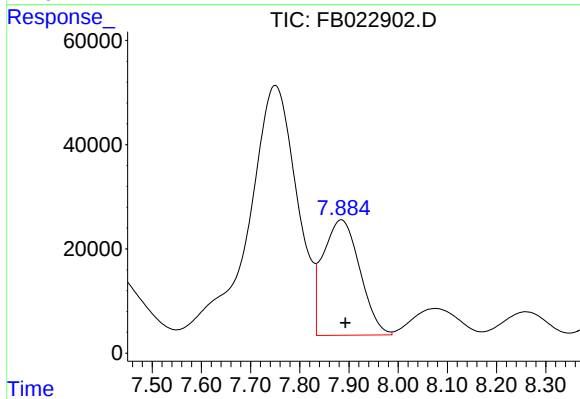


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 1152381
Conc: 26.61 ng/ml

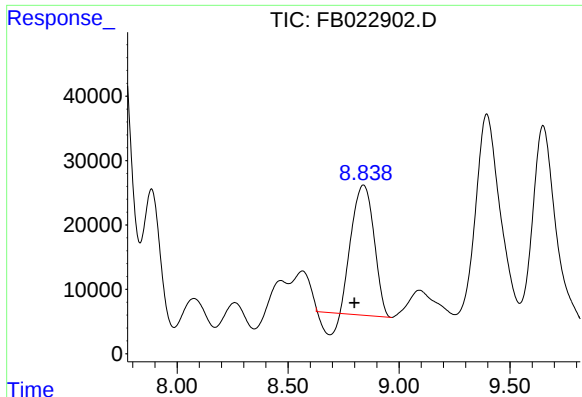


#5 AAA-TFT

R.T.: 8.840 min
Delta R.T.: 0.040 min
Response: 1317075
Conc: 58.51 ng/ml

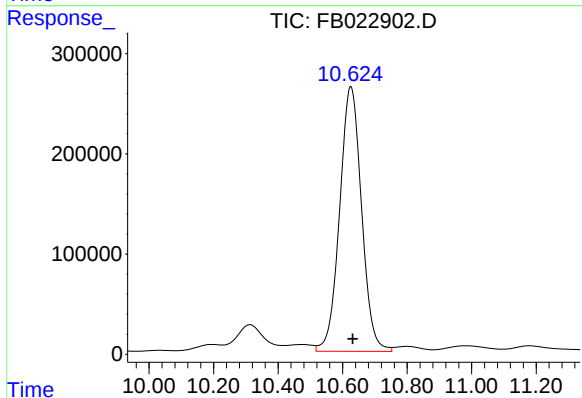


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 12468375
Conc: 289.22 ng/ml

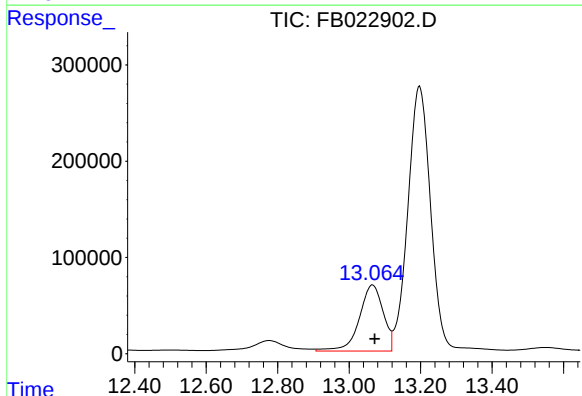


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.006 min
Response: 3187108
Conc: 79.83 ng/ml

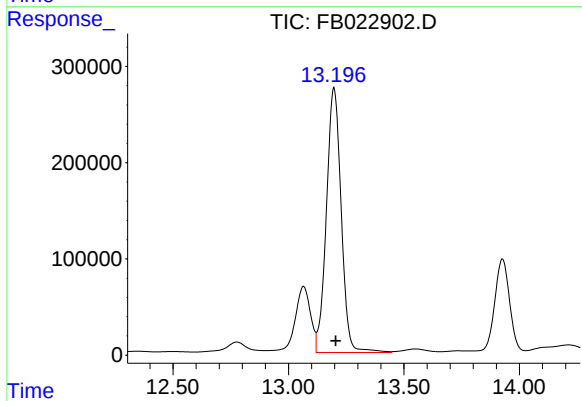


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.007 min
Response: 12267208
Conc: 324.81 ng/ml

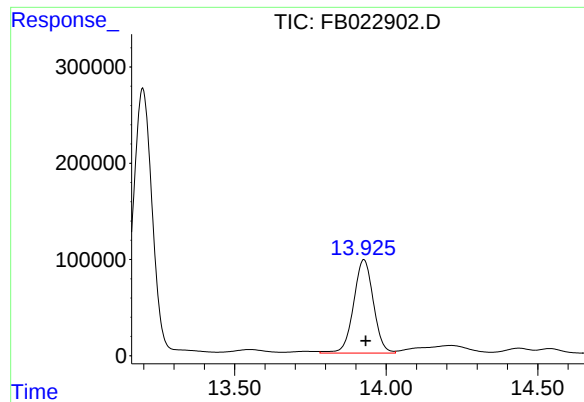

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 4417947
Conc: 123.96 ng/ml

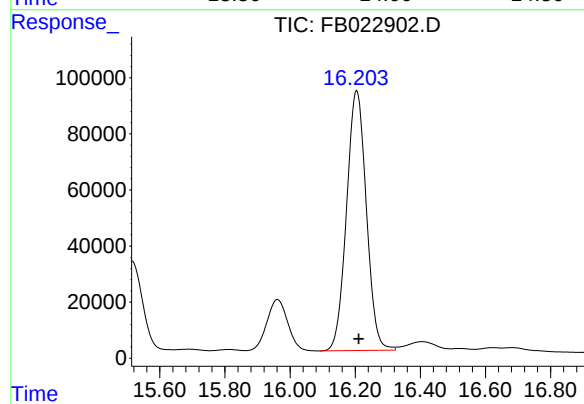

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 3914302
Conc: 138.03 ng/ml