

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
 Data File : FB022904.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2019 14:19
 Operator : DD/AJ
 Sample : K5609-15 300X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 06 14:18:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.809	659641	29.302 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.682	360969	11.222 ng/ml
2) t 2,2,4-Trimethylpentane	7.375	536495	15.198 ng/ml
3) t n-Heptane	7.752	993613	28.564 ng/ml
4) t Benzene	7.886	340344	7.858 ng/ml
6) t Toluene	10.626	3710372	86.067 ng/ml
7) t Ethylbenzene	13.065	911024	22.820 ng/ml
8) t m-Xylene	13.197	3375102	89.366 ng/ml
9) t O-Xylene	13.927	1233605	34.612 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	1193413	42.083 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110619\
Data File : FB022904.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2019 14:19
Operator : DD/AJ
Sample : K5609-15 300X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 06 14:18:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

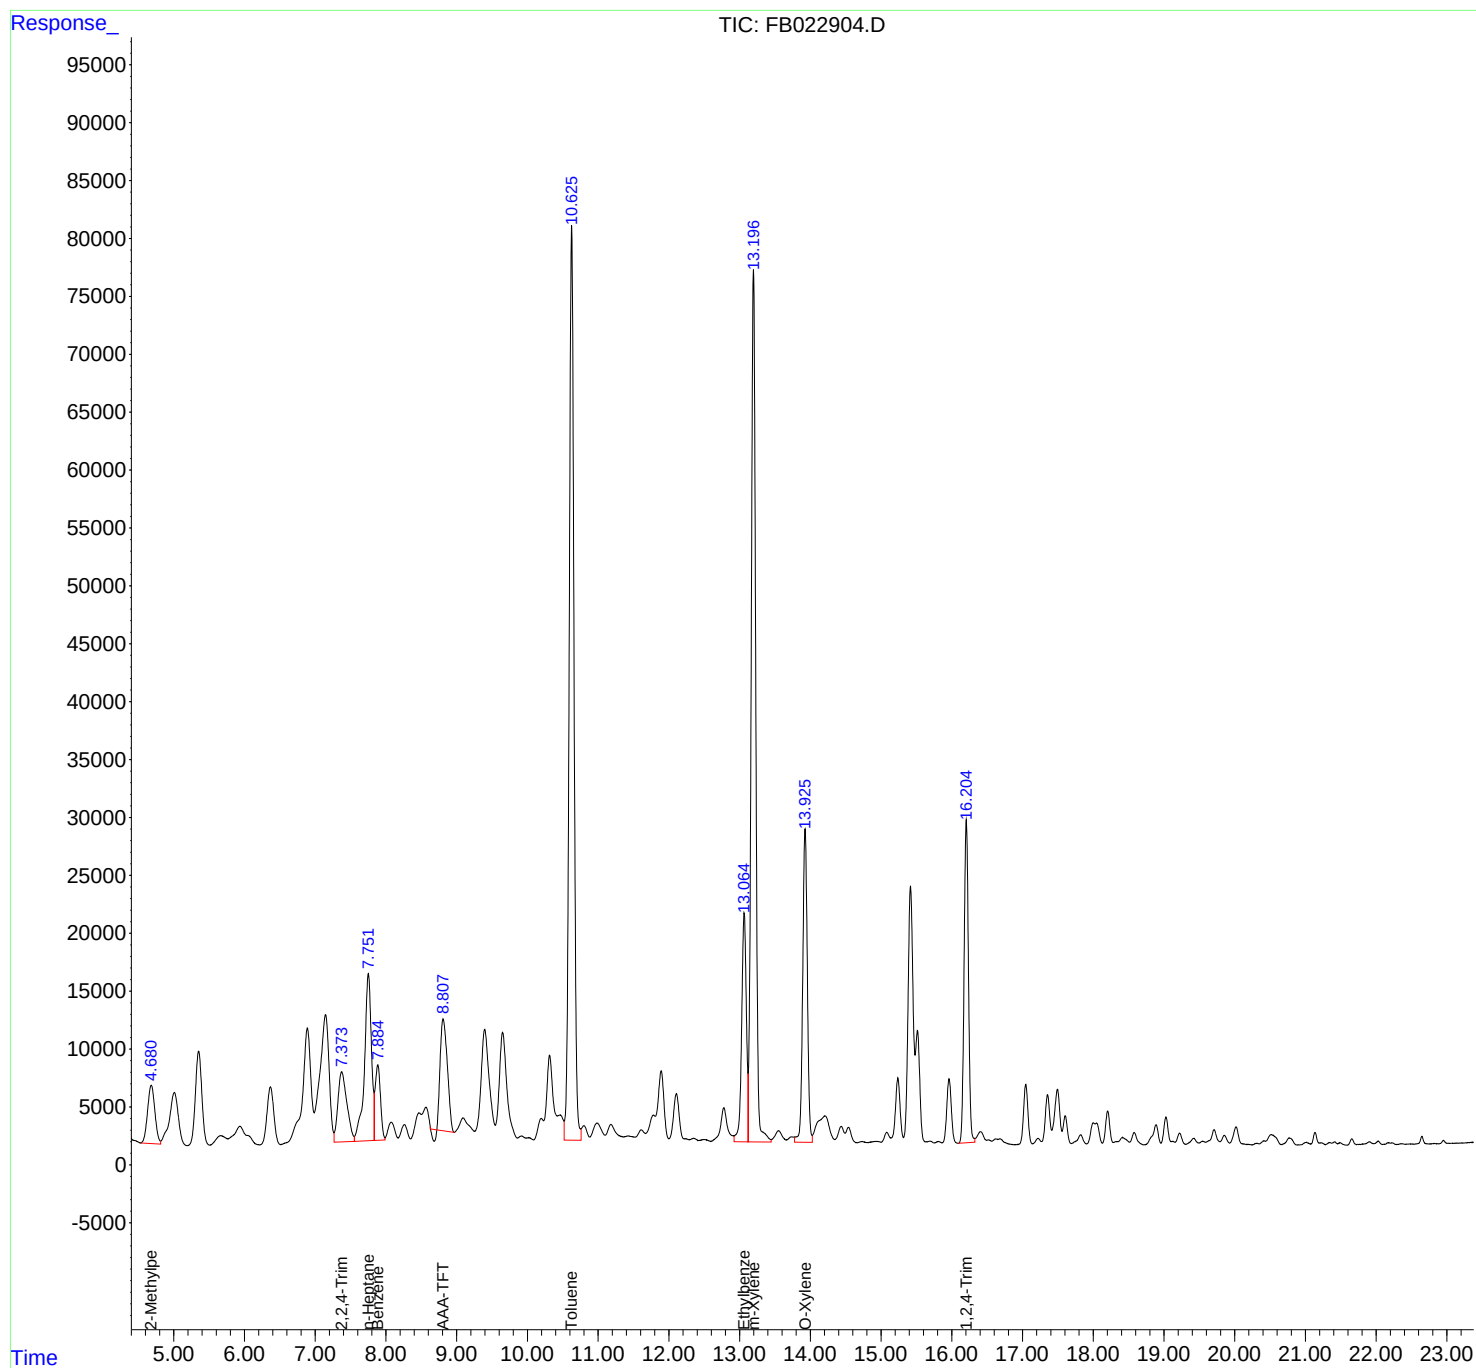

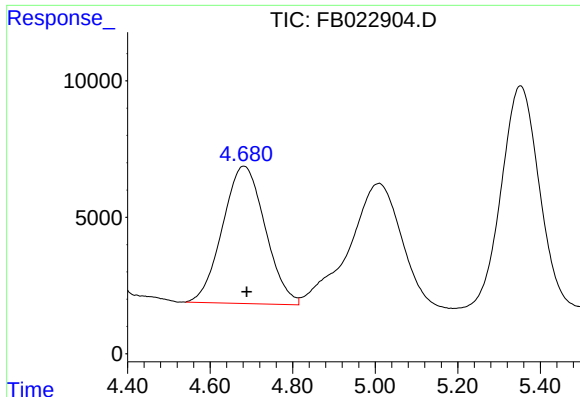


#1 2-Methylpentane

R.T.: 4.682 min
Delta R.T.: -0.007 min
Response: 360969
Conc: 11.22 ng/ml

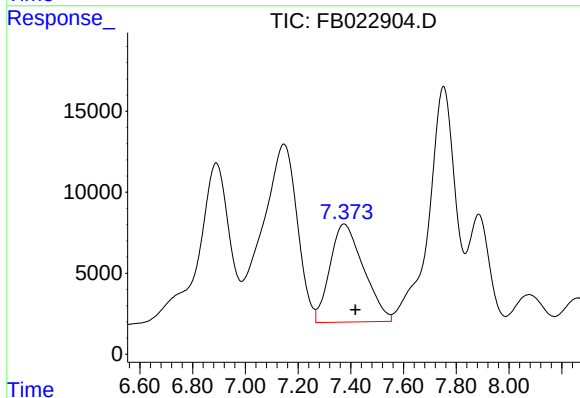


#2 2,2,4-Trimethylpentane

R.T.: 7.375 min
Delta R.T.: -0.043 min
Response: 536495
Conc: 15.20 ng/ml

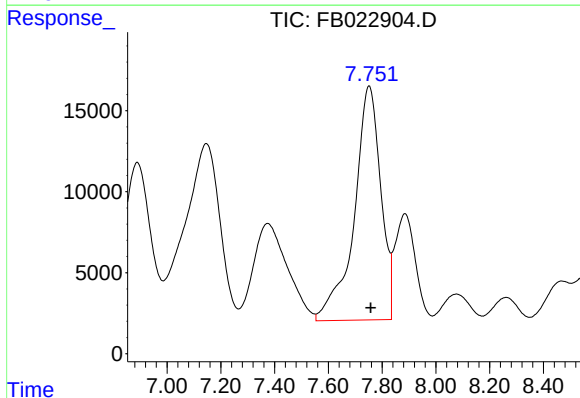


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 993613
Conc: 28.56 ng/ml

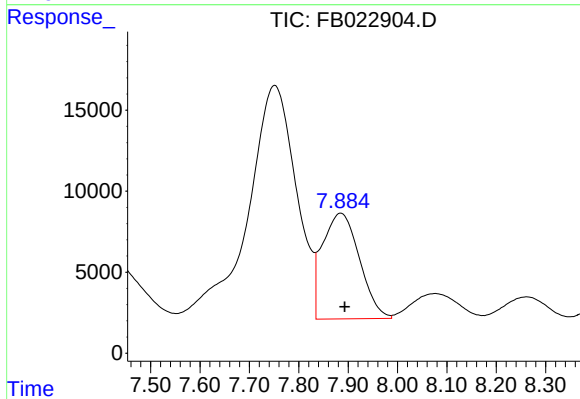


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 340344
Conc: 7.86 ng/ml

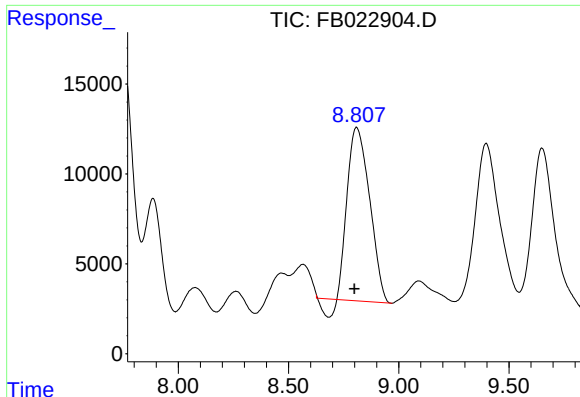


#5 AAA-TFT

R.T.: 8.809 min
Delta R.T.: 0.009 min
Response: 659641
Conc: 29.30 ng/ml

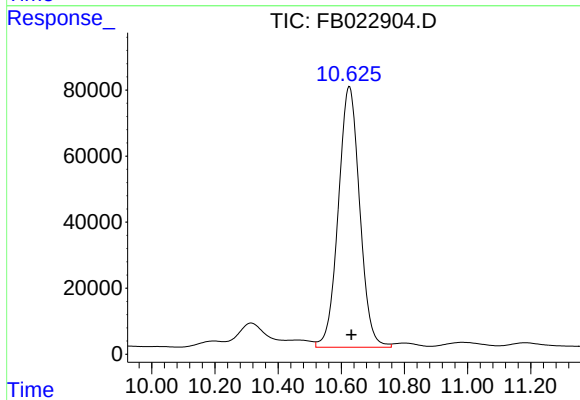


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 3710372
Conc: 86.07 ng/ml

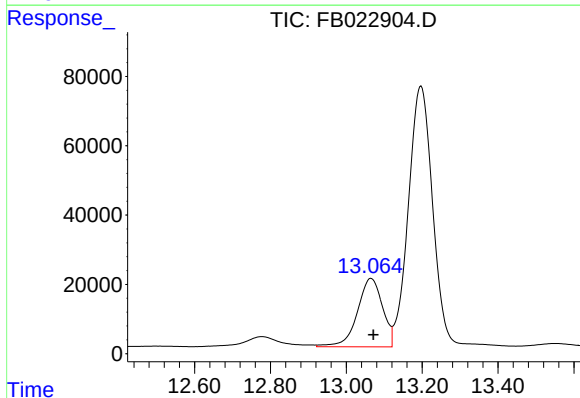


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.006 min
Response: 911024
Conc: 22.82 ng/ml

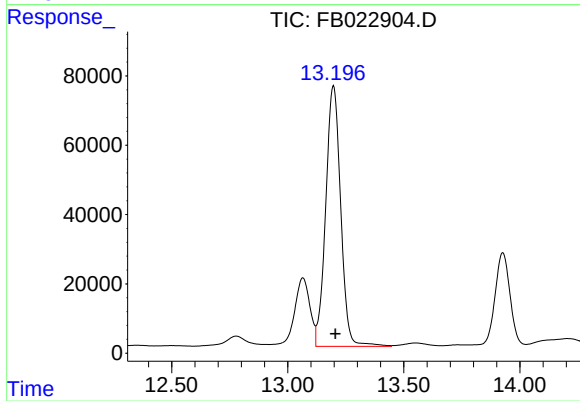


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.008 min
Response: 3375102
Conc: 89.37 ng/ml

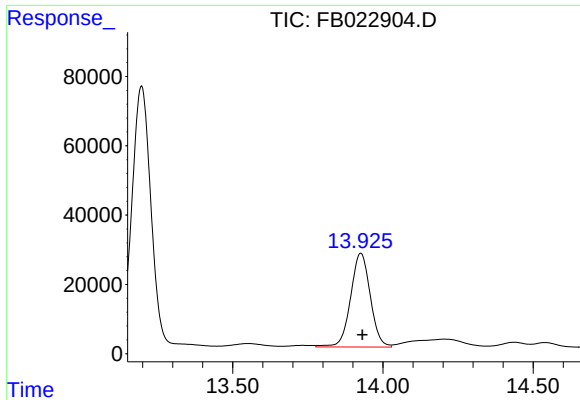

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 1233605
Conc: 34.61 ng/ml

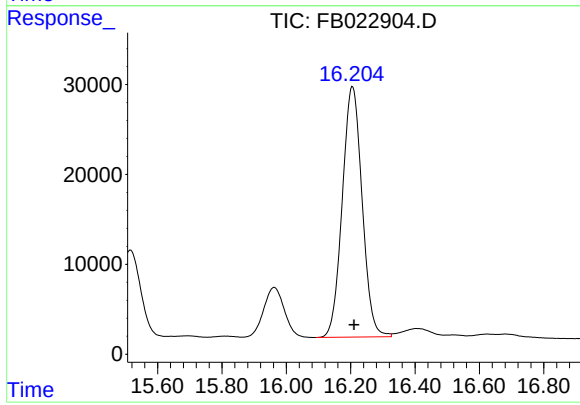

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 1193413
Conc: 42.08 ng/ml