

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110620\
 Data File : FB025199.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2020 8:16
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 06 23:14:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	440199	19.496 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	939319	29.101 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	955590	28.802 ng/ml
3) t n-Heptane	7.754	315206	9.597 ng/ml
4) t Benzene	7.890	386653	9.725 ng/ml
6) t Toluene	10.628	1115271	29.827 ng/ml
7) t Ethylbenzene	13.068	333327	9.707 ng/ml
8) t m-Xylene	13.201	667534	19.770 ng/ml
9) t O-Xylene	13.928	647274	19.796 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	538501	19.571 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110620\
Data File : FB025199.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2020 8:16
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 06 23:14:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

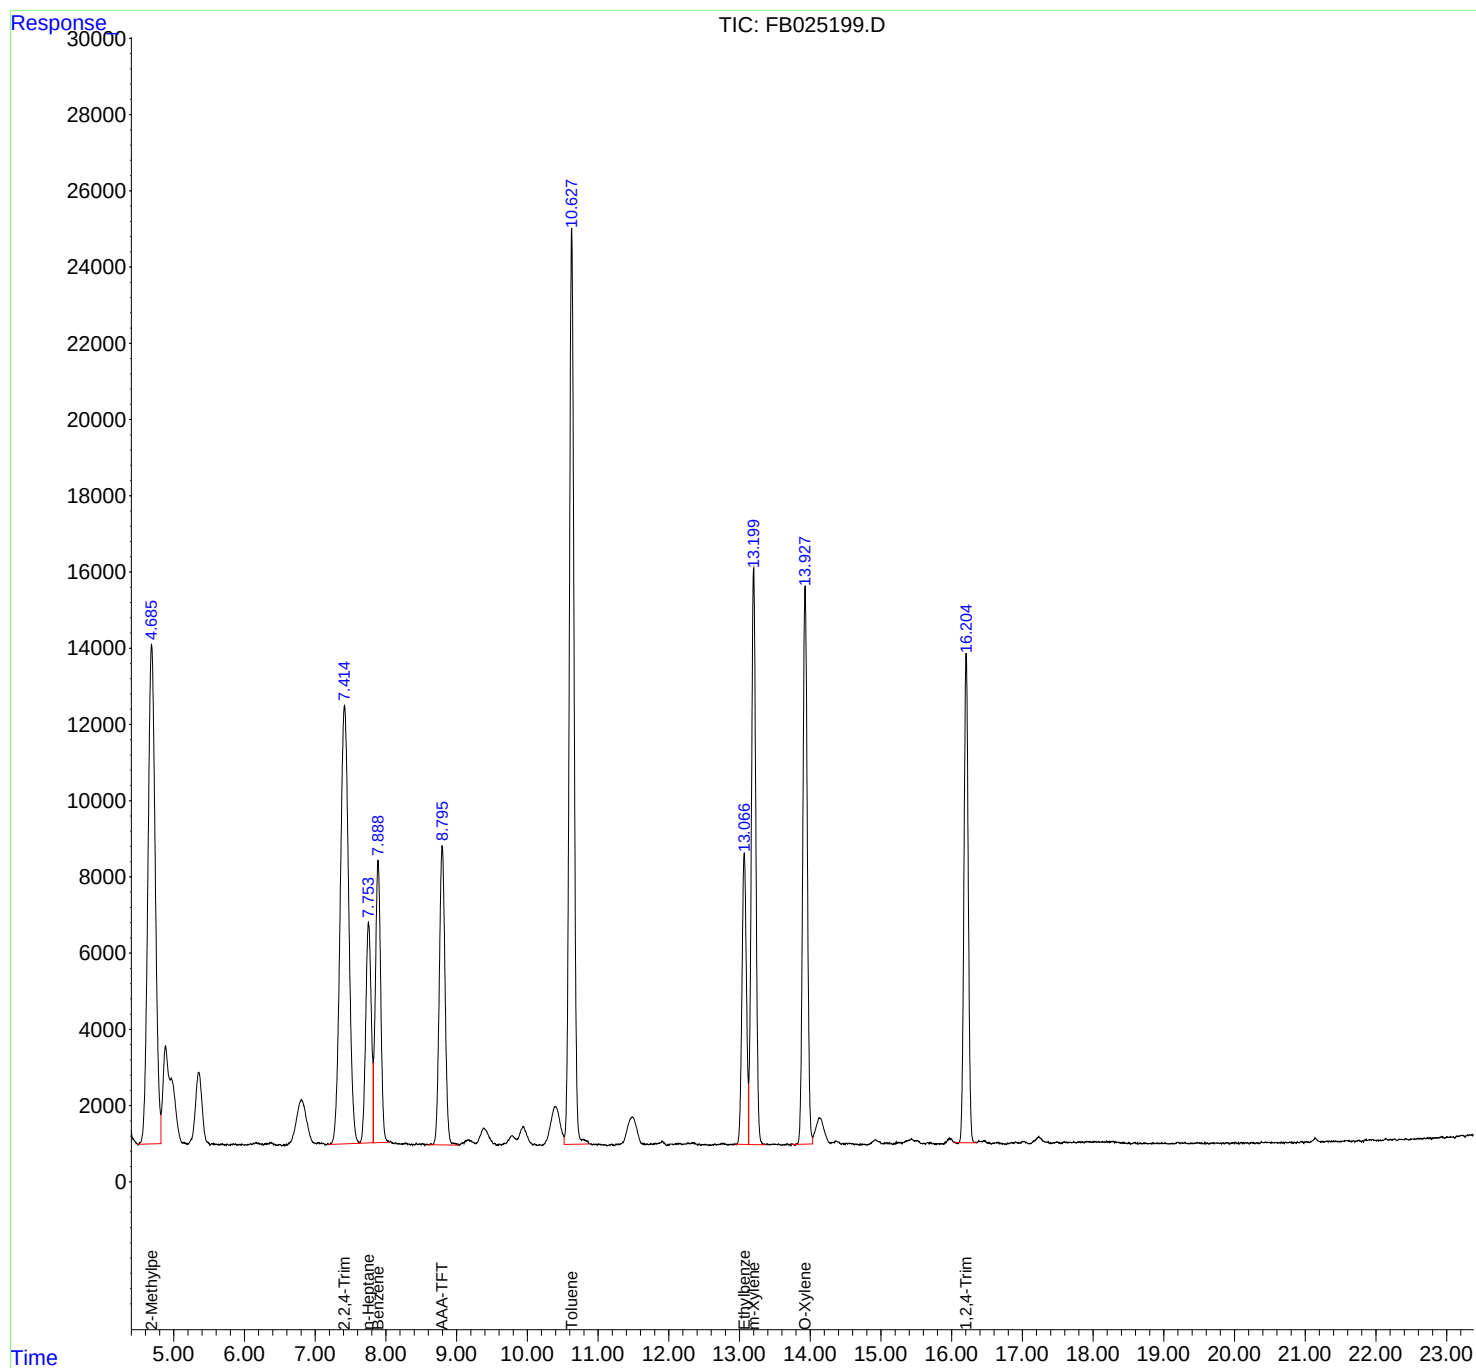

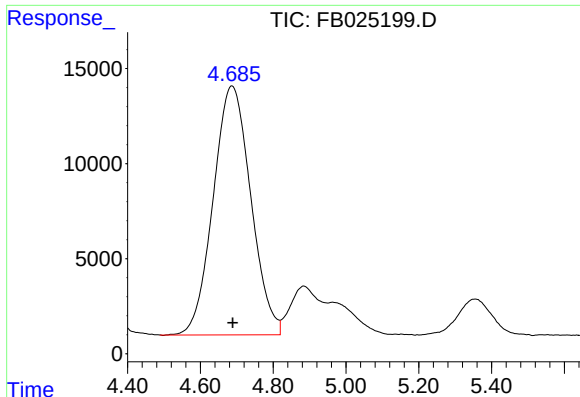


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 939319
Conc: 29.10 ng/ml

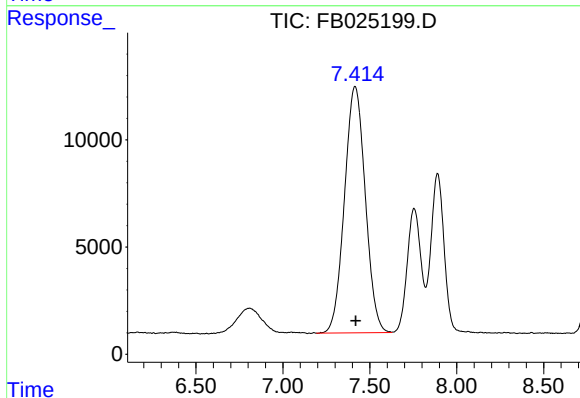


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 955590
Conc: 28.80 ng/ml

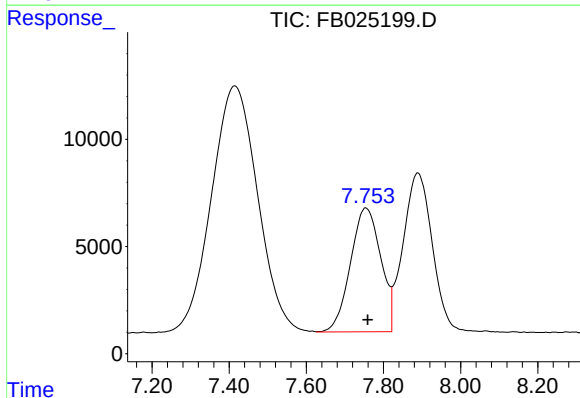


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 315206
Conc: 9.60 ng/ml

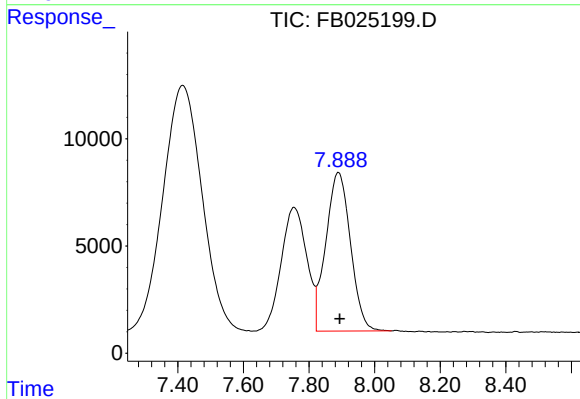


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 386653
Conc: 9.72 ng/ml

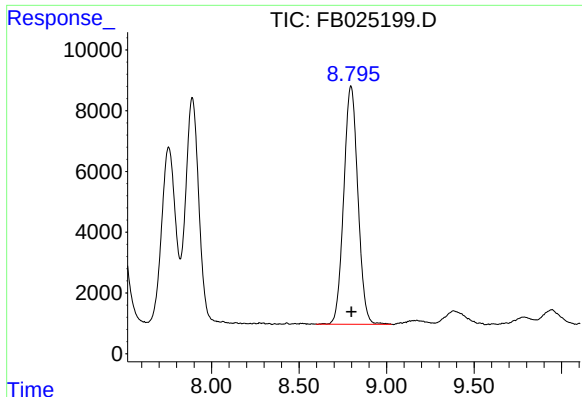


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 440199
Conc: 19.50 ng/ml

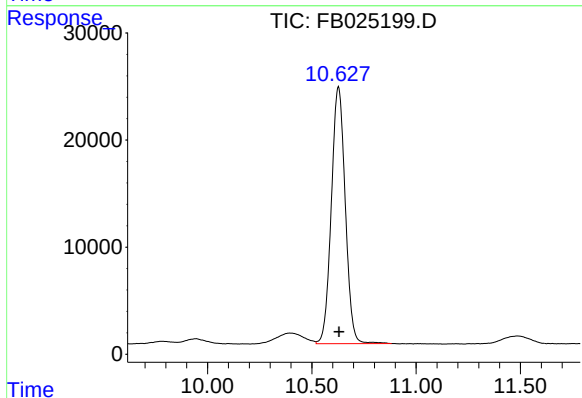


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1115271
Conc: 29.83 ng/ml

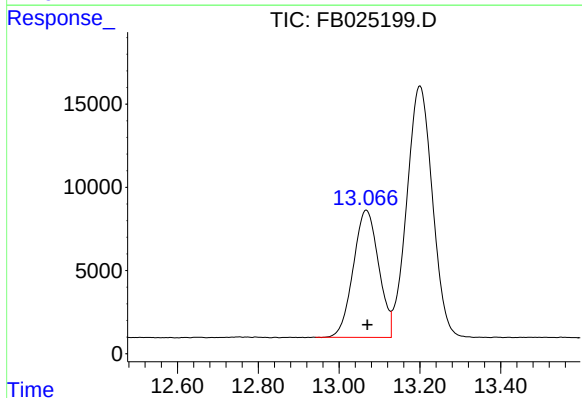


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 333327
Conc: 9.71 ng/ml

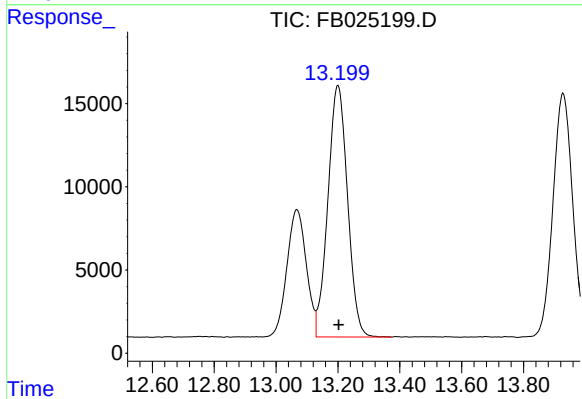


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 667534
Conc: 19.77 ng/ml

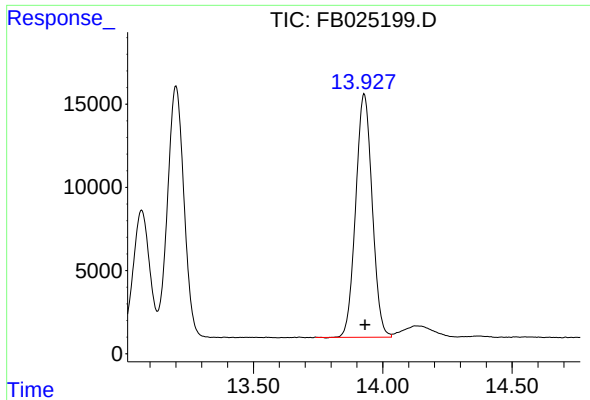

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 647274
Conc: 19.80 ng/ml

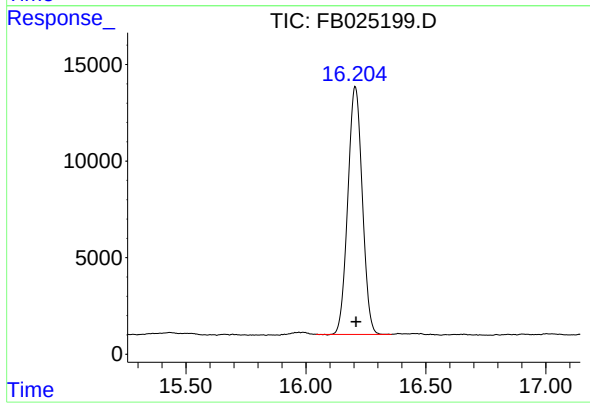

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 538501
Conc: 19.57 ng/ml