

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110620\
 Data File : FB025205.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2020 11:21
 Operator : DD/AJ
 Sample : L4657-02MSD
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 06 23:15:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	439076	19.446 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	840270	26.033 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	777851	23.445 ng/ml
3) t n-Heptane	7.759	238908	7.274 ng/ml
4) t Benzene	7.893	380080	9.559 ng/ml
6) t Toluene	10.630	1030231	27.553 ng/ml
7) t Ethylbenzene	13.070	299340	8.717 ng/ml
8) t m-Xylene	13.203	601938	17.828 ng/ml
9) t O-Xylene	13.931	585040	17.893 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	454913	16.533 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110620\
Data File : FB025205.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2020 11:21
Operator : DD/AJ
Sample : L4657-02MSD
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 06 23:15:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

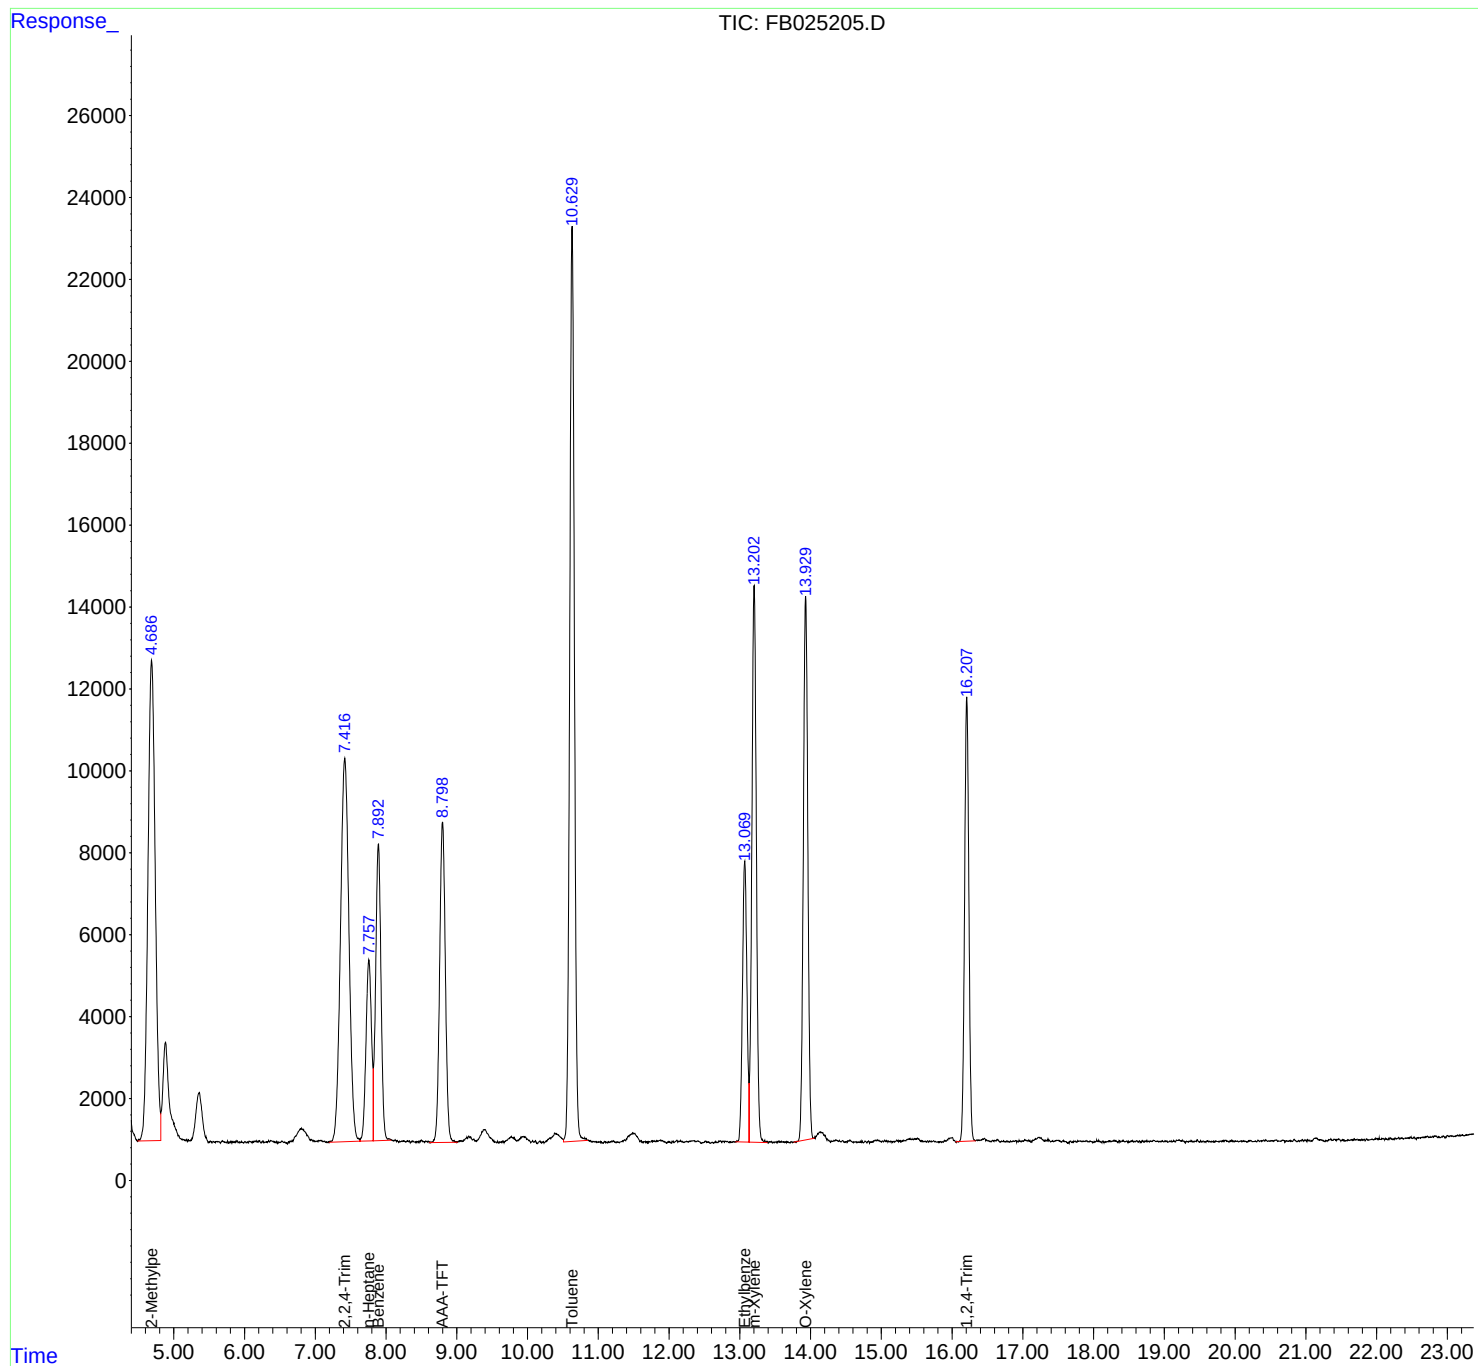

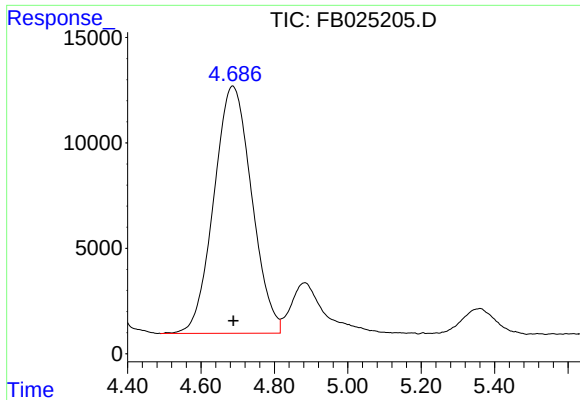


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 840270
Conc: 26.03 ng/ml

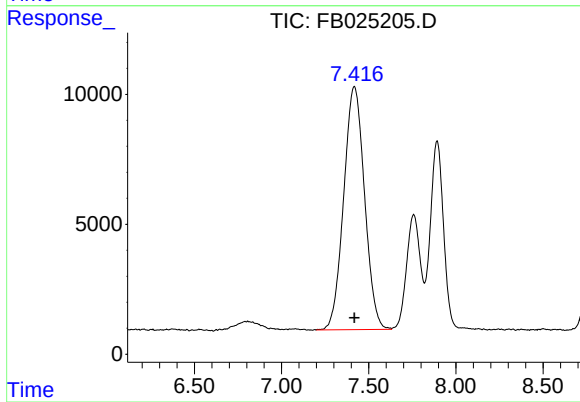


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 777851
Conc: 23.44 ng/ml

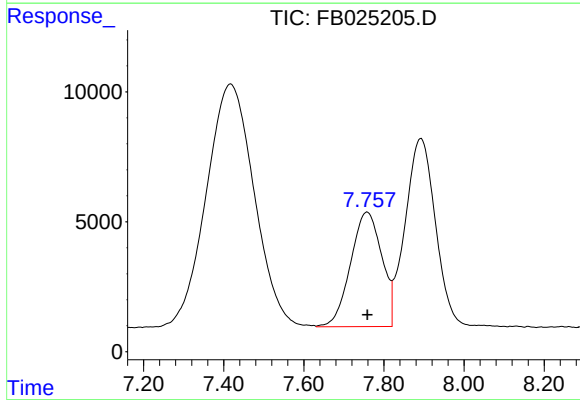


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 238908
Conc: 7.27 ng/ml

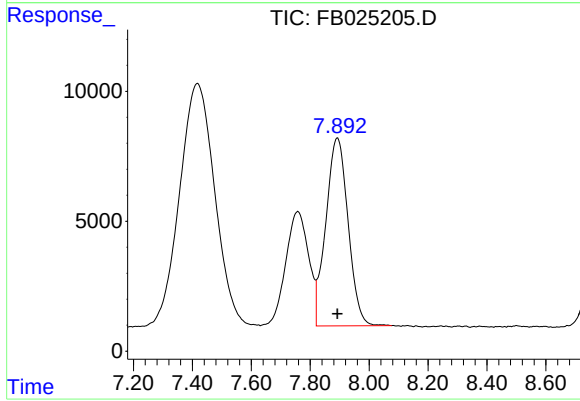


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 380080
Conc: 9.56 ng/ml

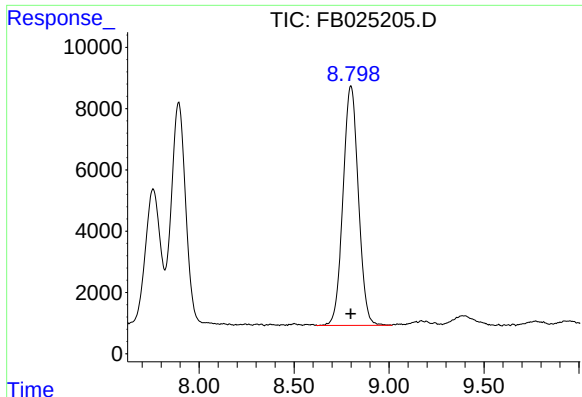


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 439076
Conc: 19.45 ng/ml

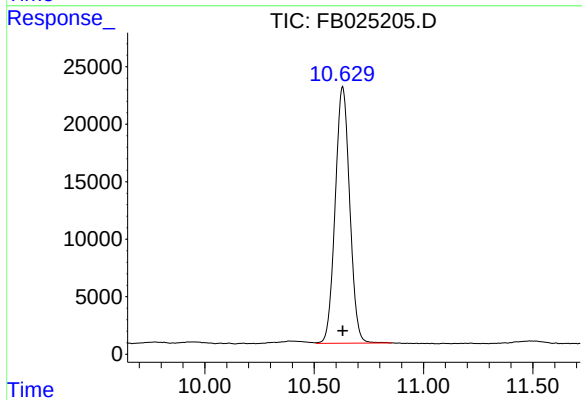


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1030231
Conc: 27.55 ng/ml

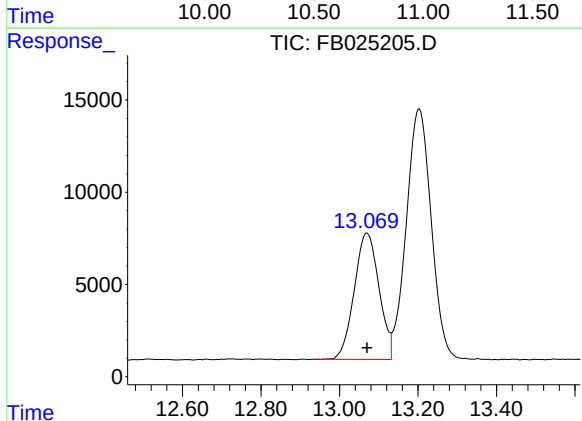


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 299340
Conc: 8.72 ng/ml

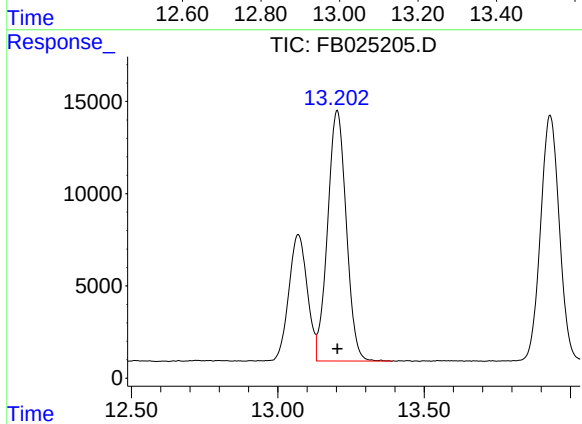


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 601938
Conc: 17.83 ng/ml

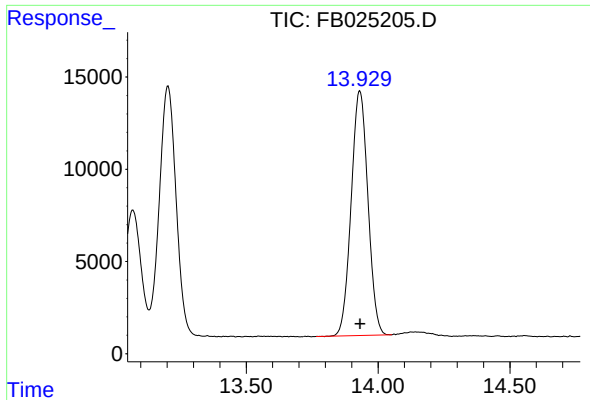

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 585040
Conc: 17.89 ng/ml

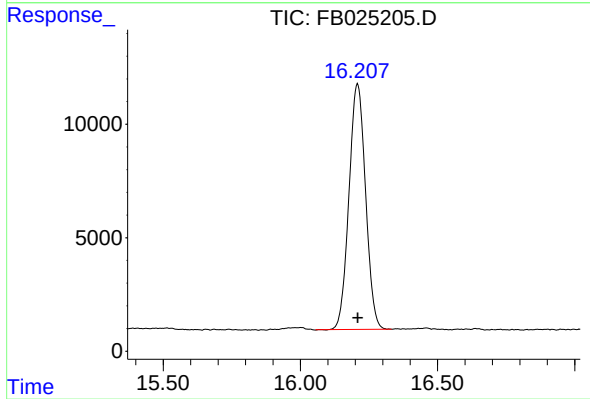

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 454913
Conc: 16.53 ng/ml