

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
 Data File : FB030431.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2023 12:06
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 23:13:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	361921	31.698 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	613	0.044 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	3471	0.210 ng/ml
3) t n-Heptane	7.748	31702	2.115 ng/ml
4) t Benzene	7.881	6280	0.306 ng/ml
6) t Toluene	10.609	334102	16.548 ng/ml
7) t Ethylbenzene	13.044	260718	13.062 ng/ml
8) t m-Xylene	13.176	335918	17.043 ng/ml
9) t O-Xylene	13.906	210969	10.719 ng/ml
10) t 1,2,4-Trimethylbenzene	16.176	1203088	58.238 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030431.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 12:06
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:13:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

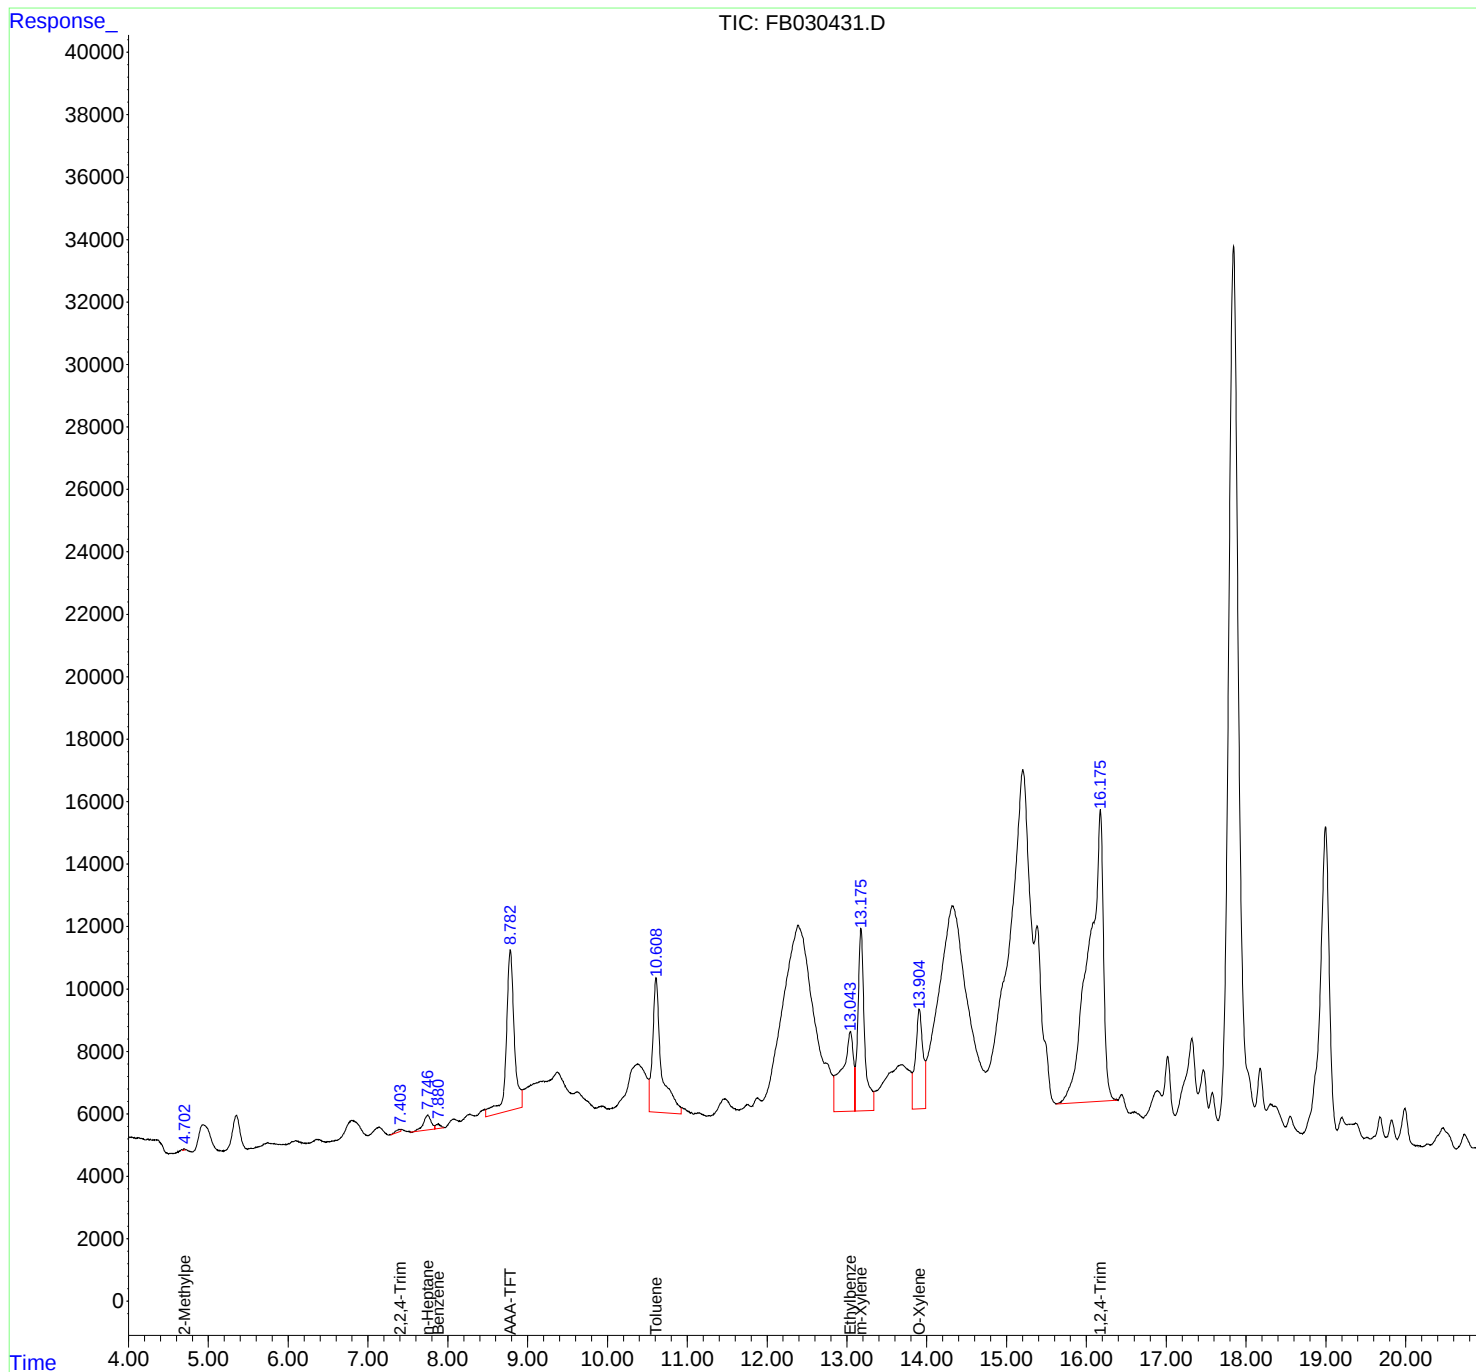


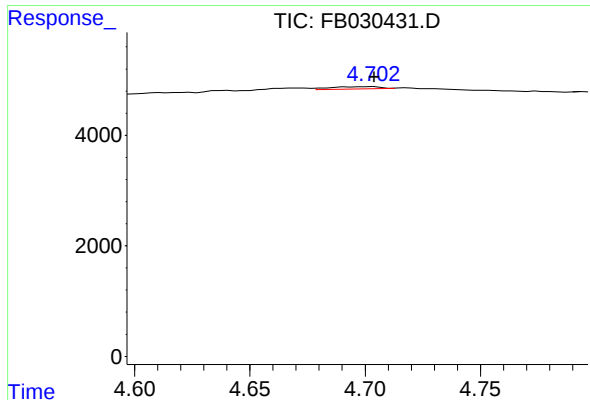

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 613
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :

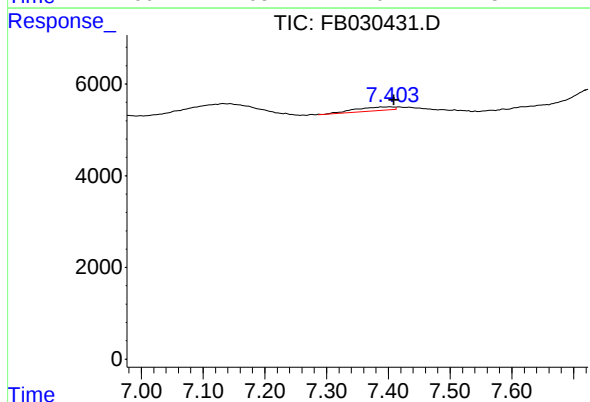


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: -0.005 min
Response: 3471
Conc: 0.21 ng/ml

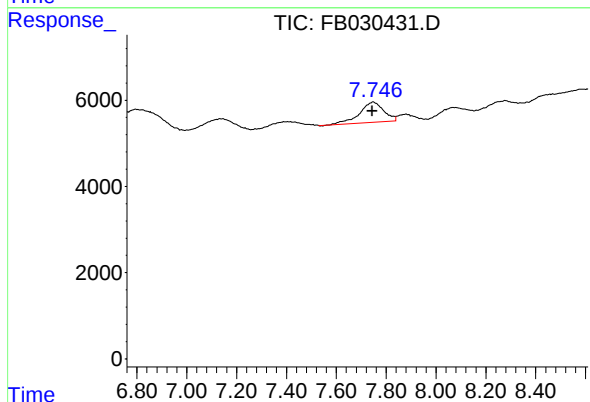


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.004 min
Response: 31702
Conc: 2.11 ng/ml

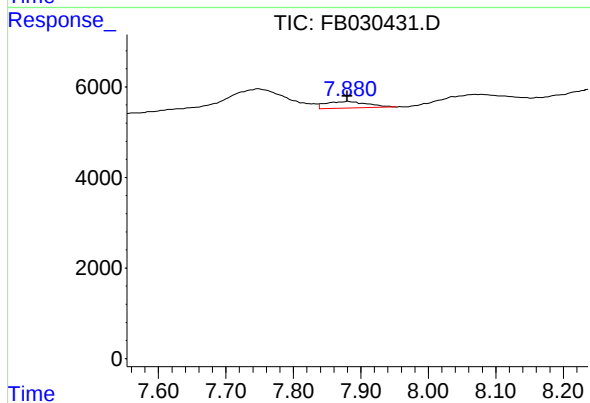

#4 Benzene


R.T.: 7.881 min
Delta R.T.: 0.002 min
Response: 6280
Conc: 0.31 ng/ml

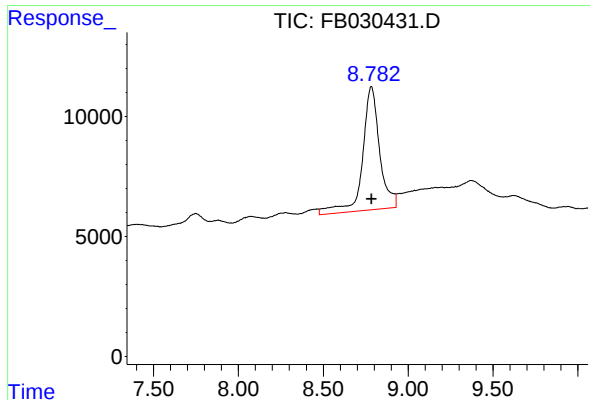

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: -0.001 min
Response: 361921
Conc: 31.70 ng/ml

Instrument :
FID_B
ClientSampleId :

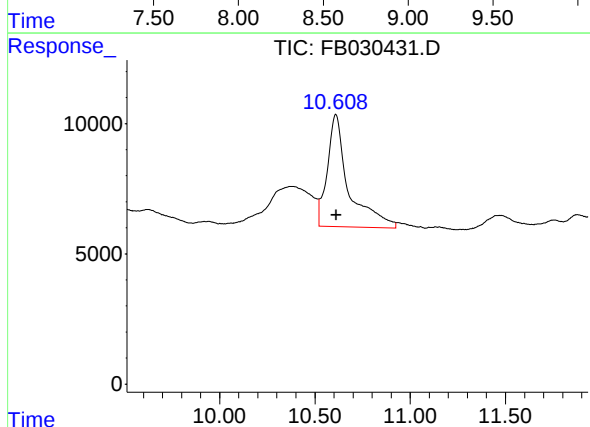


#6 Toluene

R.T.: 10.609 min
Delta R.T.: -0.003 min
Response: 334102
Conc: 16.55 ng/ml

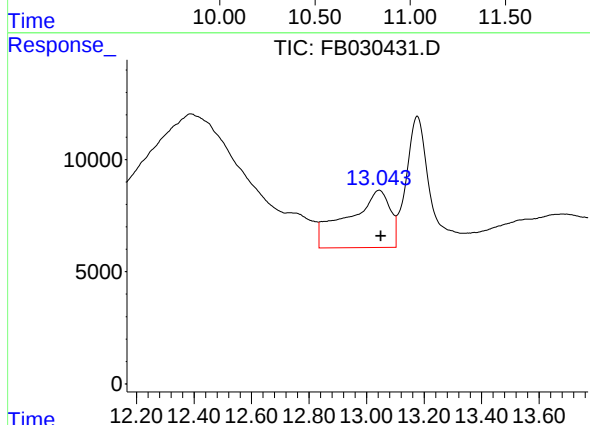


#7 Ethylbenzene

R.T.: 13.044 min
Delta R.T.: -0.005 min
Response: 260718
Conc: 13.06 ng/ml

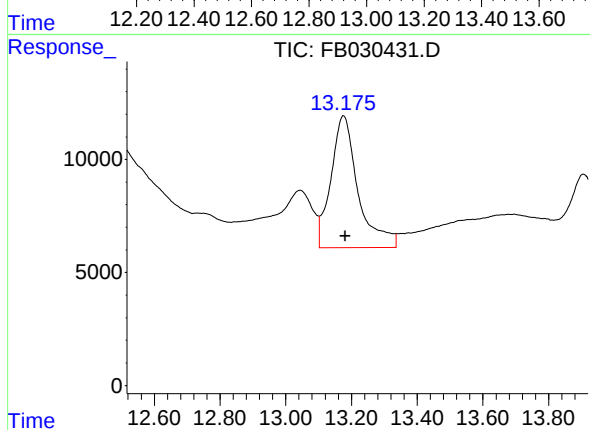

#8 m-Xylene


R.T.: 13.176 min
Delta R.T.: -0.005 min
Response: 335918
Conc: 17.04 ng/ml

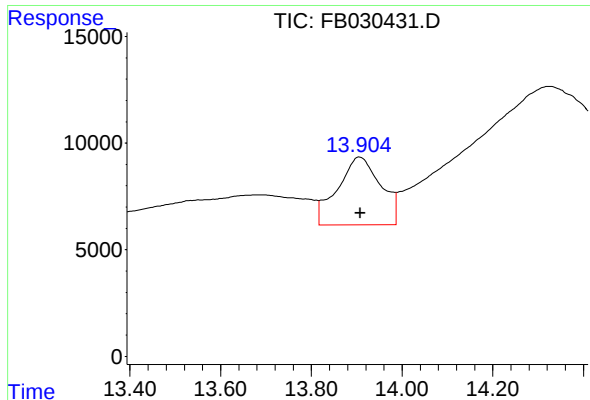

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: -0.002 min
Response: 210969
Conc: 10.72 ng/ml

Instrument :
FID_B
ClientSampleId :

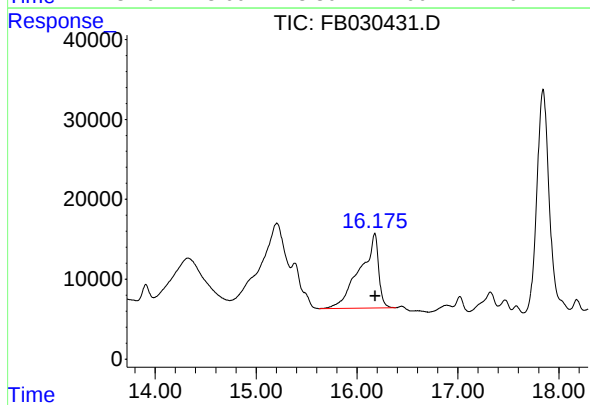

#10 1,2,4-Trimethylbenzene

R.T.: 16.176 min
Delta R.T.: -0.008 min
Response: 1203088
Conc: 58.24 ng/ml