

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030432.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 12:44
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:13:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	186581	16.341 ng/ml
Target Compounds			
6) t Toluene	10.610	40968	2.029 ng/ml
7) t Ethylbenzene	13.047	14571	0.730 ng/ml
8) t m-Xylene	13.177	56734	2.879 ng/ml
9) t O-Xylene	13.909	23800	1.209 ng/ml
10) t 1,2,4-Trimethylbenzene	16.180	54431	2.635 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030432.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 12:44
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:13:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

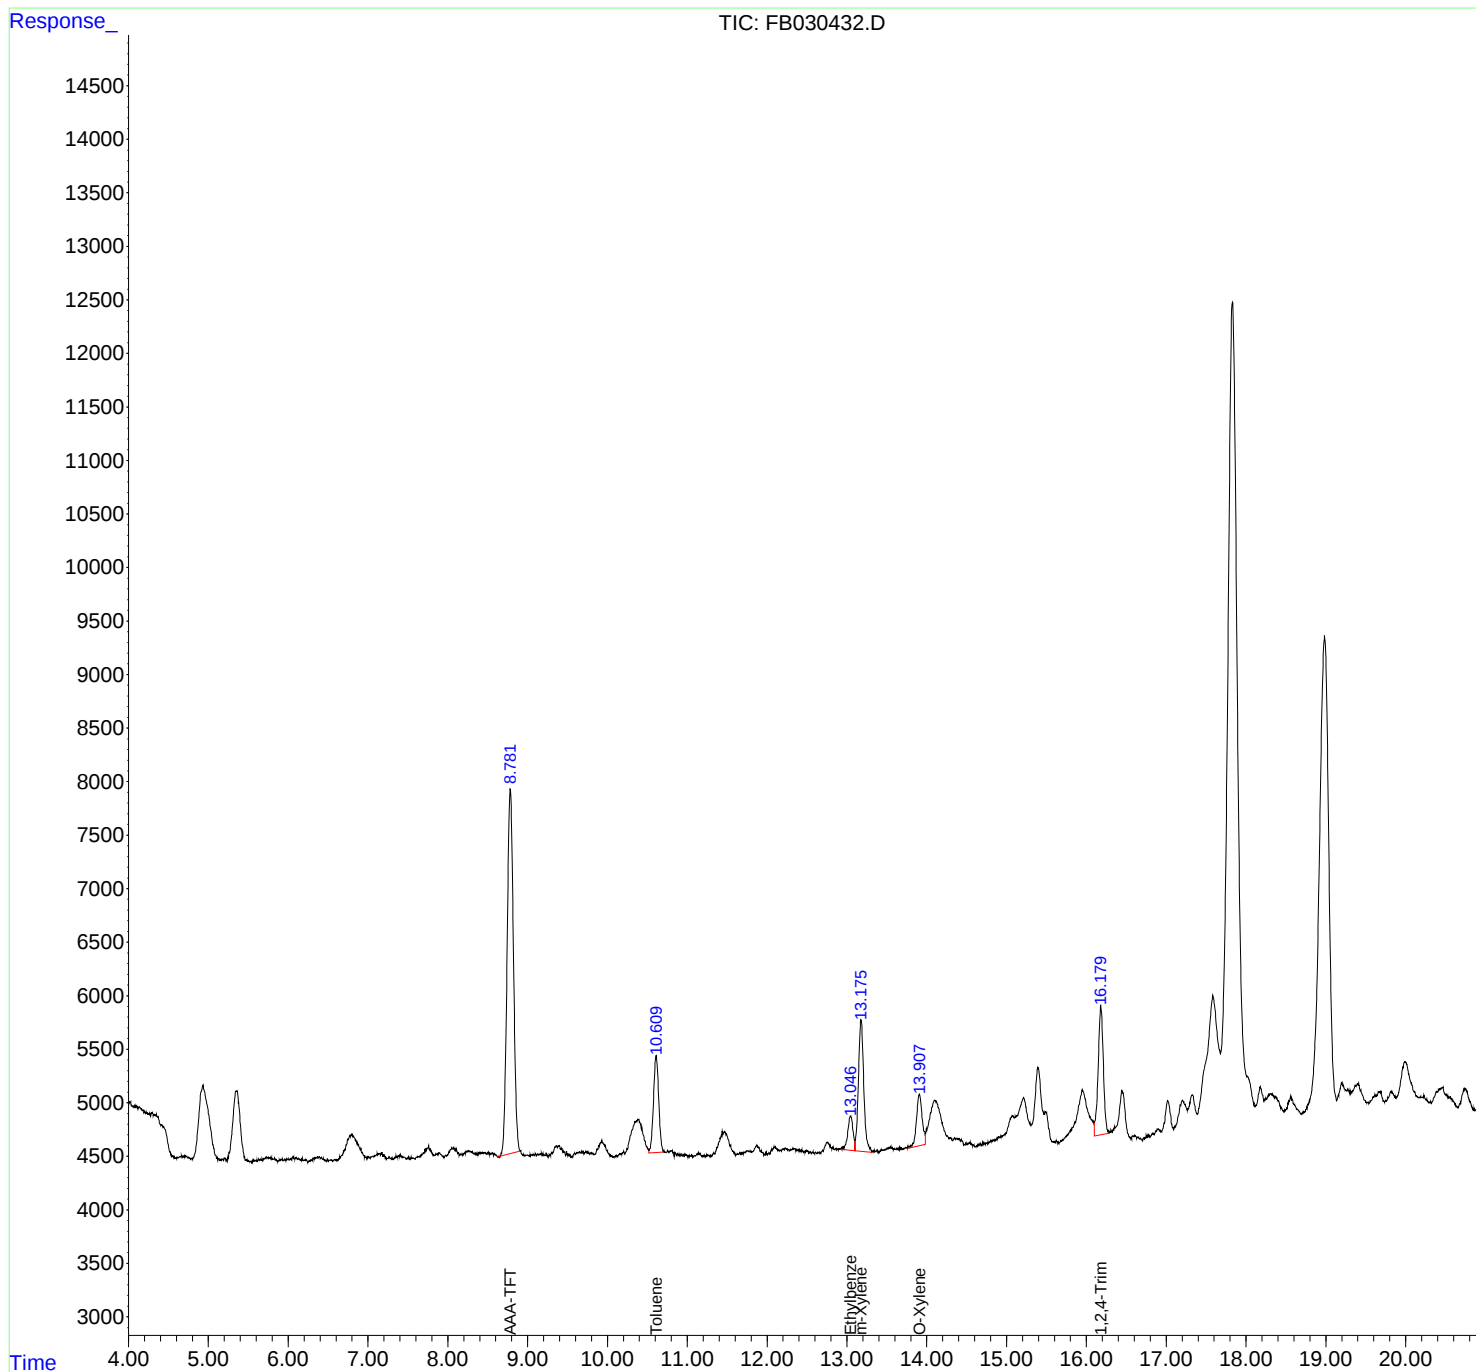


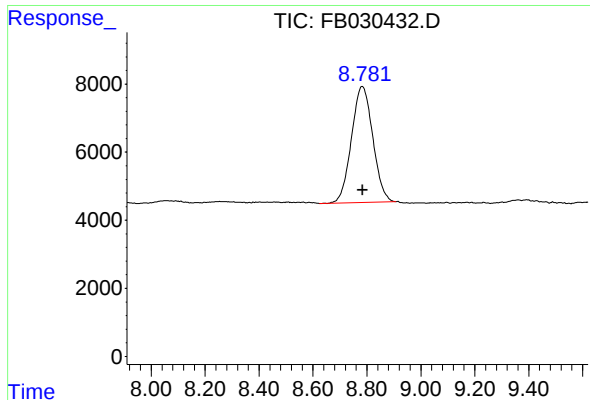

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: -0.002 min
Response: 186581
Conc: 16.34 ng/ml

Instrument :
FID_B
ClientSampleId :

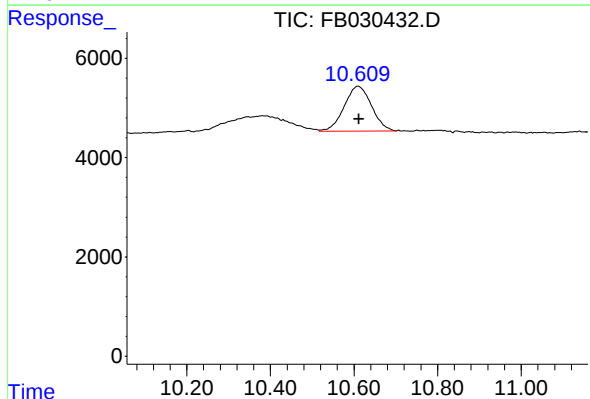


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.002 min
Response: 40968
Conc: 2.03 ng/ml

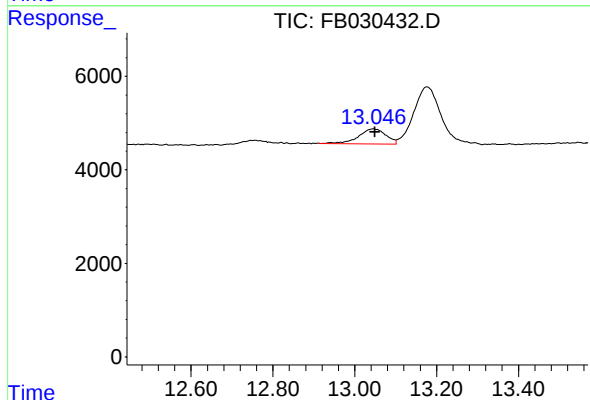


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.002 min
Response: 14571
Conc: 0.73 ng/ml

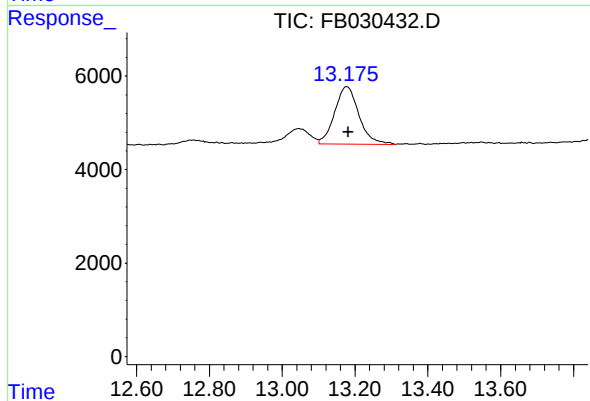

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: -0.005 min
Response: 56734
Conc: 2.88 ng/ml

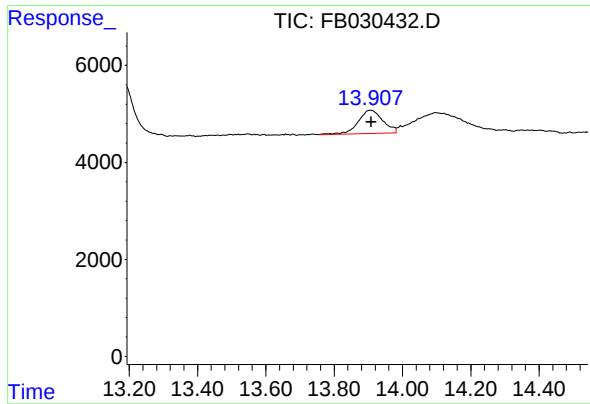

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.000 min
Response: 23800
Conc: 1.21 ng/ml

Instrument :
FID_B
ClientSampleId :

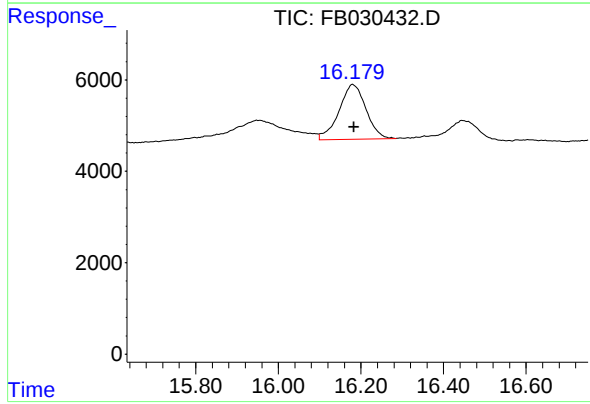

#10 1,2,4-Trimethylbenzene

R.T.: 16.180 min
Delta R.T.: -0.003 min
Response: 54431
Conc: 2.63 ng/ml