

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030436.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 15:16
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:13:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	190192	16.657 ng/ml
Target Compounds			
6) t Toluene	10.612	9202	0.456 ng/ml
8) t m-Xylene	13.175	11329	0.575 ng/ml
9) t O-Xylene	13.913	5254	0.267 ng/ml
10) t 1,2,4-Trimethylbenzene	16.174	11546	0.559 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030436.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 15:16
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:13:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

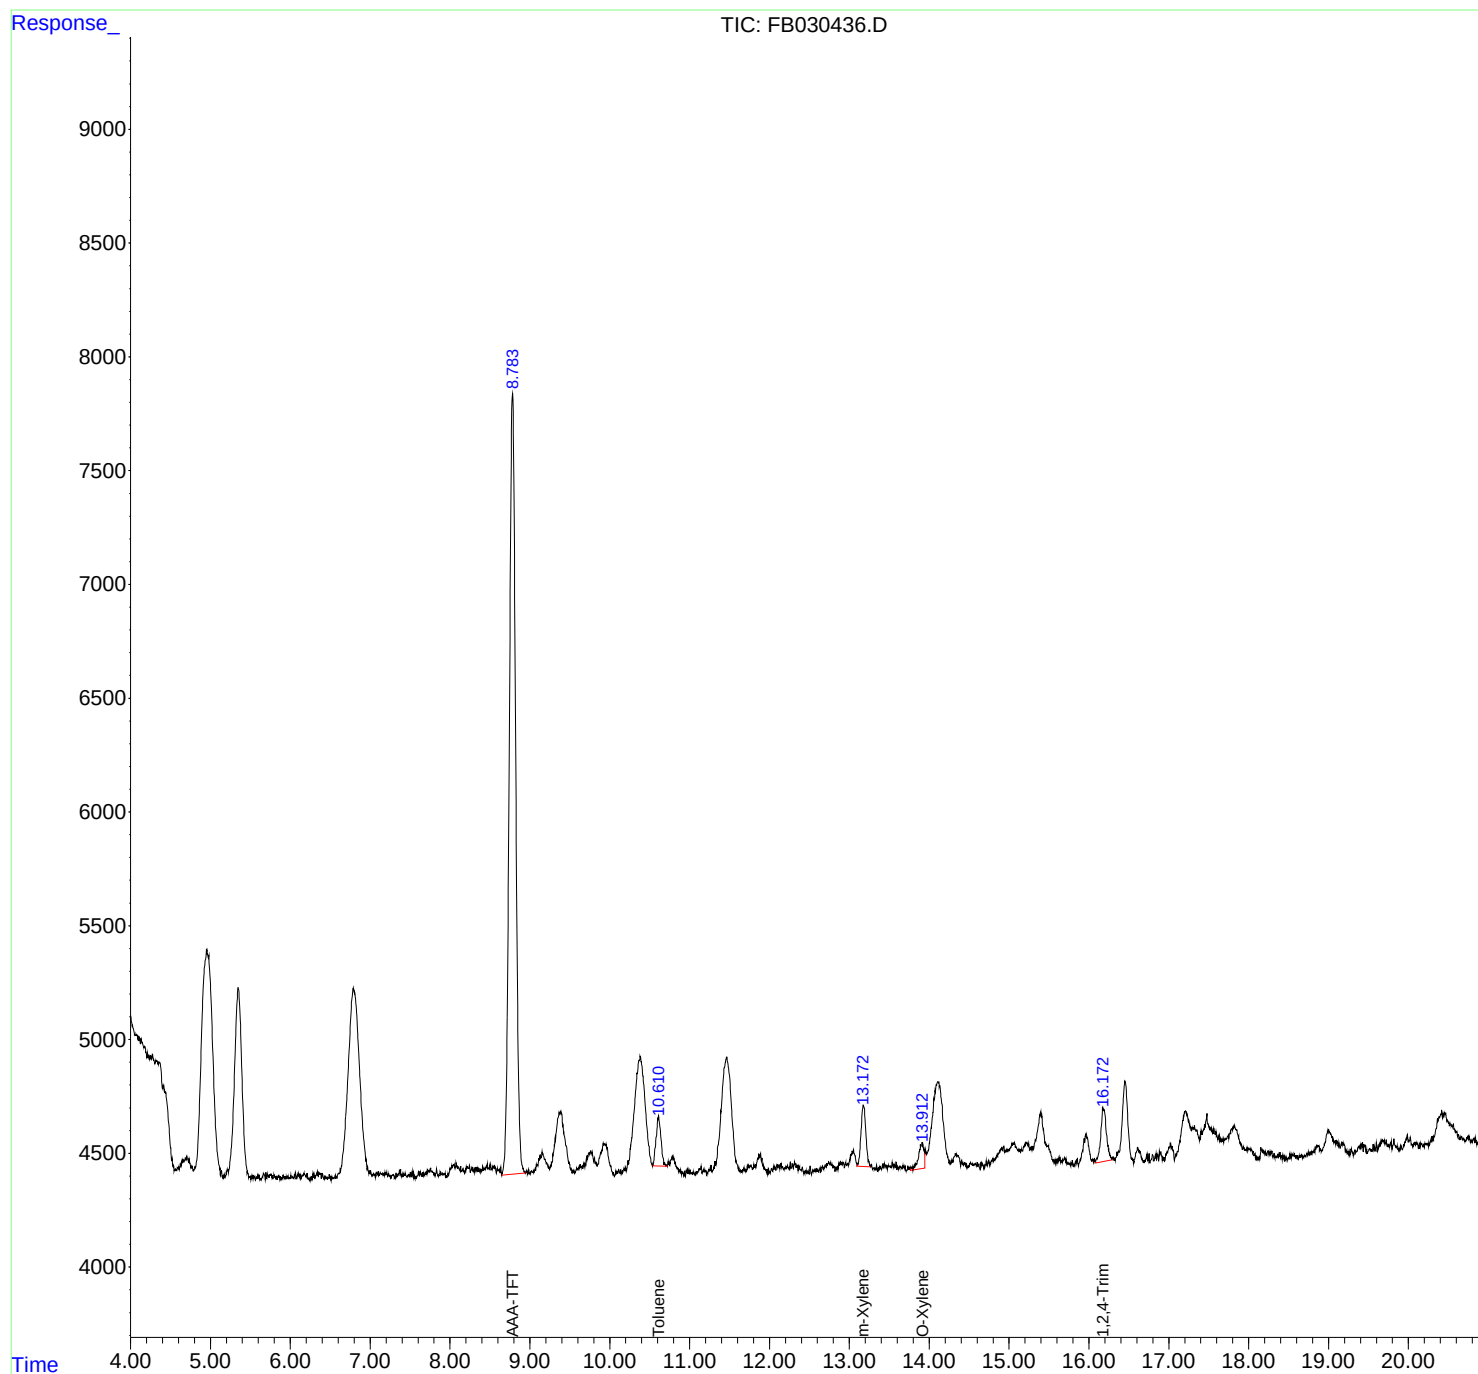


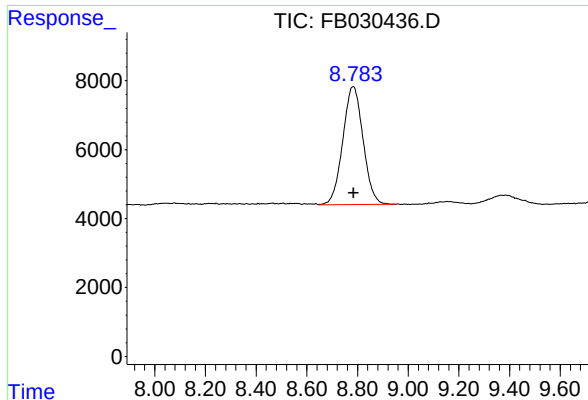

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 190192
Conc: 16.66 ng/ml

Instrument :
FID_B
ClientSampleId :

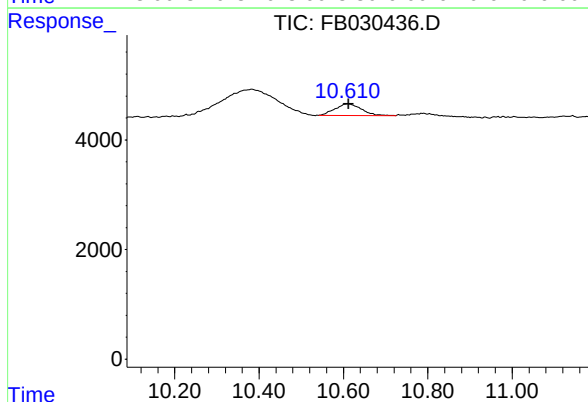


#6 Toluene

R.T.: 10.612 min
Delta R.T.: 0.000 min
Response: 9202
Conc: 0.46 ng/ml

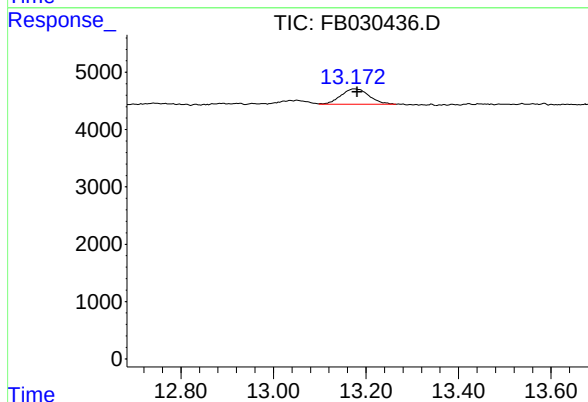


#8 m-Xylene

R.T.: 13.175 min
Delta R.T.: -0.006 min
Response: 11329
Conc: 0.57 ng/ml

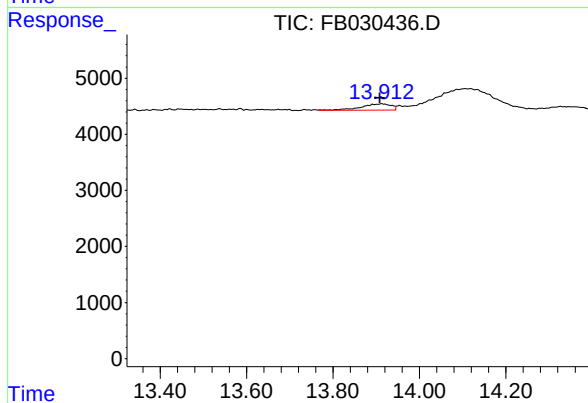

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.005 min
Response: 5254
Conc: 0.27 ng/ml

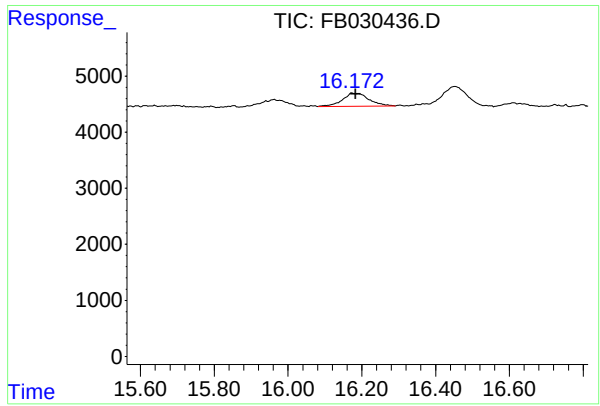

#10 1,2,4-Trimethylbenzene

R.T.: 16.174 min

Delta R.T.: -0.010 min

Response: 11546

Conc: 0.56 ng/ml

Instrument :

FID_B

ClientSampleId :