

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
 Data File : FB030438.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2023 16:32
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 23:14:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	239620	20.987 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	400602	28.632 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	501631	30.383 ng/ml
3) t n-Heptane	7.744	139612	9.314 ng/ml
4) t Benzene	7.879	212895	10.377 ng/ml
6) t Toluene	10.611	624161	30.915 ng/ml
7) t Ethylbenzene	13.047	209142	10.478 ng/ml
8) t m-Xylene	13.180	414891	21.050 ng/ml
9) t O-Xylene	13.906	409595	20.811 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	434683	21.042 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030438.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 16:32
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:14:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

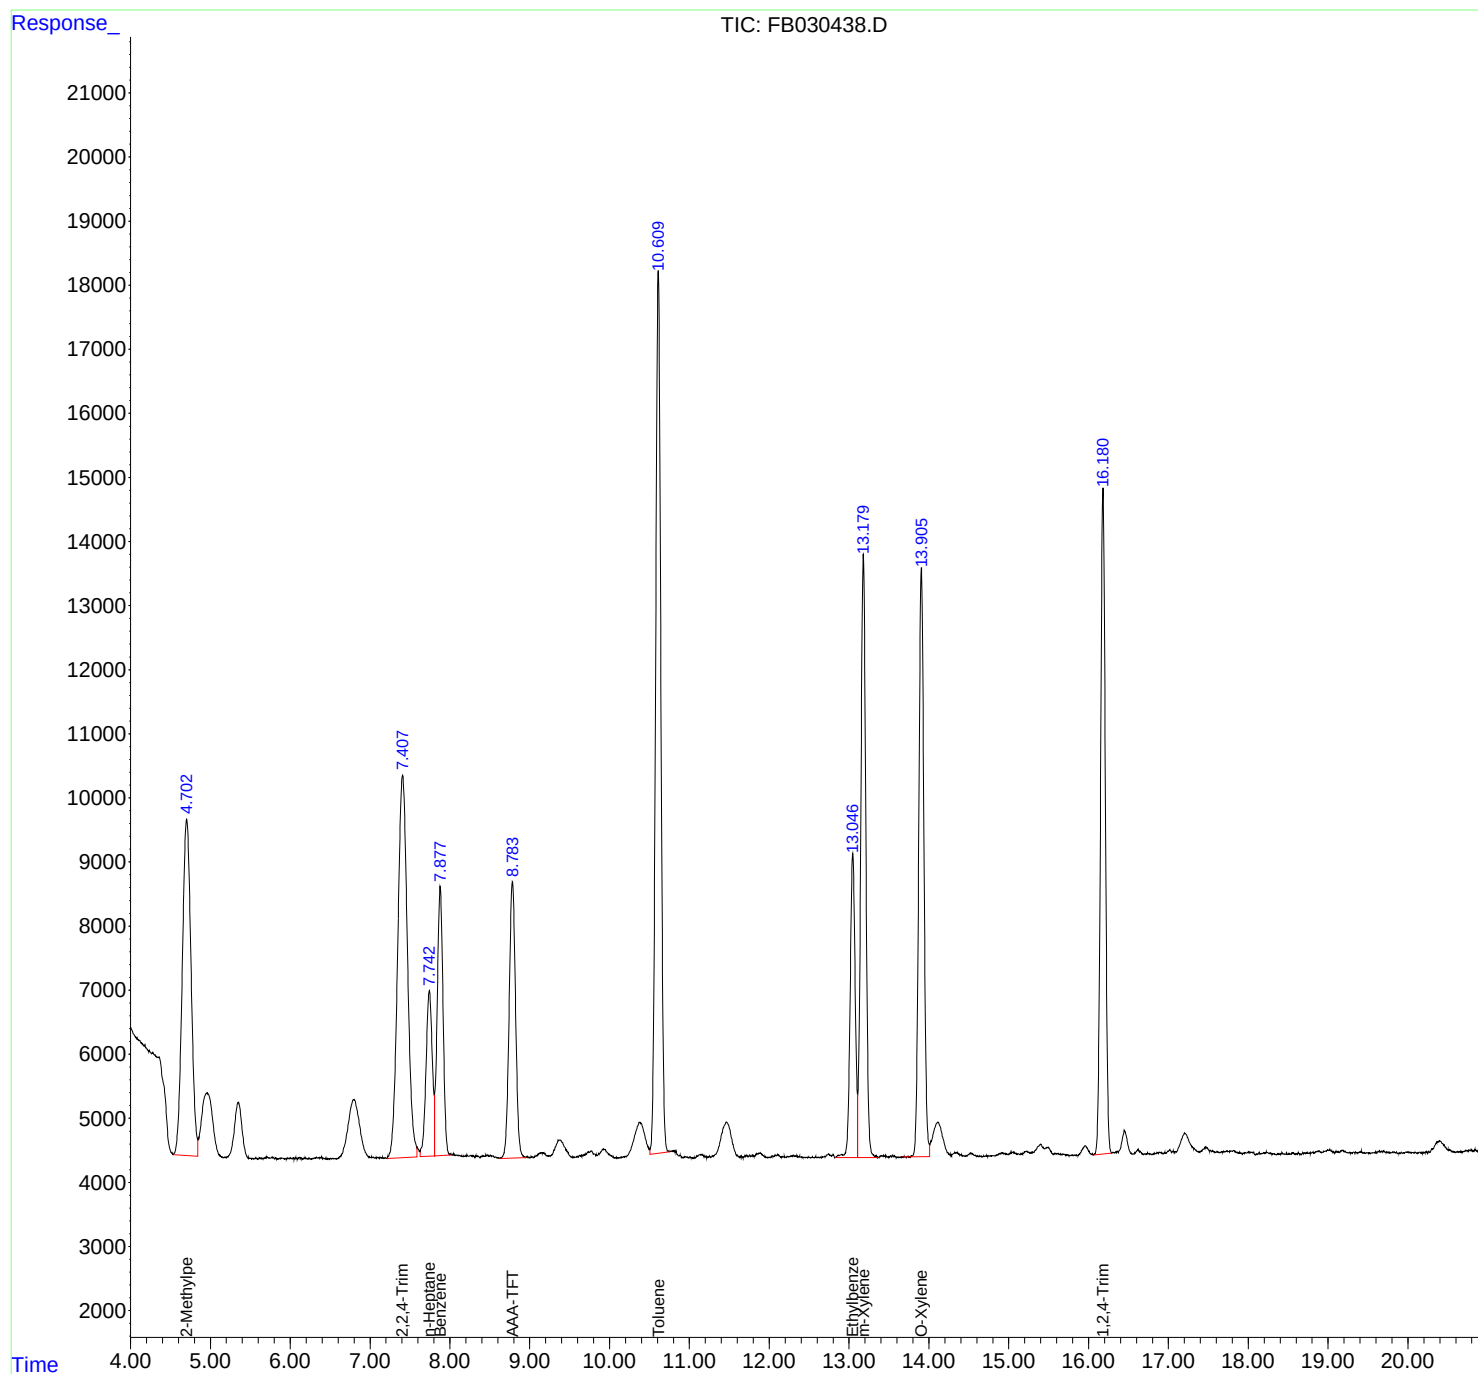


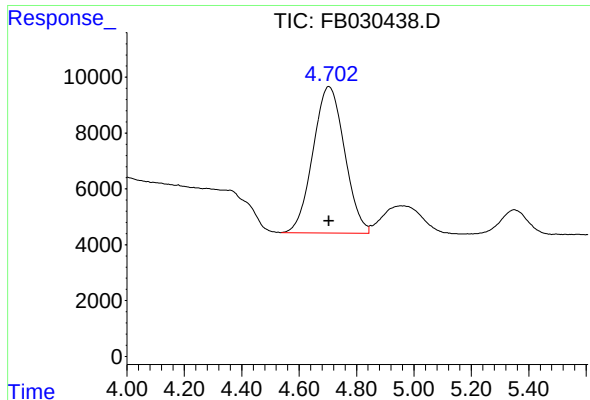

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 400602
Conc: 28.63 ng/ml

Instrument :
FID_B
ClientSampleId :

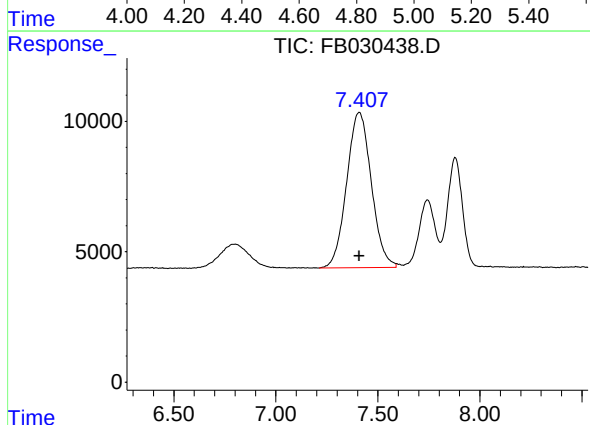


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 501631
Conc: 30.38 ng/ml

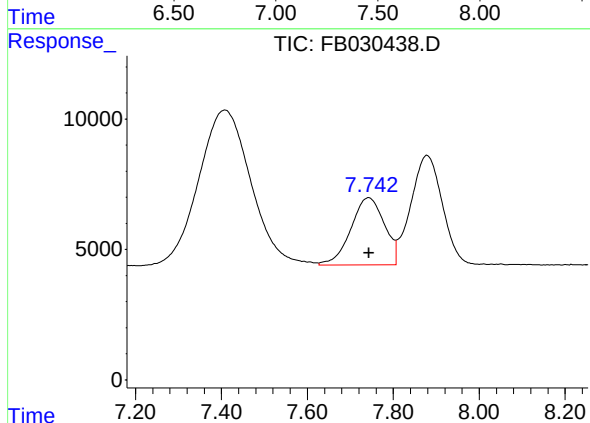


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 139612
Conc: 9.31 ng/ml

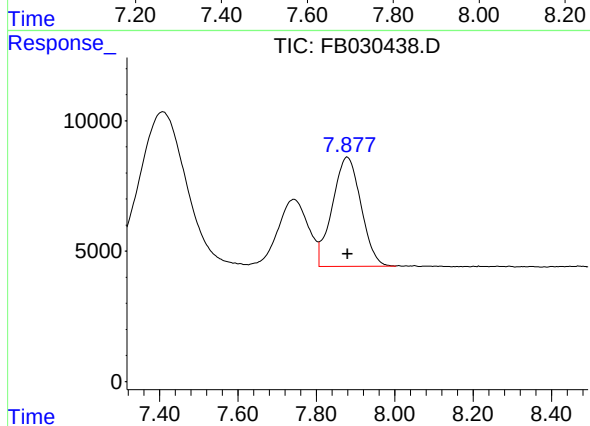

#4 Benzene


R.T.: 7.879 min
Delta R.T.: 0.000 min
Response: 212895
Conc: 10.38 ng/ml

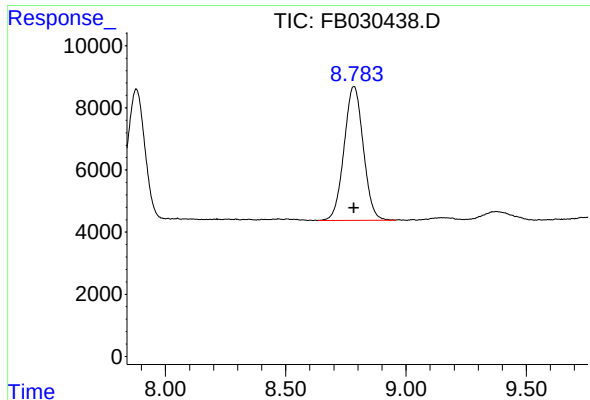

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 239620
Conc: 20.99 ng/ml

Instrument :
FID_B
ClientSampleId :

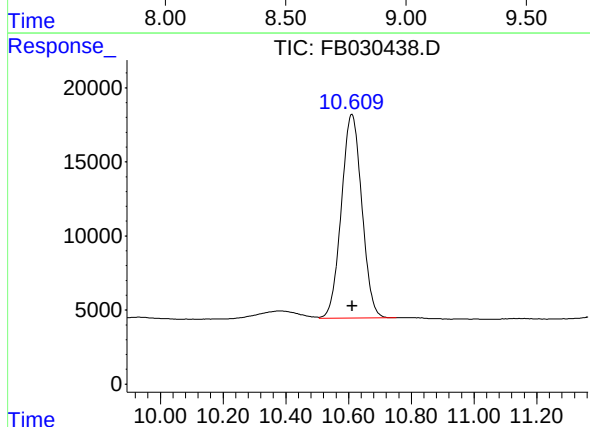


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.002 min
Response: 624161
Conc: 30.92 ng/ml

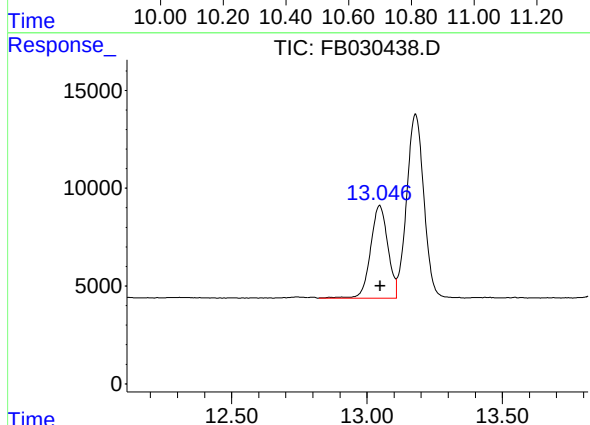


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.002 min
Response: 209142
Conc: 10.48 ng/ml

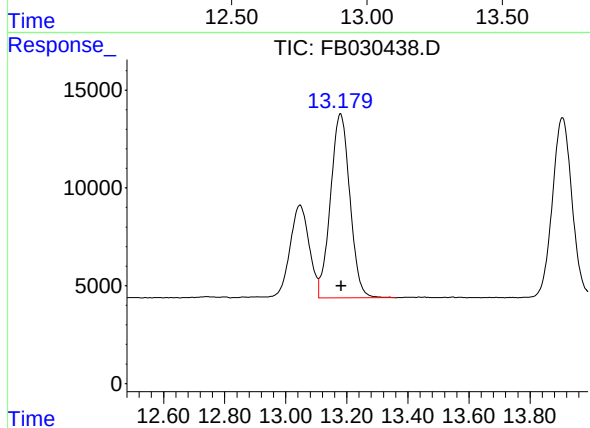

#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.002 min
Response: 414891
Conc: 21.05 ng/ml

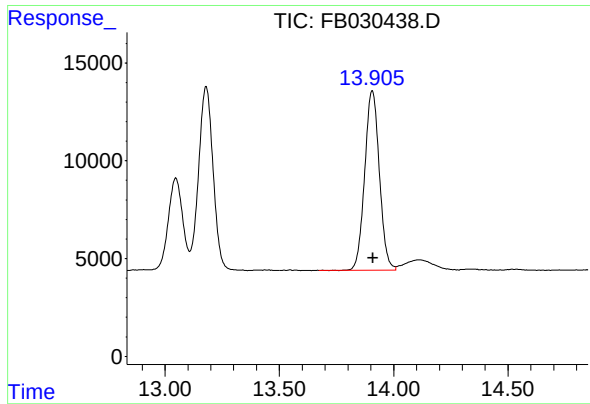


#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: -0.002 min
Response: 409595
Conc: 20.81 ng/ml

Instrument : FID_B

ClientSampleId :

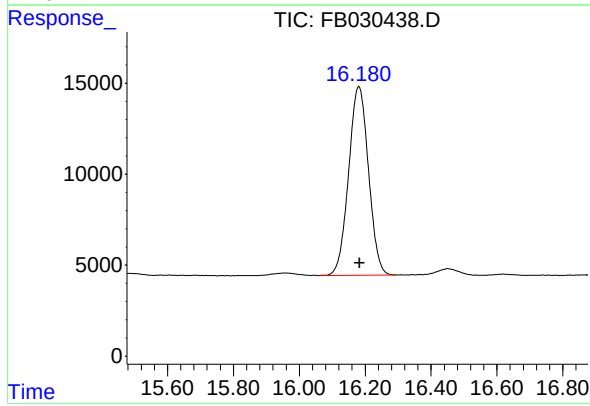

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: -0.002 min
Response: 434683
Conc: 21.04 ng/ml