

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
 Data File : FB030442.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2023 19:43
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 06 23:14:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	216717	18.981 ng/ml
Target Compounds			
6) t Toluene	10.612	4437	0.220 ng/ml
8) t m-Xylene	13.181	4655	0.236 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	7830	0.379 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030442.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 19:43
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 06 23:14:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

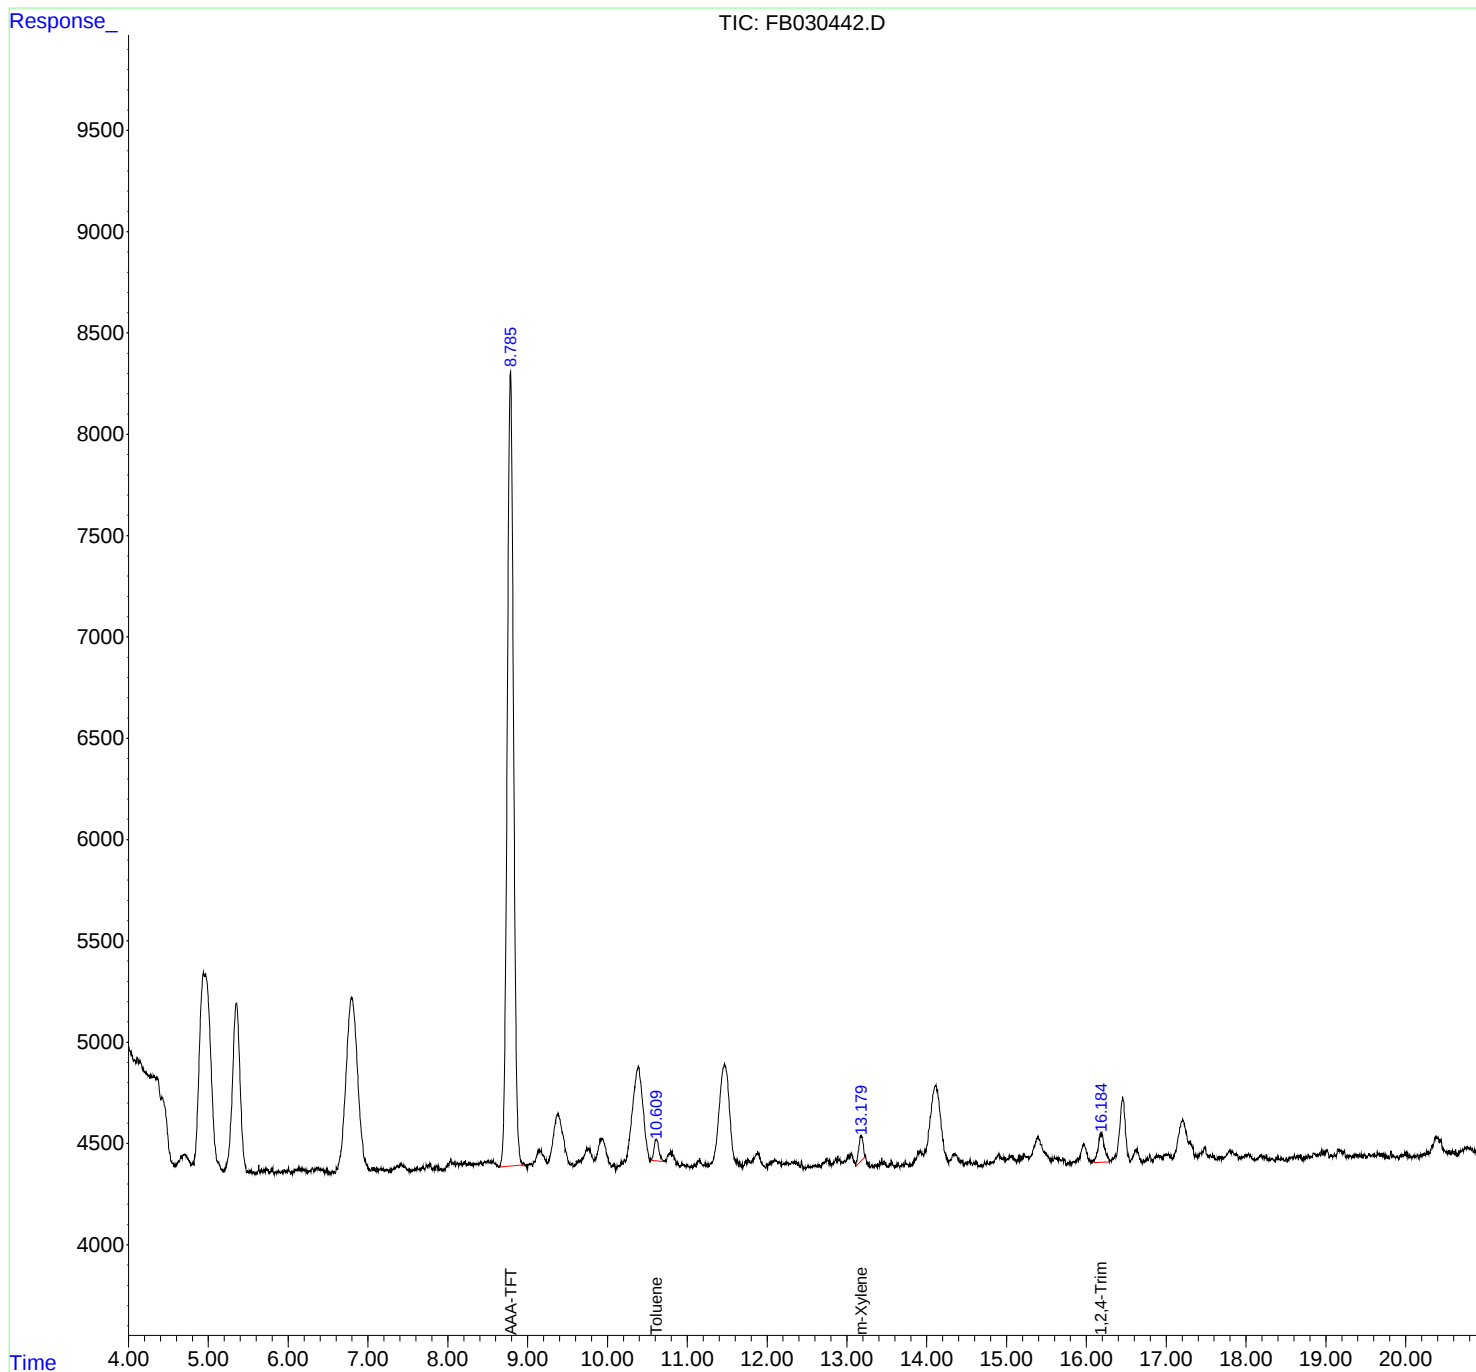

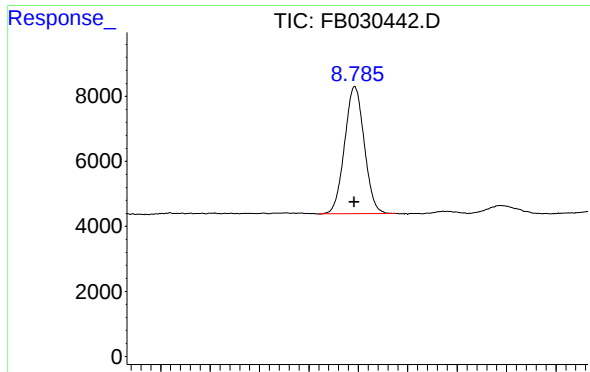


#5 AAA-TFT

R.T.: 8.786 min
Delta R.T.: 0.002 min
Response: 216717
Conc: 18.98 ng/ml

Instrument :


FID_B

ClientSampleId :

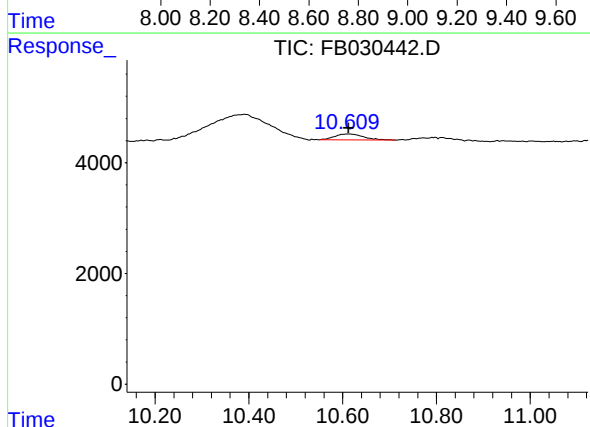


#6 Toluene

R.T.: 10.612 min
Delta R.T.: 0.000 min
Response: 4437
Conc: 0.22 ng/ml

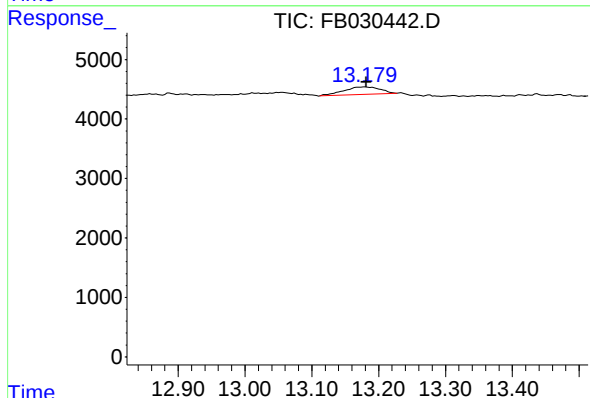

#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: 0.000 min
Response: 4655
Conc: 0.24 ng/ml

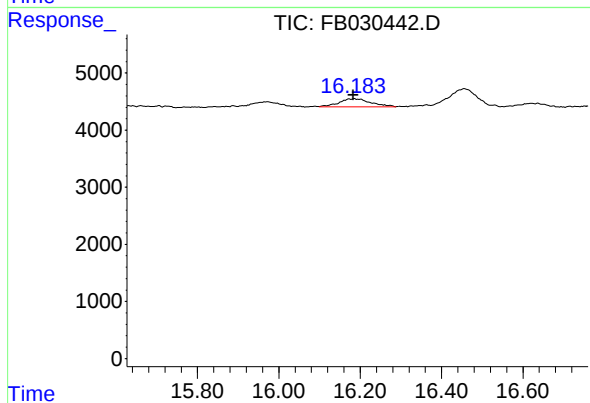

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.003 min
Response: 7830
Conc: 0.38 ng/ml