

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030427.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 9:35
Operator : YP/AJ
Sample : VBF1106S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1106S1

Integration File: Calibration.e
Quant Time: Nov 06 23:12:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	203795	17.849 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030427.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 9:35
Operator : YP/AJ
Sample : VBF1106S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1106S1

Integration File: Calibration.e
Quant Time: Nov 06 23:12:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

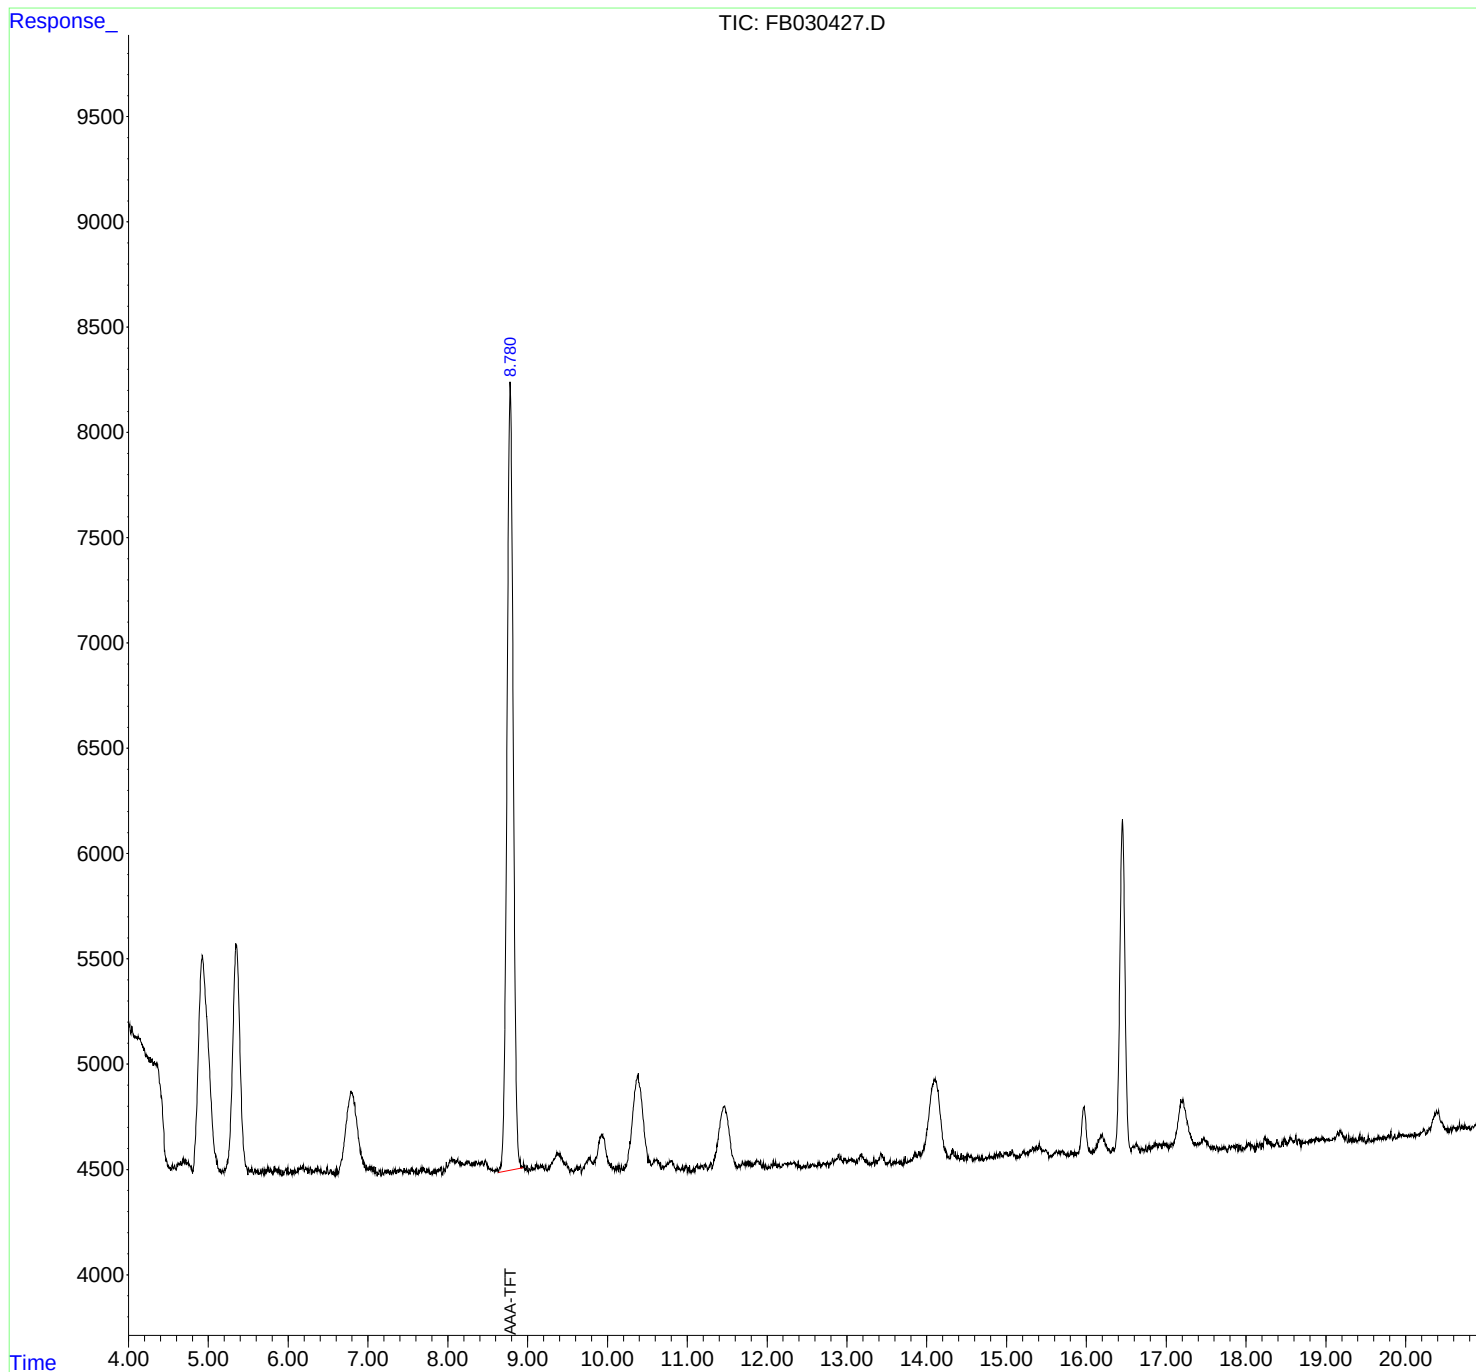

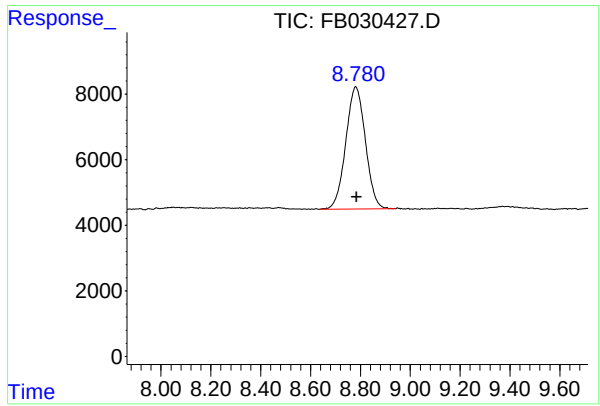

#5 AAA-TFT

R.T.: 8.782 min
Delta R.T.: -0.003 min
Response: 203795
Conc: 17.85 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1106S1