

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
 Data File : FB030429.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2023 10:51
 Operator : YP/AJ
 Sample : BSF1106S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1106S1

Integration File: Calibration.e
 Quant Time: Nov 06 23:13:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.781	204779	17.935 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	404155	28.886 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	460919	27.917 ng/ml
3) t n-Heptane	7.740	151062	10.078 ng/ml
4) t Benzene	7.876	216786	10.566 ng/ml
6) t Toluene	10.608	646668	32.030 ng/ml
7) t Ethylbenzene	13.044	207130	10.377 ng/ml
8) t m-Xylene	13.177	408167	20.709 ng/ml
9) t O-Xylene	13.903	400669	20.358 ng/ml
10) t 1,2,4-Trimethylbenzene	16.179	405774	19.643 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110623\
Data File : FB030429.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2023 10:51
Operator : YP/AJ
Sample : BSF1106S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1106S1

Integration File: Calibration.e
Quant Time: Nov 06 23:13:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

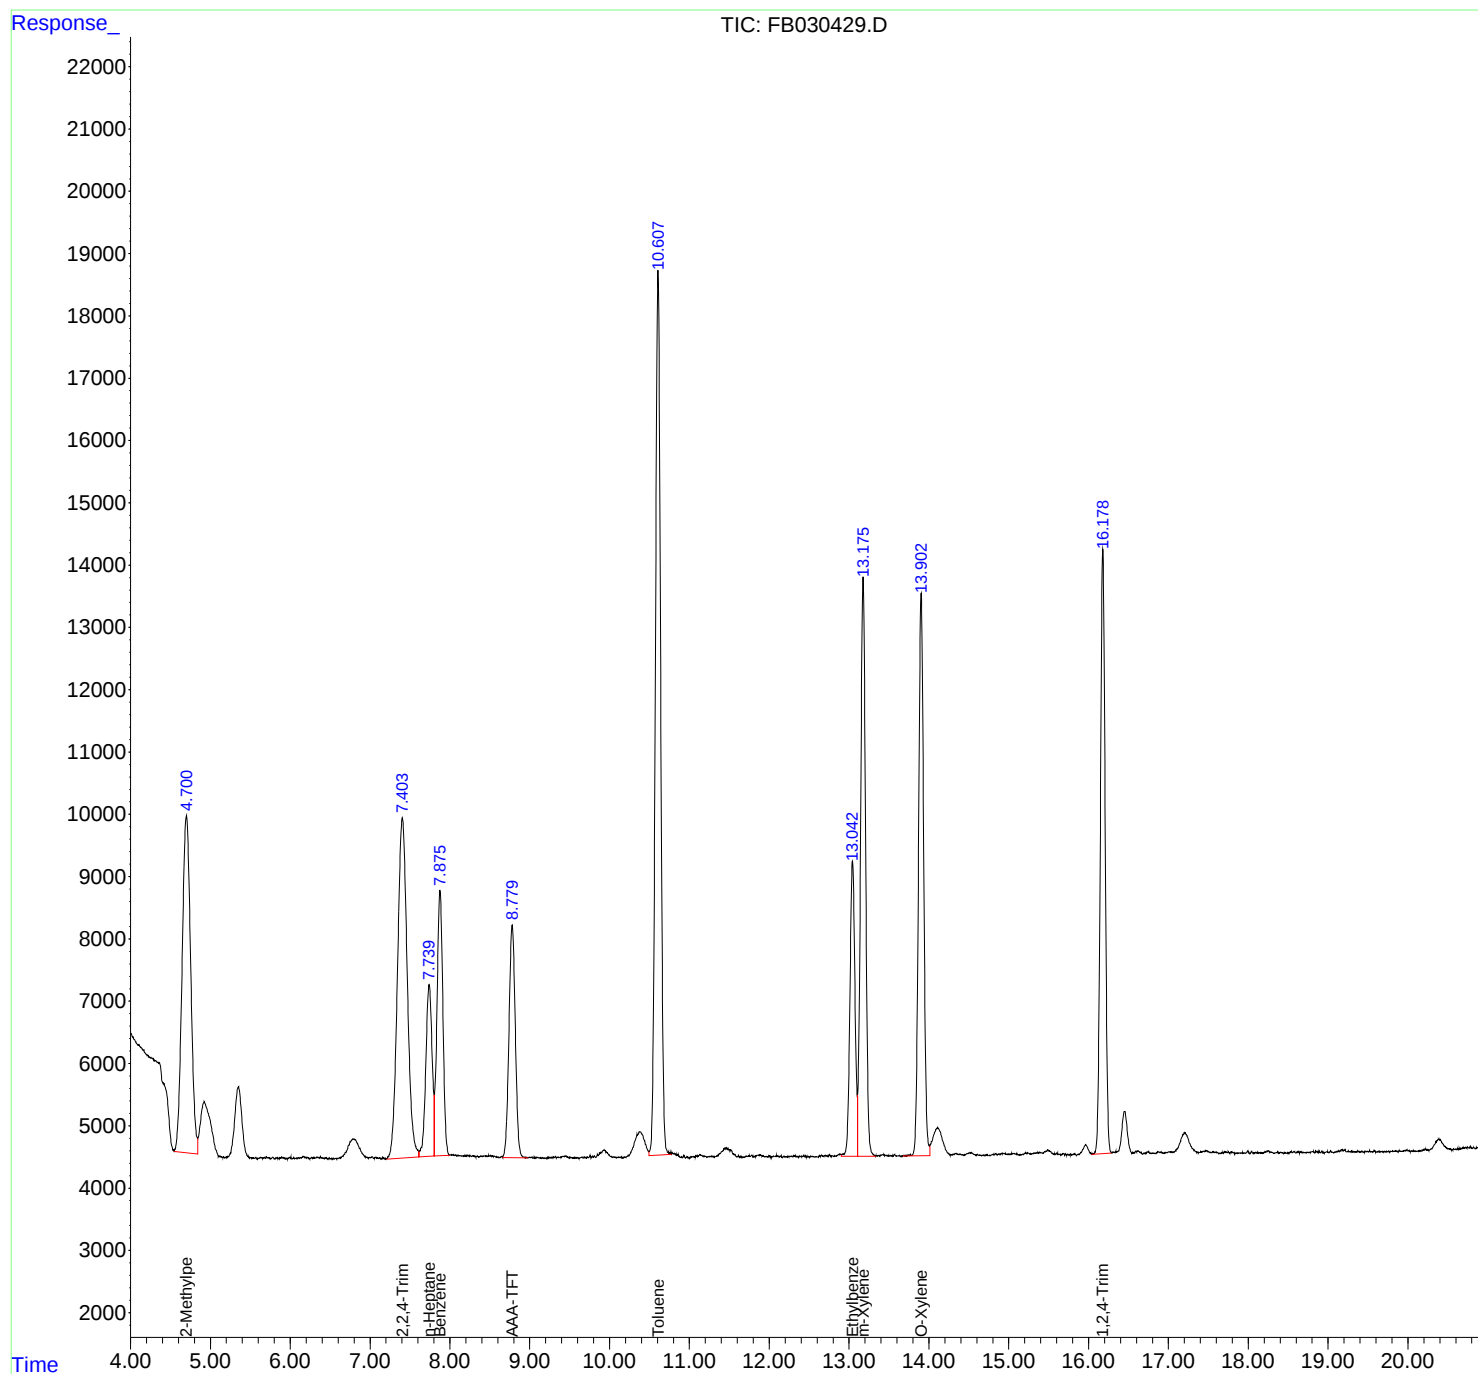


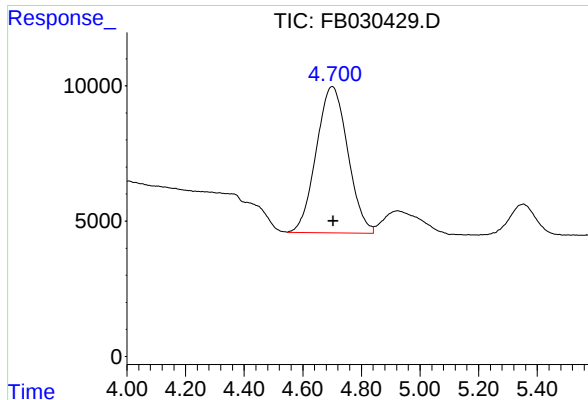

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.003 min
Response: 404155
Conc: 28.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S1

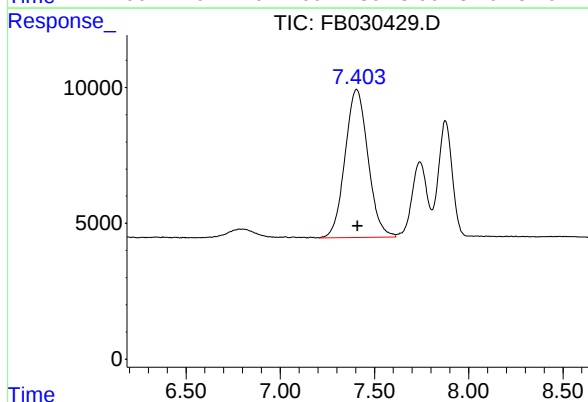


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: -0.005 min
Response: 460919
Conc: 27.92 ng/ml

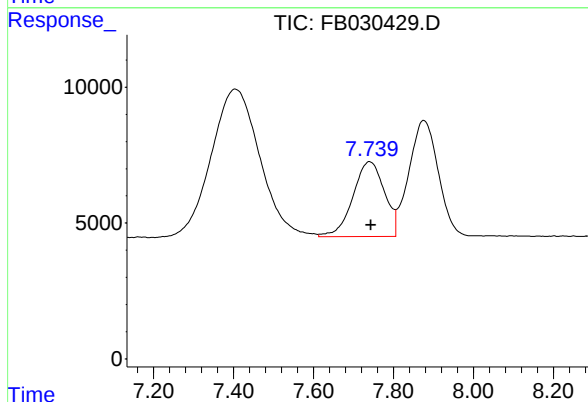


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.003 min
Response: 151062
Conc: 10.08 ng/ml

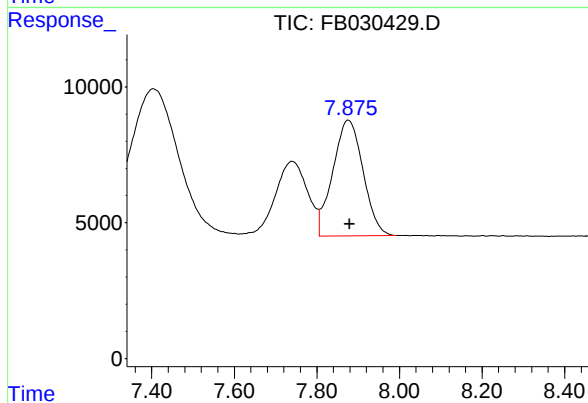

#4 Benzene


R.T.: 7.876 min
Delta R.T.: -0.003 min
Response: 216786
Conc: 10.57 ng/ml

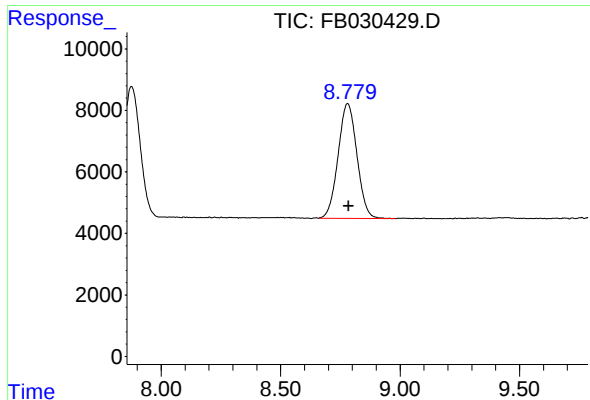

#5 AAA-TFT


R.T.: 8.781 min
Delta R.T.: -0.003 min
Response: 204779
Conc: 17.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S1

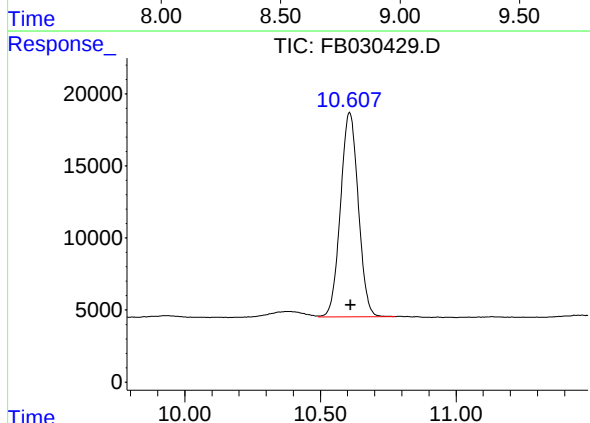


#6 Toluene

R.T.: 10.608 min
Delta R.T.: -0.004 min
Response: 646668
Conc: 32.03 ng/ml

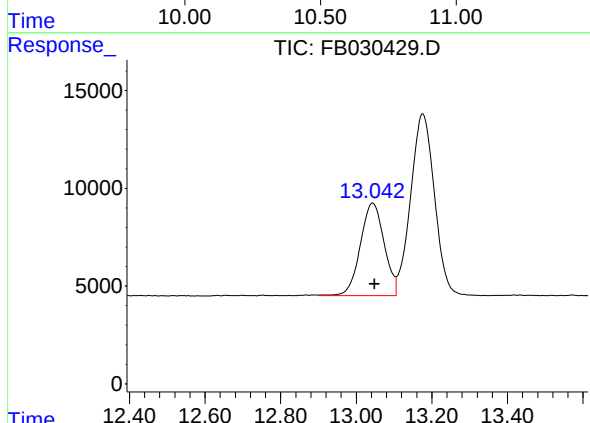


#7 Ethylbenzene

R.T.: 13.044 min
Delta R.T.: -0.006 min
Response: 207130
Conc: 10.38 ng/ml

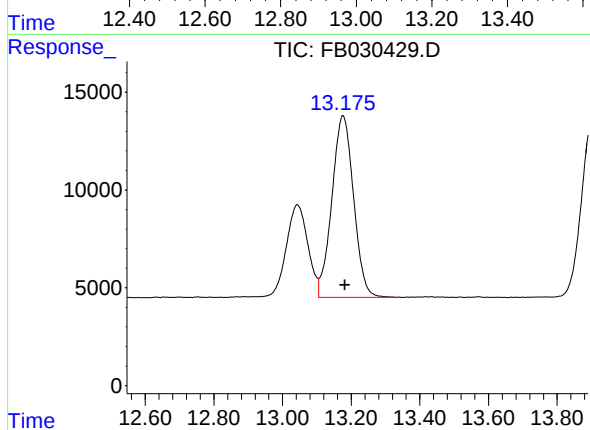

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: -0.005 min
Response: 408167
Conc: 20.71 ng/ml

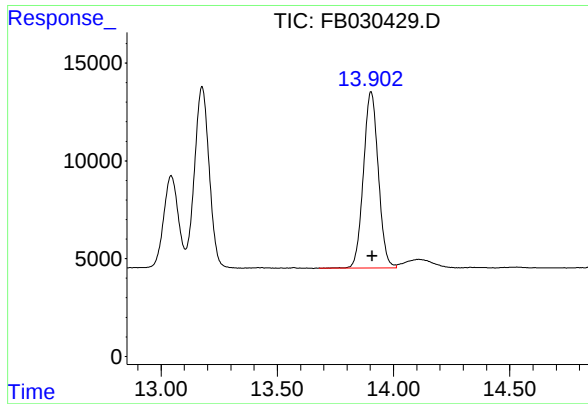

#9 O-Xylene

R.T.: 13.903 min
Delta R.T.: -0.005 min
Response: 400669
Conc: 20.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S1

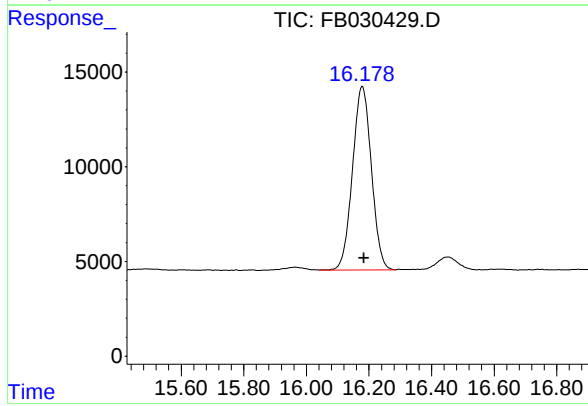

#10 1,2,4-Trimethylbenzene

R.T.: 16.179 min
Delta R.T.: -0.004 min
Response: 405774
Conc: 19.64 ng/ml