

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
Data File : FB031105.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2024 14:52
Operator : YP/AJ
Sample : VBF1106S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 01:52:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	544259	19.717 ng/ml
Target Compounds			
6) t Toluene	10.625	15019	0.301 ng/ml
7) t Ethylbenzene	13.059	7338	0.164 ng/ml
8) t m-Xylene	13.188	21424	0.440 ng/ml
9) t O-Xylene	13.916	14206	0.312 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	33346	0.896 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
Data File : FB031105.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2024 14:52
Operator : YP/AJ
Sample : VBF1106S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 01:52:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

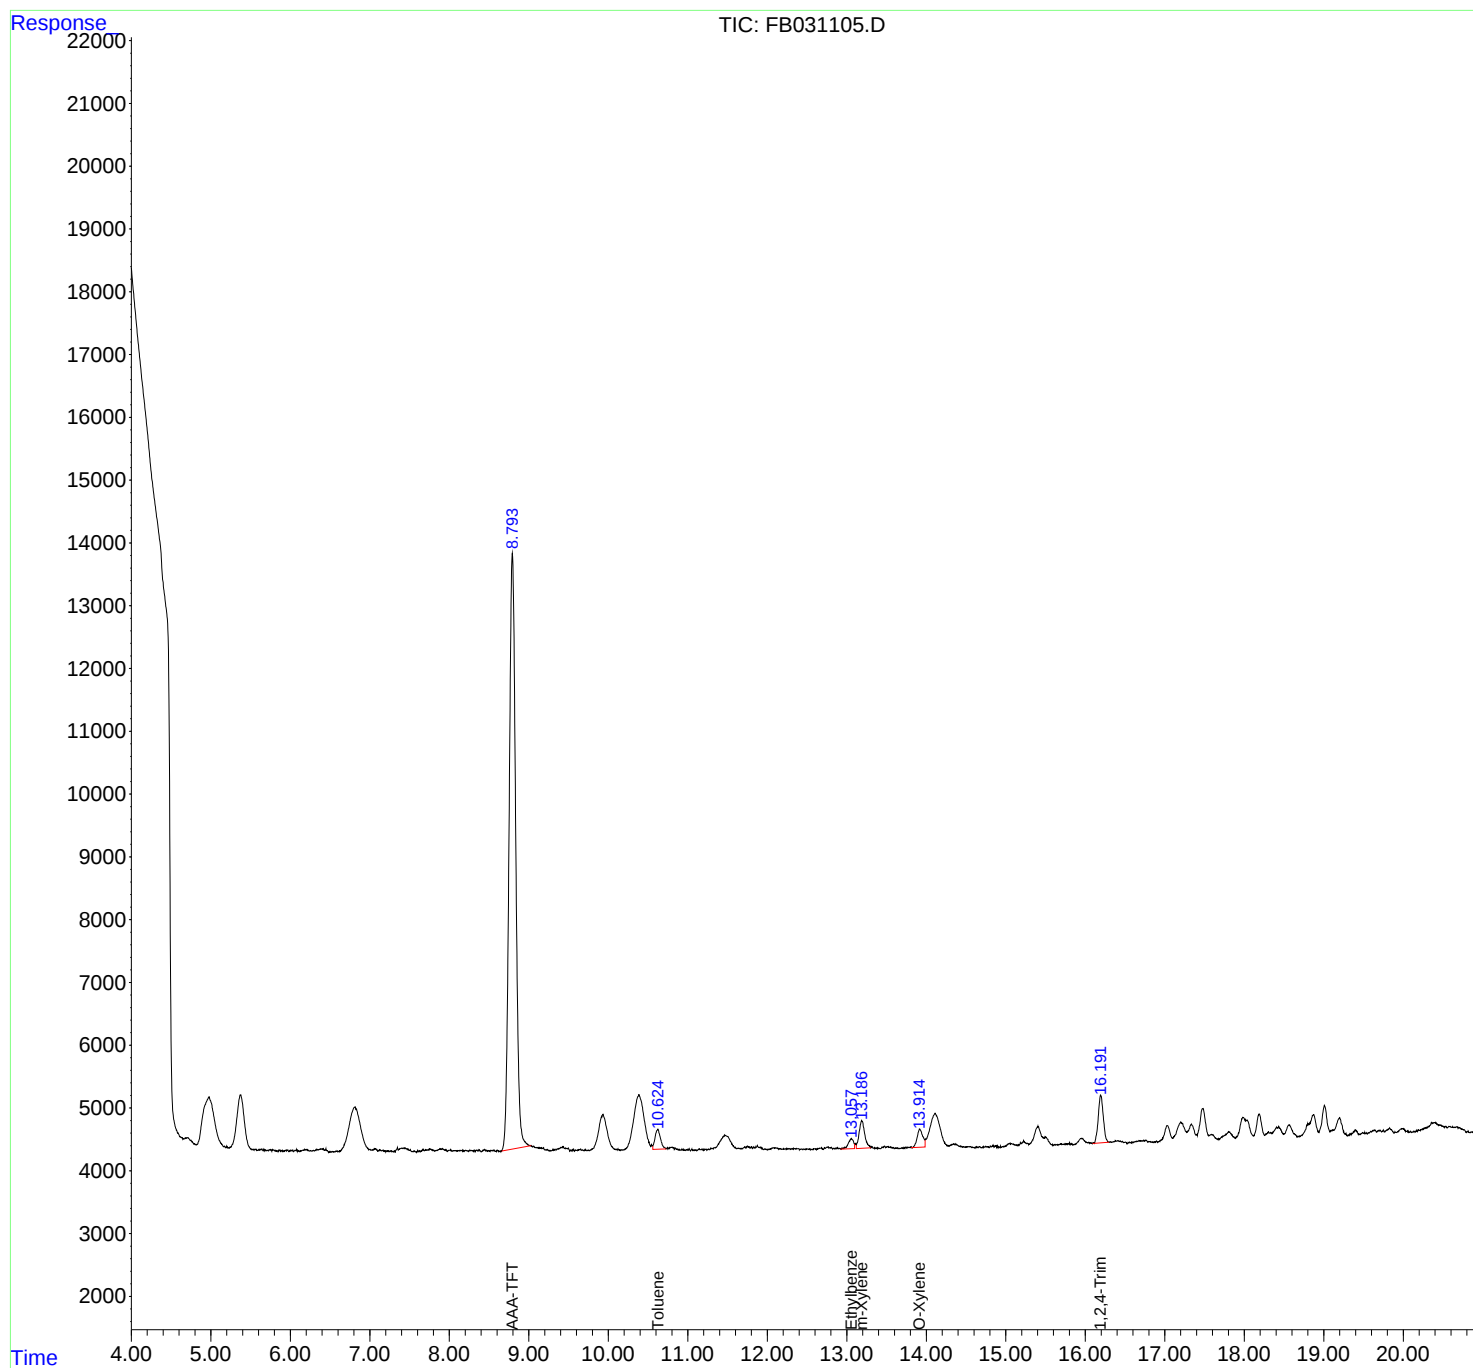


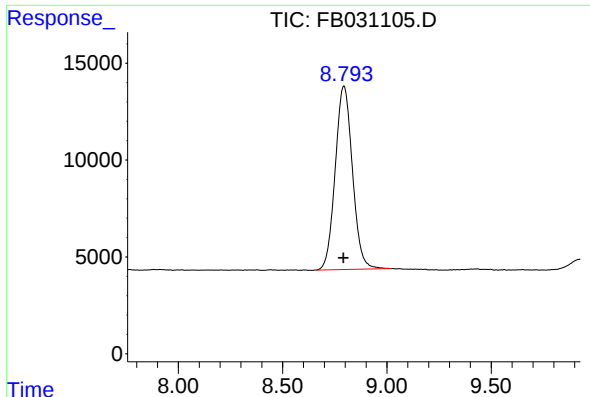

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 544259
Conc: 19.72 ng/ml

Instrument :
FID_B
ClientSampleId :

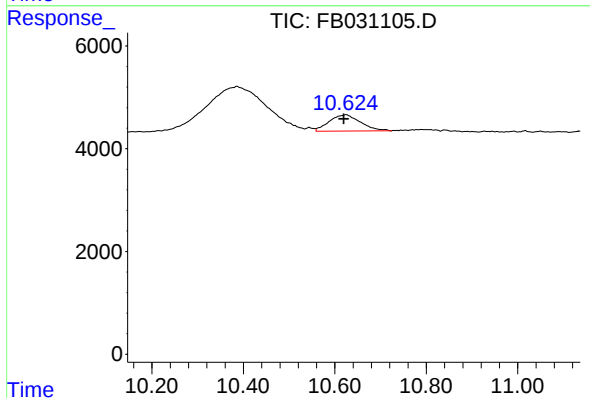


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 15019
Conc: 0.30 ng/ml

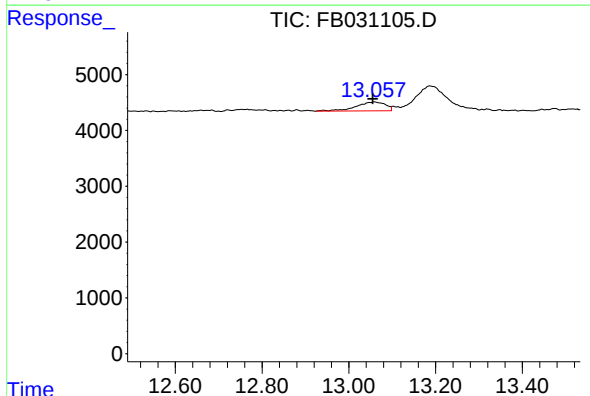


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 7338
Conc: 0.16 ng/ml

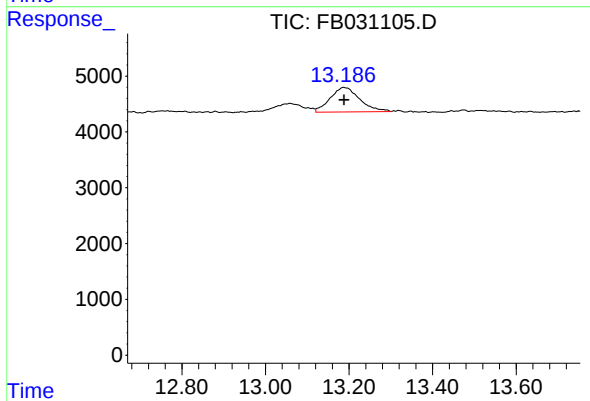

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 21424
Conc: 0.44 ng/ml

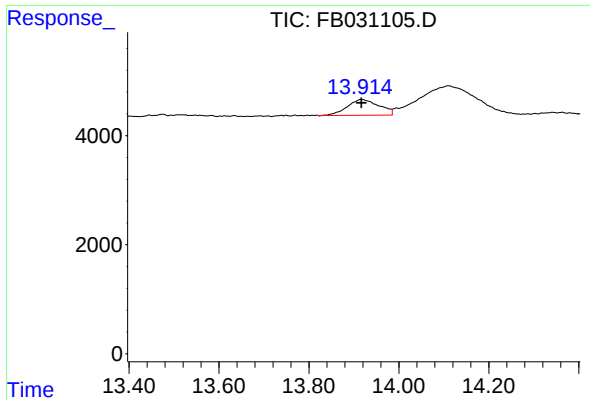

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.001 min
Response: 14206
Conc: 0.31 ng/ml

Instrument :
FID_B
ClientSampleId :

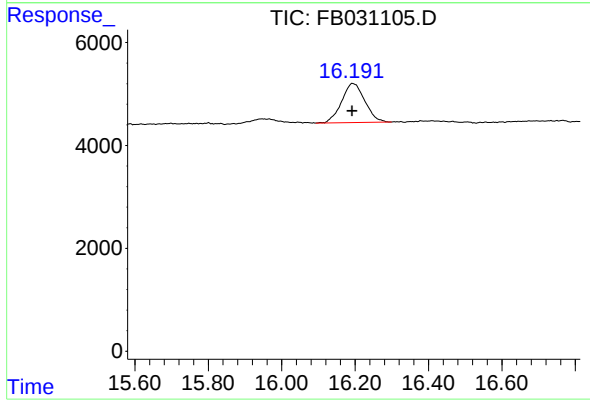

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 33346
Conc: 0.90 ng/ml