

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
 Data File : FB031122.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2024 23:23
 Operator : YP/AJ
 Sample : P4721-13 50X
 Misc : 8.03G/5.00 ML MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 07 01:53:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	624865	22.638 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	90941	2.316 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	319633	6.824 ng/ml
3) t n-Heptane	7.750	86851	1.916 ng/ml
6) t Toluene	10.672	3568	0.071 ng/ml
7) t Ethylbenzene	13.051	100278	2.240 ng/ml
8) t m-Xylene	13.191	147846	3.040 ng/ml
9) t O-Xylene	13.922	22403	0.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	49428	1.328 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
Data File : FB031122.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2024 23:23
Operator : YP/AJ
Sample : P4721-13 50X
Misc : 8.03G/5.00 ML MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 01:53:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

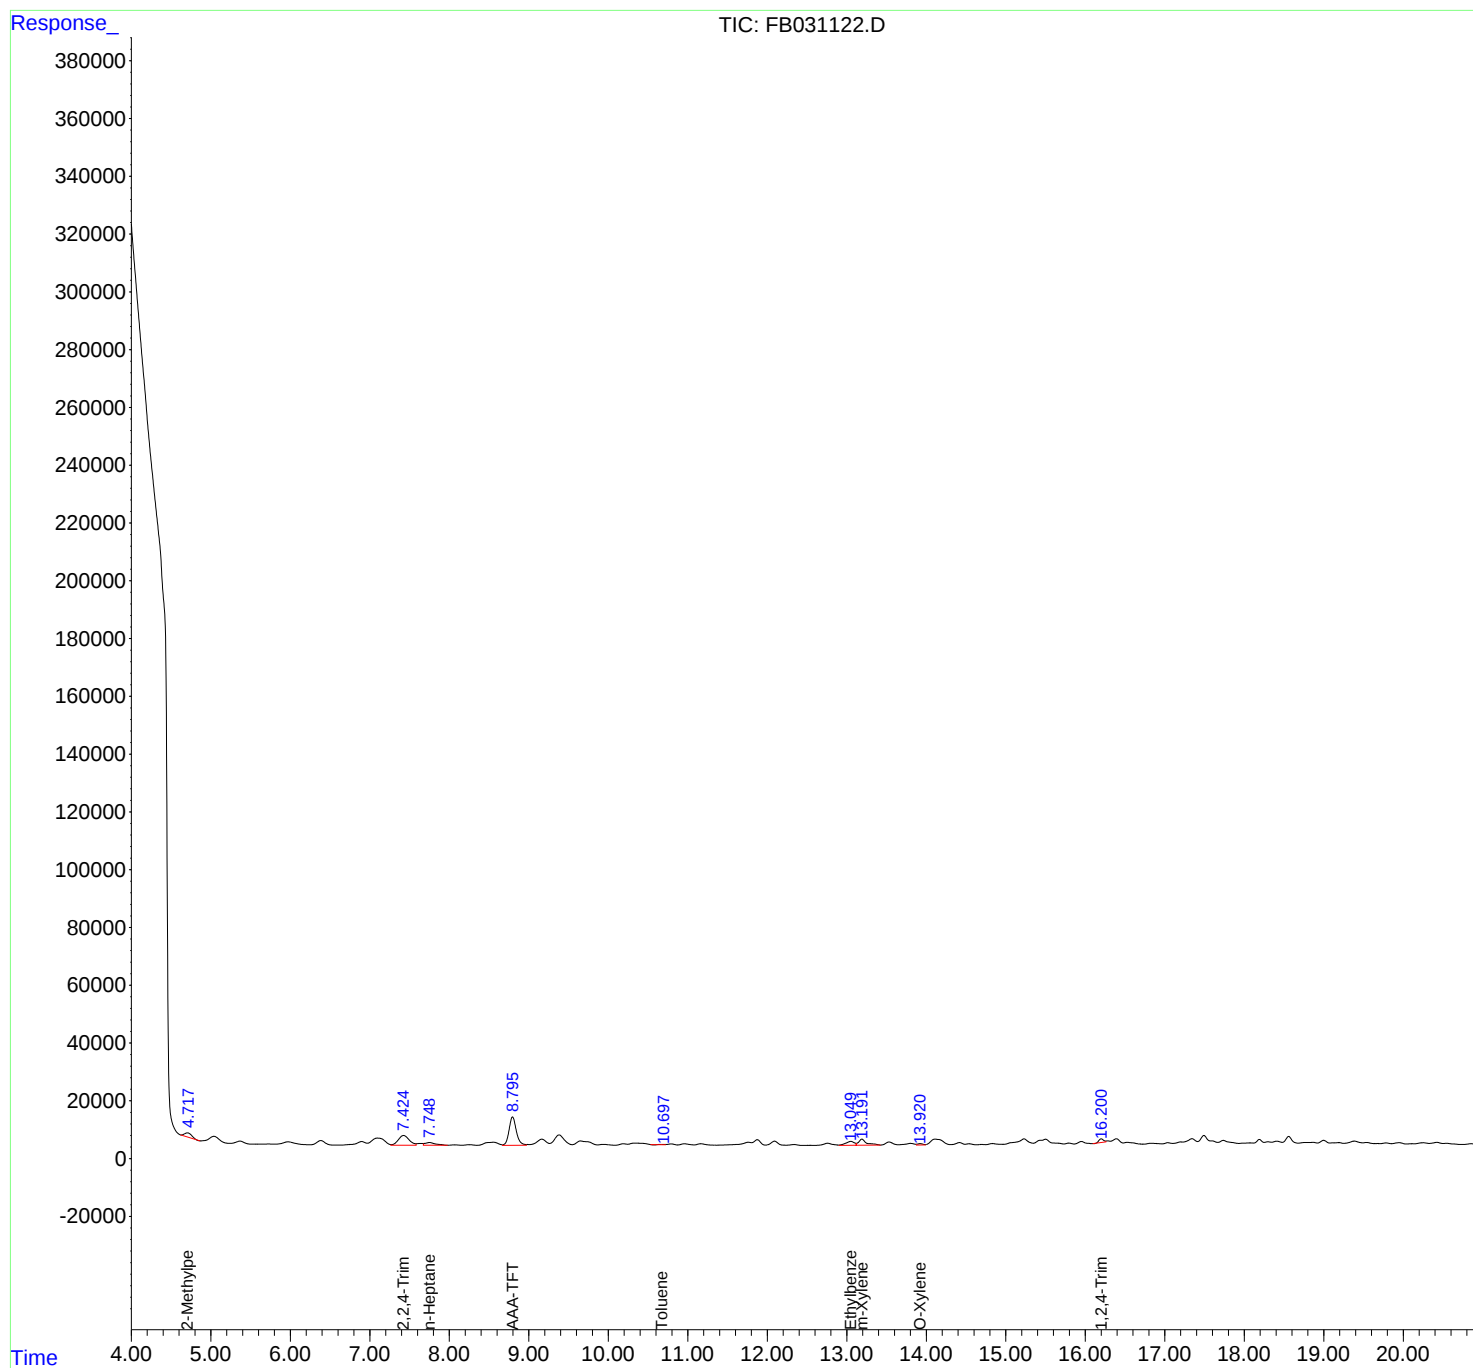


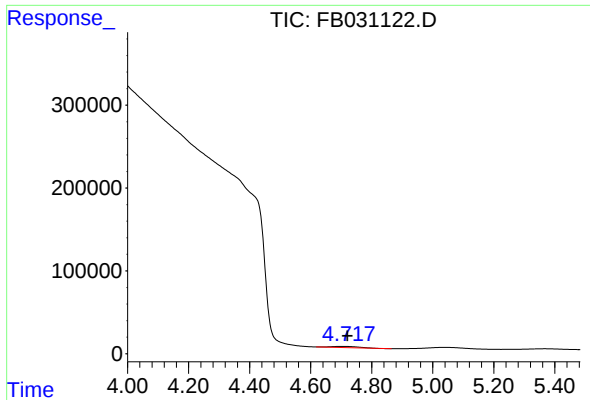

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.015 min
Response: 90941
Conc: 2.32 ng/ml

Instrument :
FID_B
ClientSampleId :

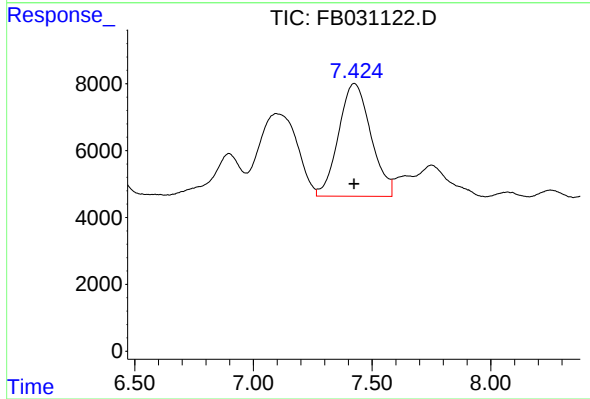


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 319633
Conc: 6.82 ng/ml

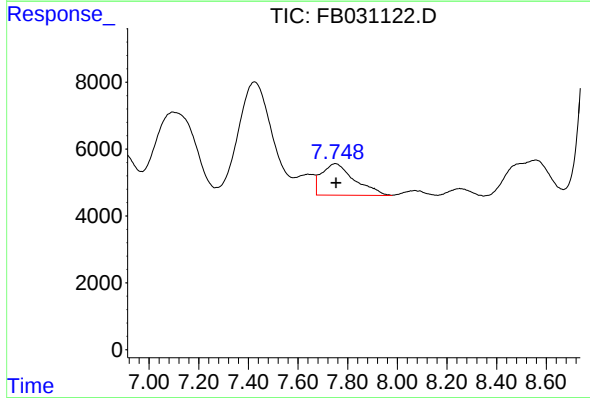


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.003 min
Response: 86851
Conc: 1.92 ng/ml

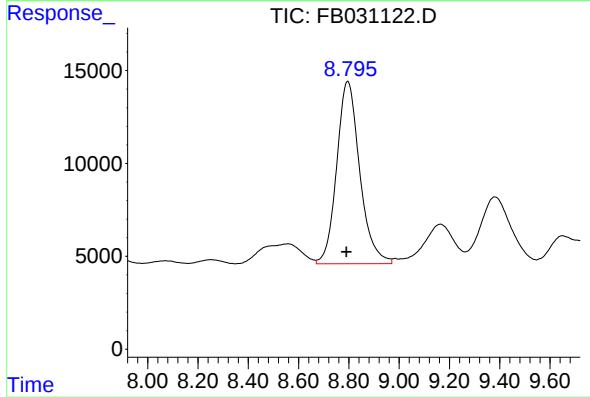

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.006 min
Response: 624865
Conc: 22.64 ng/ml

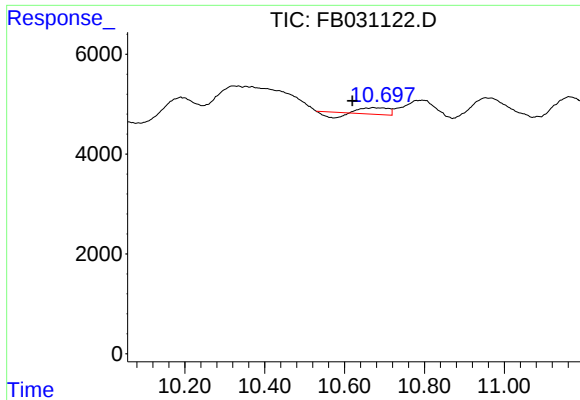

#6 Toluene


R.T.: 10.672 min
Delta R.T.: 0.053 min
Response: 3568
Conc: 0.07 ng/ml

Instrument :
FID_B
ClientSampleId :

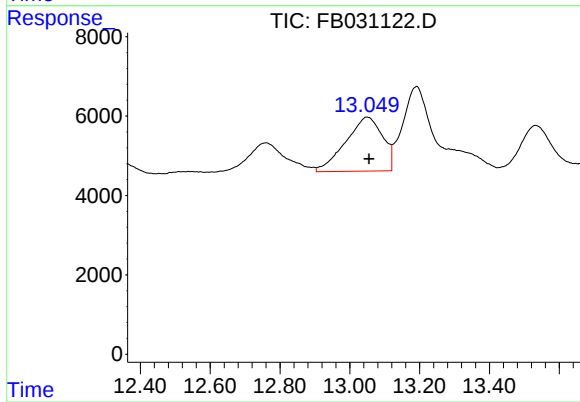


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.004 min
Response: 100278
Conc: 2.24 ng/ml

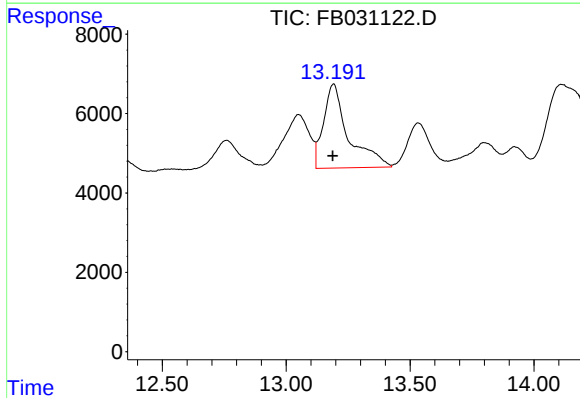


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 147846
Conc: 3.04 ng/ml

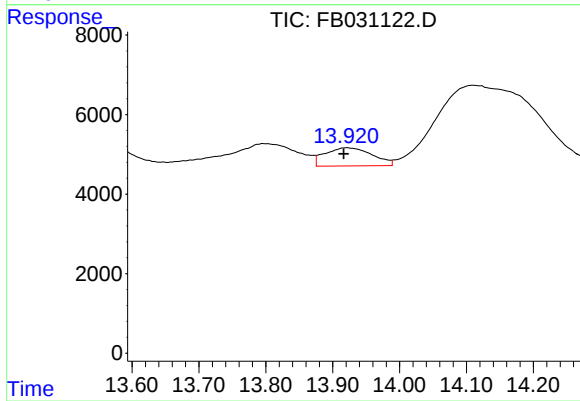

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 22403
Conc: 0.49 ng/ml

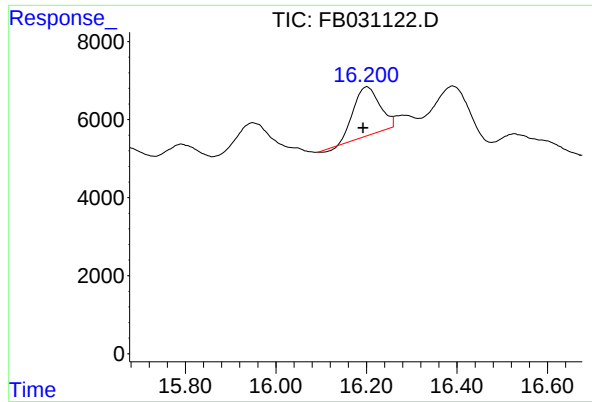

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.009 min
Response: 49428
Conc: 1.33 ng/ml

Instrument :
FID_B
ClientSampleId :