

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
 Data File : FB031125.D
 Signal(s) : FID2B.CH
 Acq On : 6 Nov 2024 00:43
 Operator : YP/AJ
 Sample : BSF1106S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1106S3

Integration File: Calibration.e
 Quant Time: Nov 07 01:54:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	521431	18.890 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	1115973	28.415 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	1332374	28.447 ng/ml
3) t n-Heptane	7.756	423968	9.355 ng/ml
4) t Benzene	7.894	516410	9.661 ng/ml
6) t Toluene	10.623	1417650	28.389 ng/ml
7) t Ethylbenzene	13.059	591169	13.207 ng/ml
8) t m-Xylene	13.192	1628410	33.480 ng/ml
9) t O-Xylene	13.921	998564	21.907 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	1783014	47.919 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110624\
Data File : FB031125.D
Signal(s) : FID2B.CH
Acq On : 6 Nov 2024 00:43
Operator : YP/AJ
Sample : BSF1106S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1106S3

Integration File: Calibration.e
Quant Time: Nov 07 01:54:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

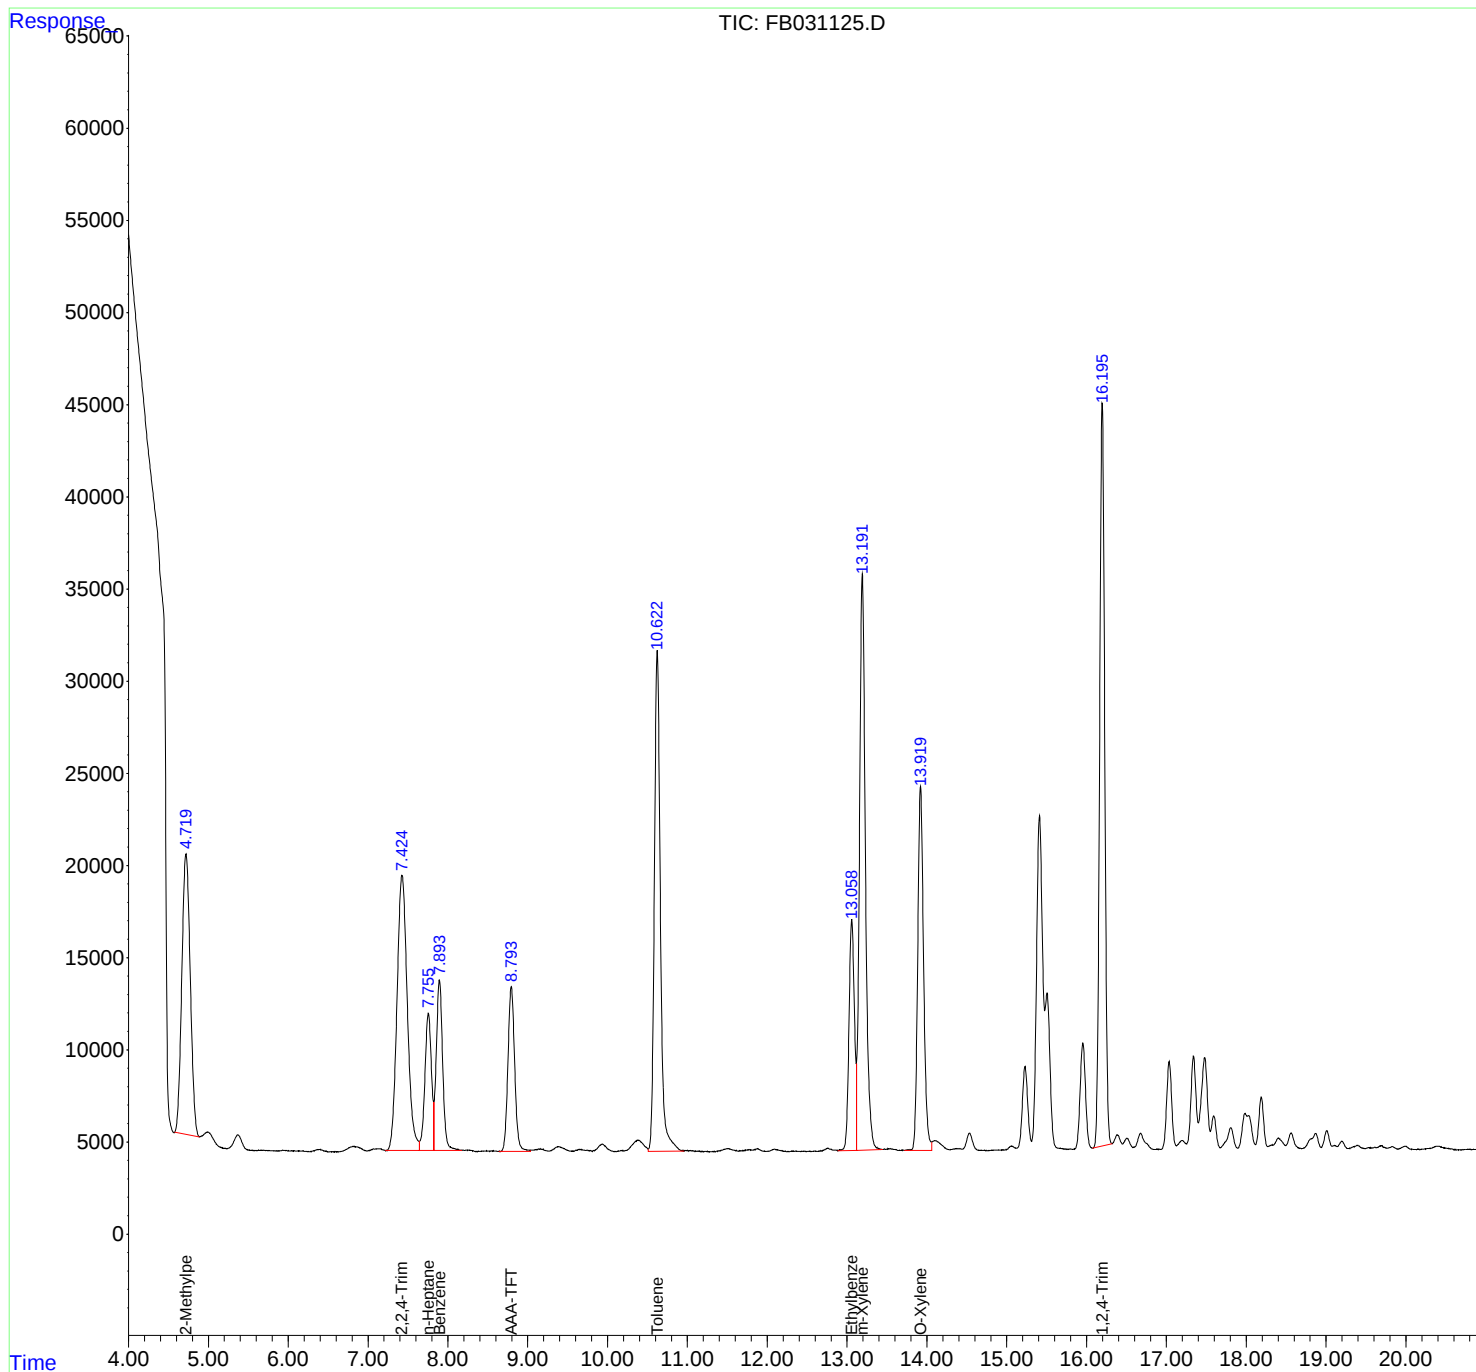


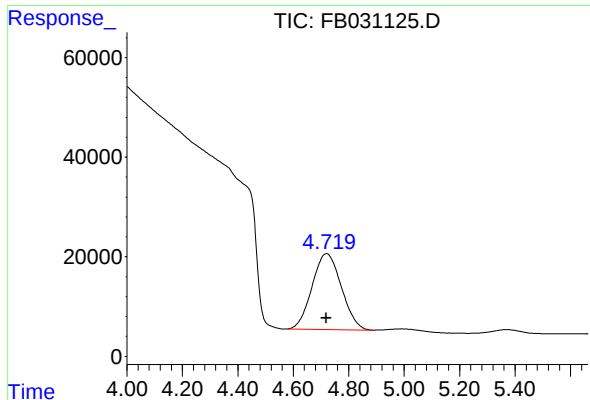

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: 0.000 min
Response: 1115973
Conc: 28.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S3

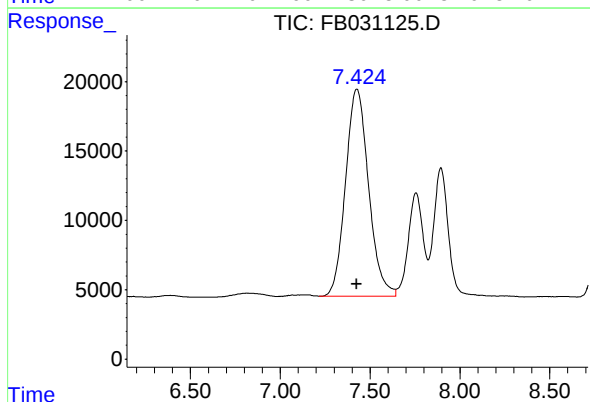


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.001 min
Response: 1332374
Conc: 28.45 ng/ml

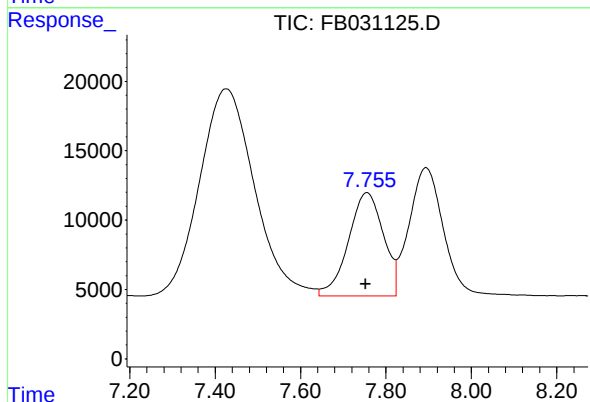


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.003 min
Response: 423968
Conc: 9.35 ng/ml

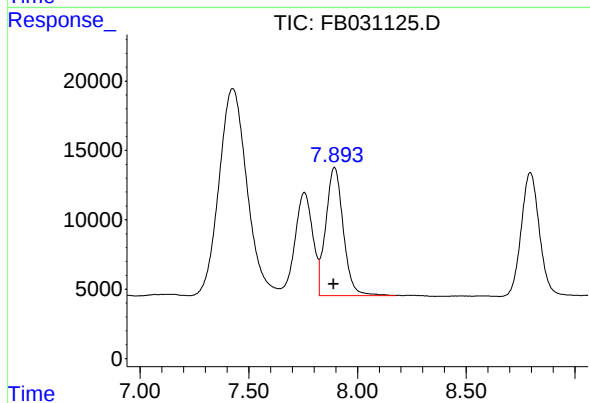

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.003 min
Response: 516410
Conc: 9.66 ng/ml

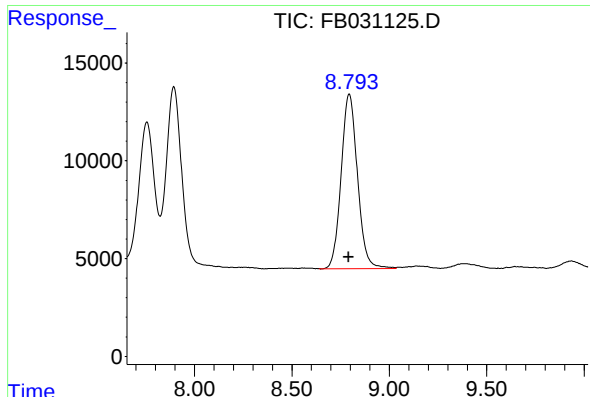

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.004 min
Response: 521431
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S3

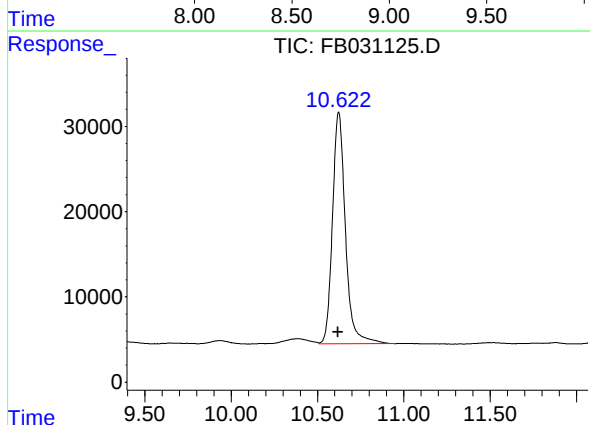


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1417650
Conc: 28.39 ng/ml

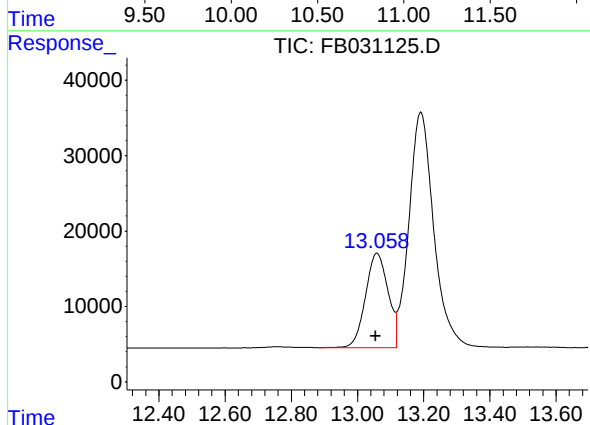


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 591169
Conc: 13.21 ng/ml

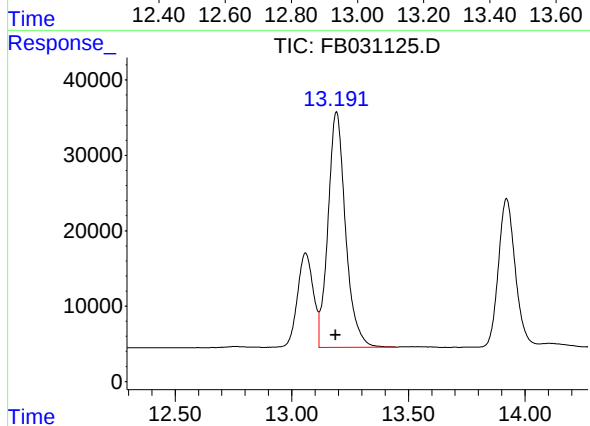

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 1628410
Conc: 33.48 ng/ml

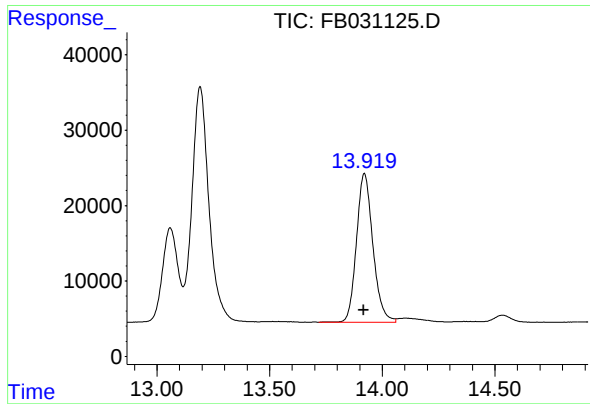

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.004 min
Response: 998564
Conc: 21.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1106S3

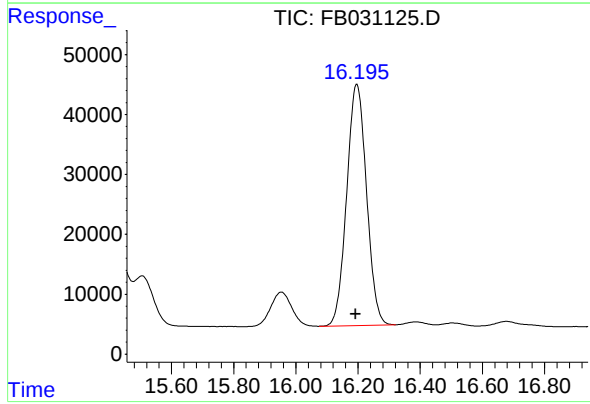

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.004 min
Response: 1783014
Conc: 47.92 ng/ml