

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110718\
 Data File : FB018597.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2018 15:13
 Operator : MJ/SJ
 Sample : BSF1107S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 09 07:18:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	154415	17.928 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	405667	26.524 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	433097	29.310 ng/ml
3) t n-Heptane	8.063	134103	9.463 ng/ml
4) t Benzene	8.203	174956	9.392 ng/ml
6) t Toluene	10.958	446968	29.327 ng/ml
7) t Ethylbenzene	13.407	141705	8.932 ng/ml
8) t m-Xylene	13.540	294062	17.673 ng/ml
9) t O-Xylene	14.272	315429	17.691 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	379632	18.661 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110718\
Data File : FB018597.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2018 15:13
Operator : MJ/SJ
Sample : BSF1107S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 09 07:18:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

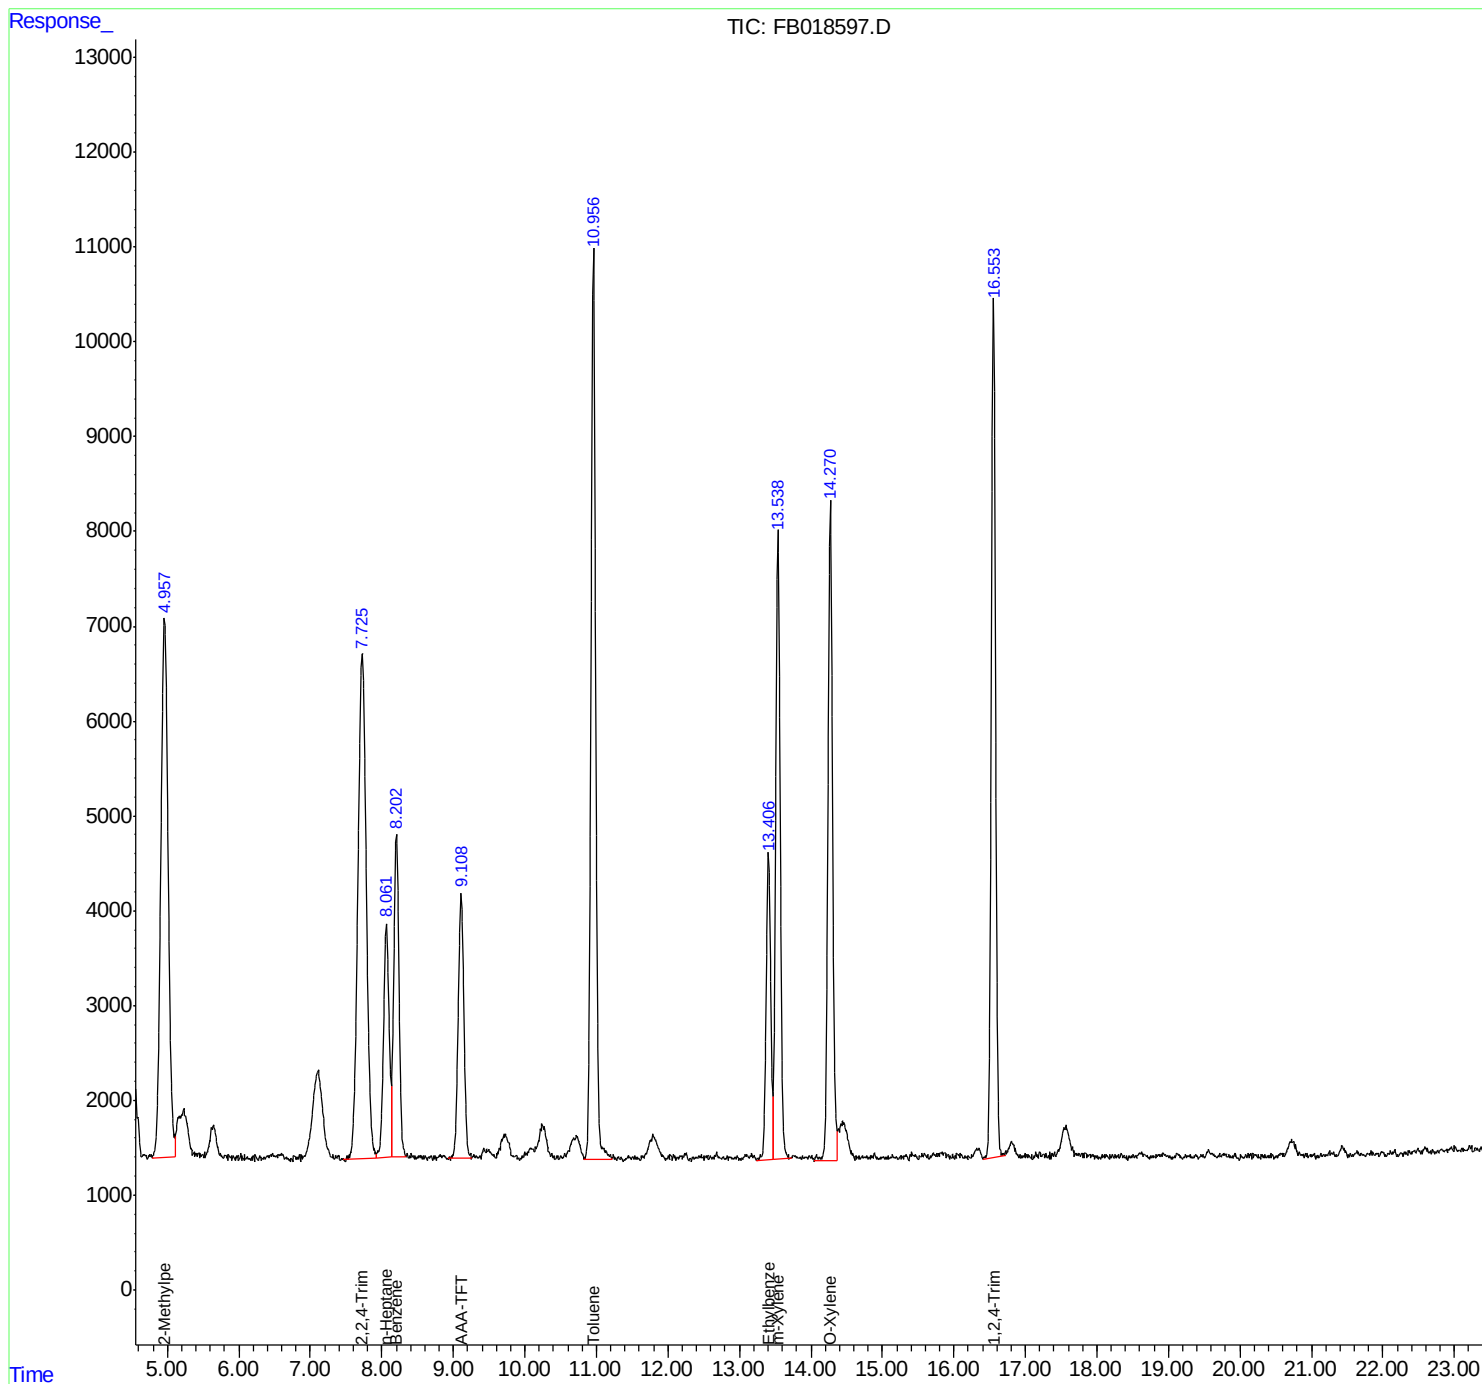

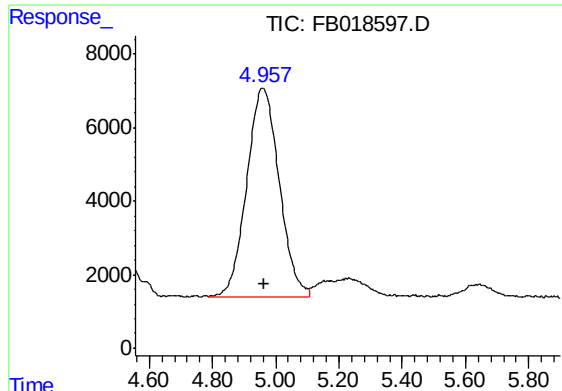


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 405667
Conc: 26.52 ng/ml

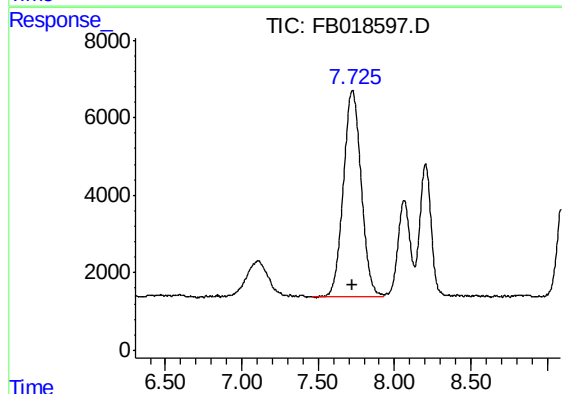


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.003 min
Response: 433097
Conc: 29.31 ng/ml

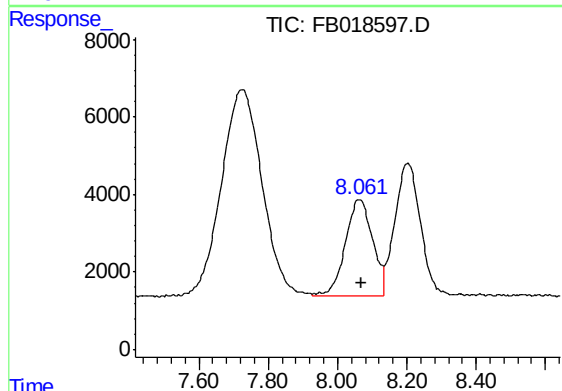


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.004 min
Response: 134103
Conc: 9.46 ng/ml

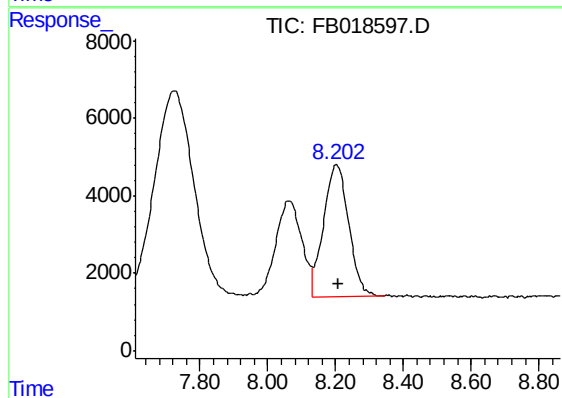


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 174956
Conc: 9.39 ng/ml

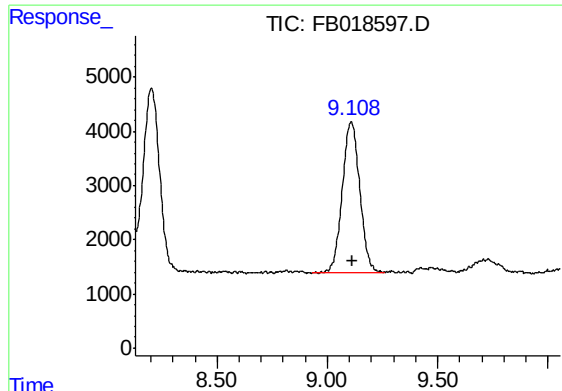


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.004 min
Response: 154415
Conc: 17.93 ng/ml

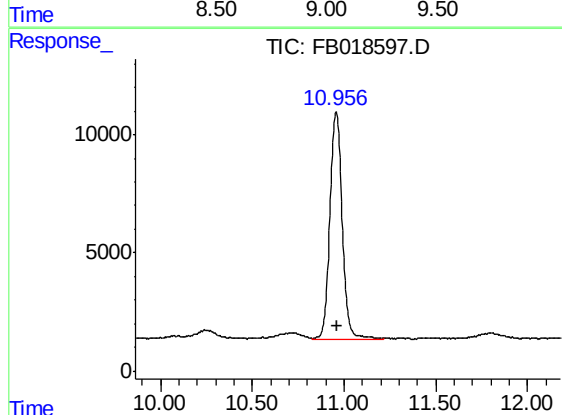


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.004 min
Response: 446968
Conc: 29.33 ng/ml

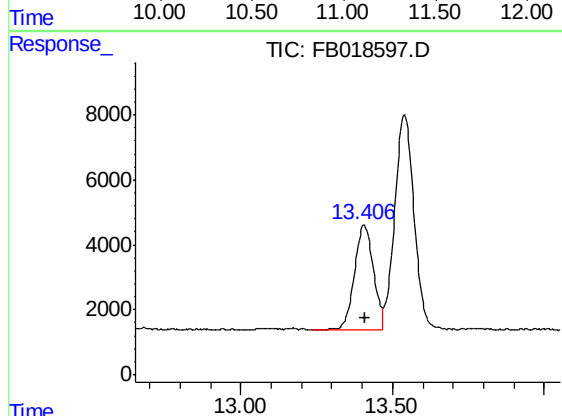


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.005 min
Response: 141705
Conc: 8.93 ng/ml

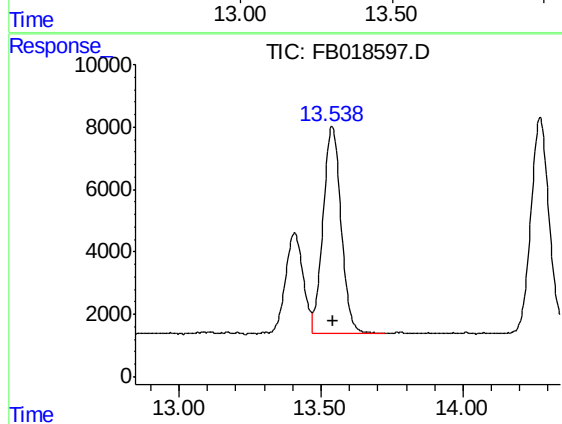


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.005 min
Response: 294062
Conc: 17.67 ng/ml

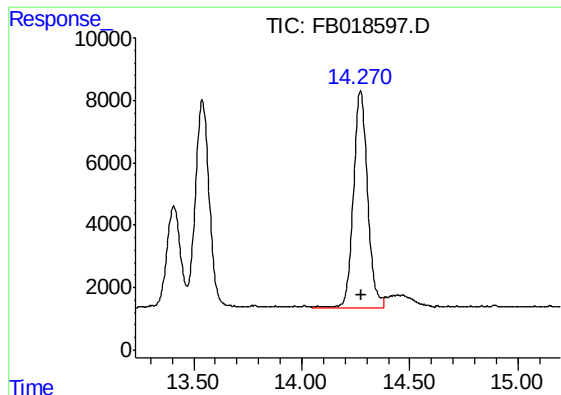

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.004 min
Response: 315429
Conc: 17.69 ng/ml

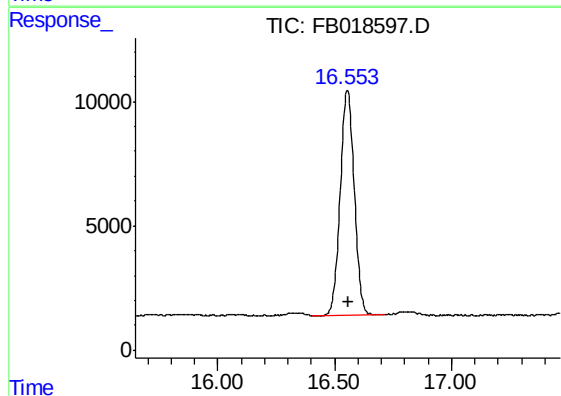

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.005 min
Response: 379632
Conc: 18.66 ng/ml