

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022914.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 10:49
 Operator : DD/AJ
 Sample : VBF1107S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF1107S1

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	419266	18.624 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	4231	0.132 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	1213	0.034 ng/ml
6) t Toluene	10.624	7789	0.181 ng/ml
7) t Ethylbenzene	13.062	1471	0.037 ng/ml
8) t m-Xylene	13.194	4722	0.125 ng/ml
9) t O-Xylene	13.937	1347	0.038 ng/ml
10) t 1,2,4-Trimethylbenzene	16.218	2270	0.080 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022914.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 10:49
Operator : DD/AJ
Sample : VBF1107S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1107S1

Integration File: Calibration.e
Quant Time: Nov 07 15:19:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

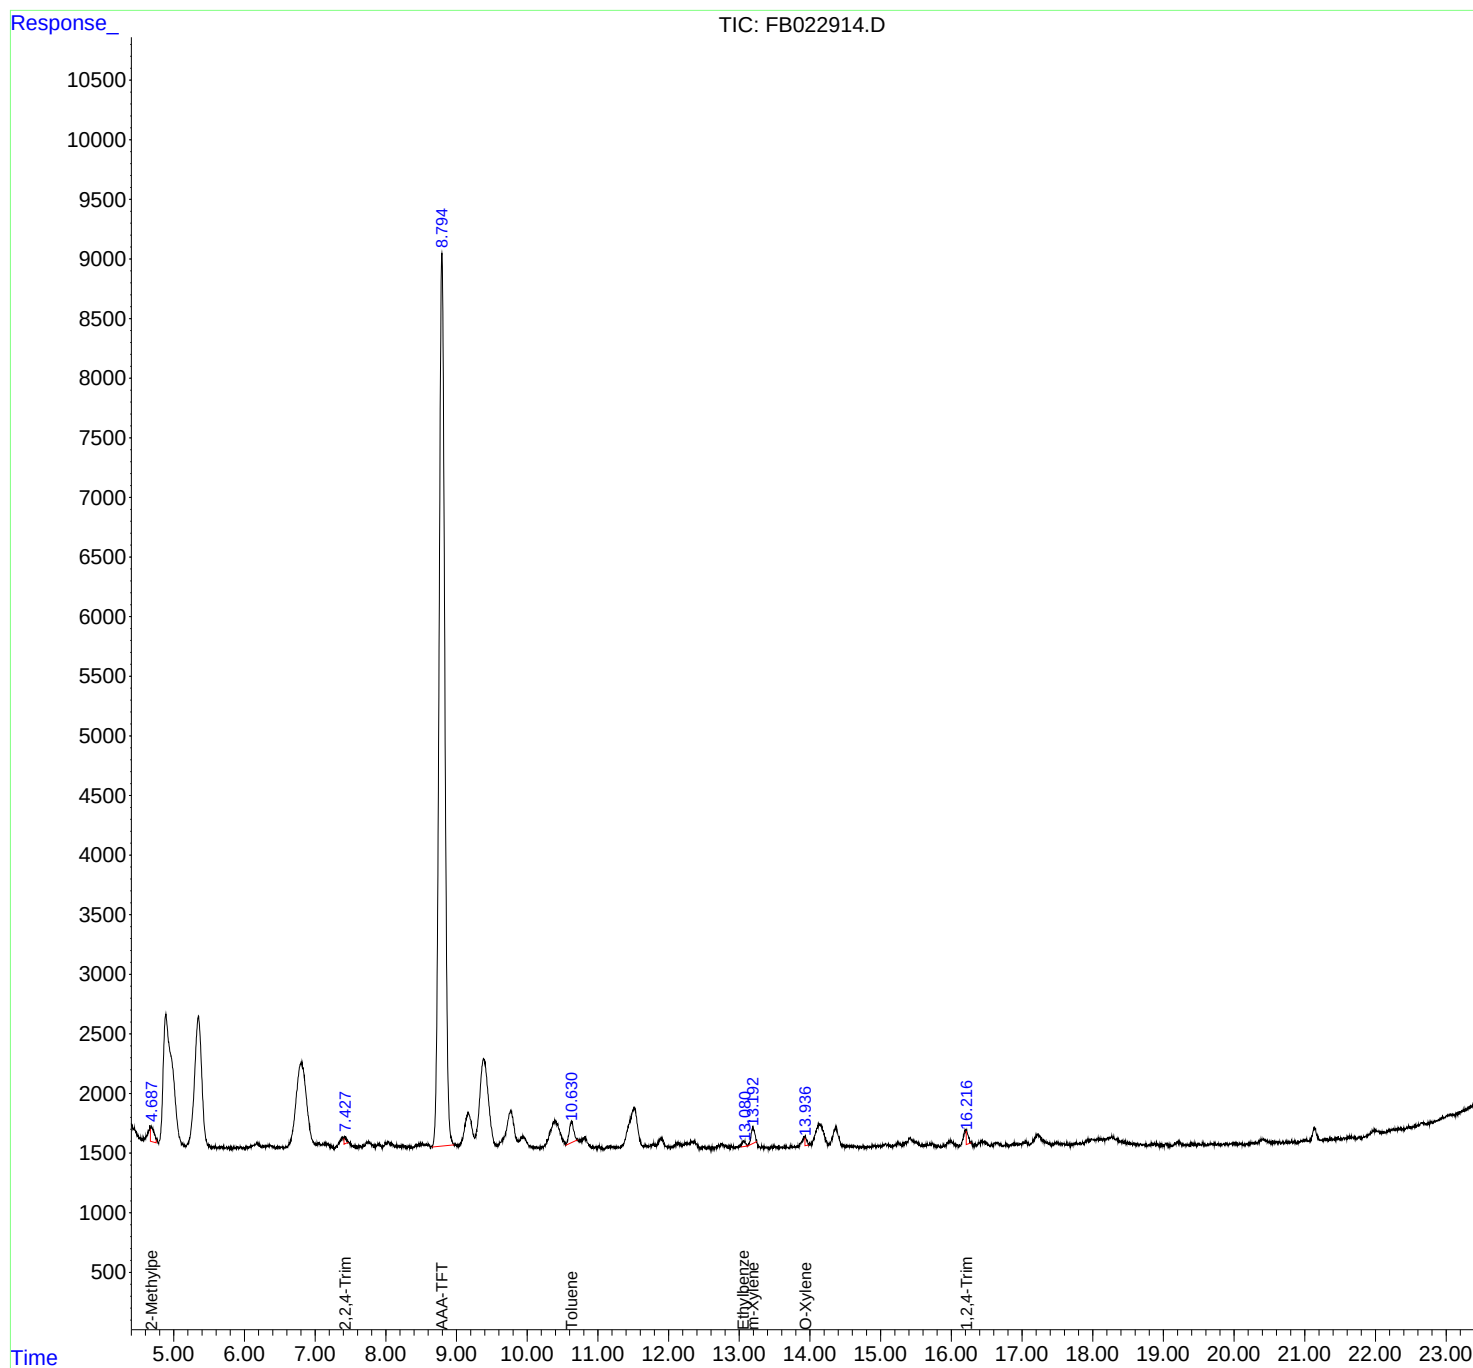


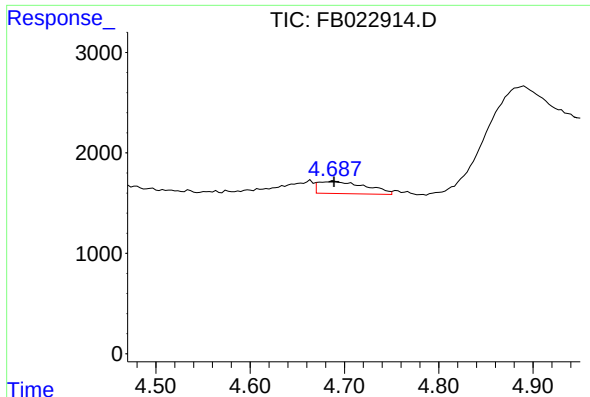

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 4231
Conc: 0.13 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1107S1

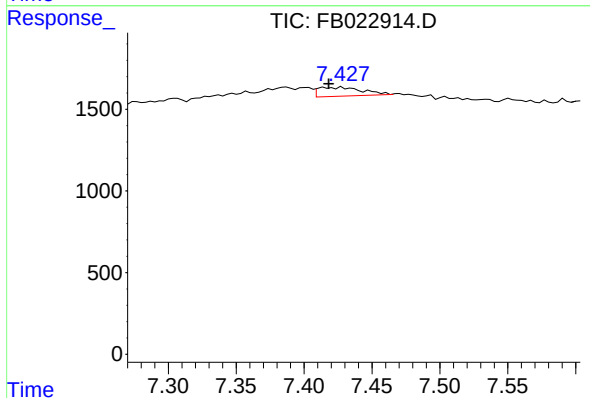


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.010 min
Response: 1213
Conc: 0.03 ng/ml

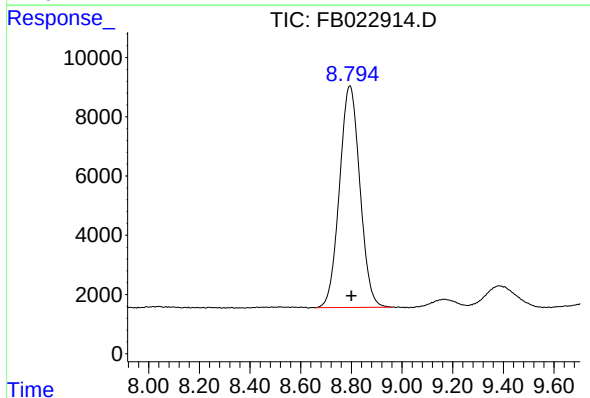


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 419266
Conc: 18.62 ng/ml

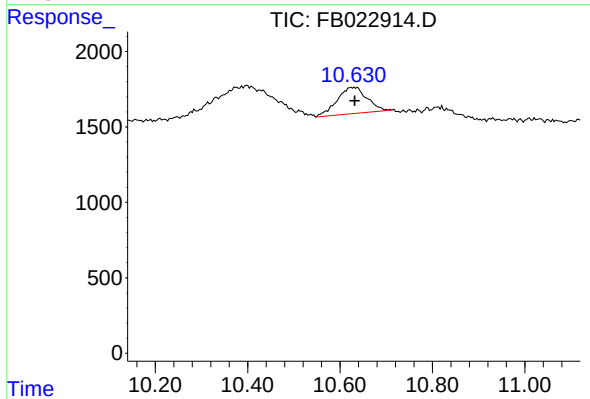

#6 Toluene


R.T.: 10.624 min
Delta R.T.: -0.008 min
Response: 7789
Conc: 0.18 ng/ml

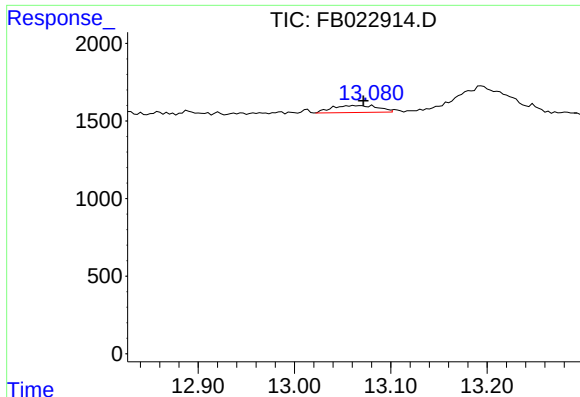

#7 Ethylbenzene


R.T.: 13.062 min
Delta R.T.: -0.010 min
Response: 1471
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1107S1

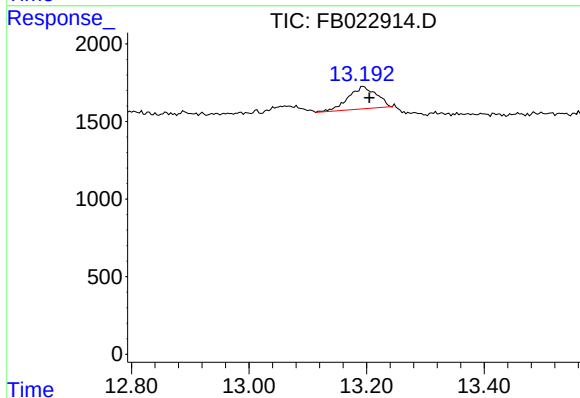


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: -0.011 min
Response: 4722
Conc: 0.13 ng/ml

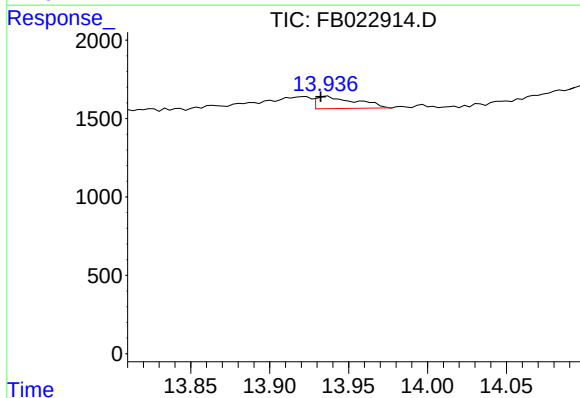

#9 o-Xylene

R.T.: 13.937 min
Delta R.T.: 0.005 min
Response: 1347
Conc: 0.04 ng/ml

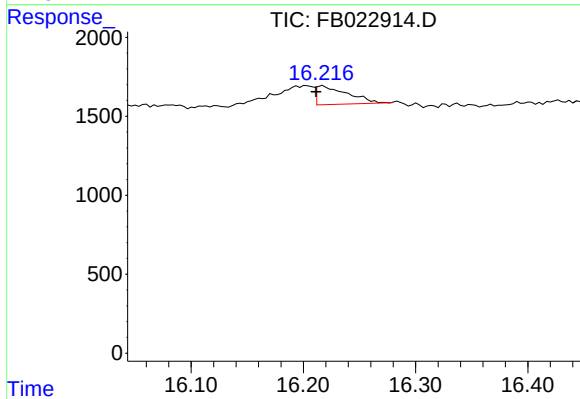

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.006 min
Response: 2270
Conc: 0.08 ng/ml