

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022916.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 11:48
 Operator : DD/AJ
 Sample : K5675-07
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TR-04-110619

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	455529	20.235 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.682	322	0.010 ng/ml
6) t Toluene	10.628	5205	0.121 ng/ml
8) t m-Xylene	13.200	580	0.015 ng/ml
9) t O-Xylene	13.929	394	0.011 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	1213	0.043 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022916.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 11:48
Operator : DD/AJ
Sample : K5675-07
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-04-110619

Integration File: Calibration.e
Quant Time: Nov 07 15:19:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

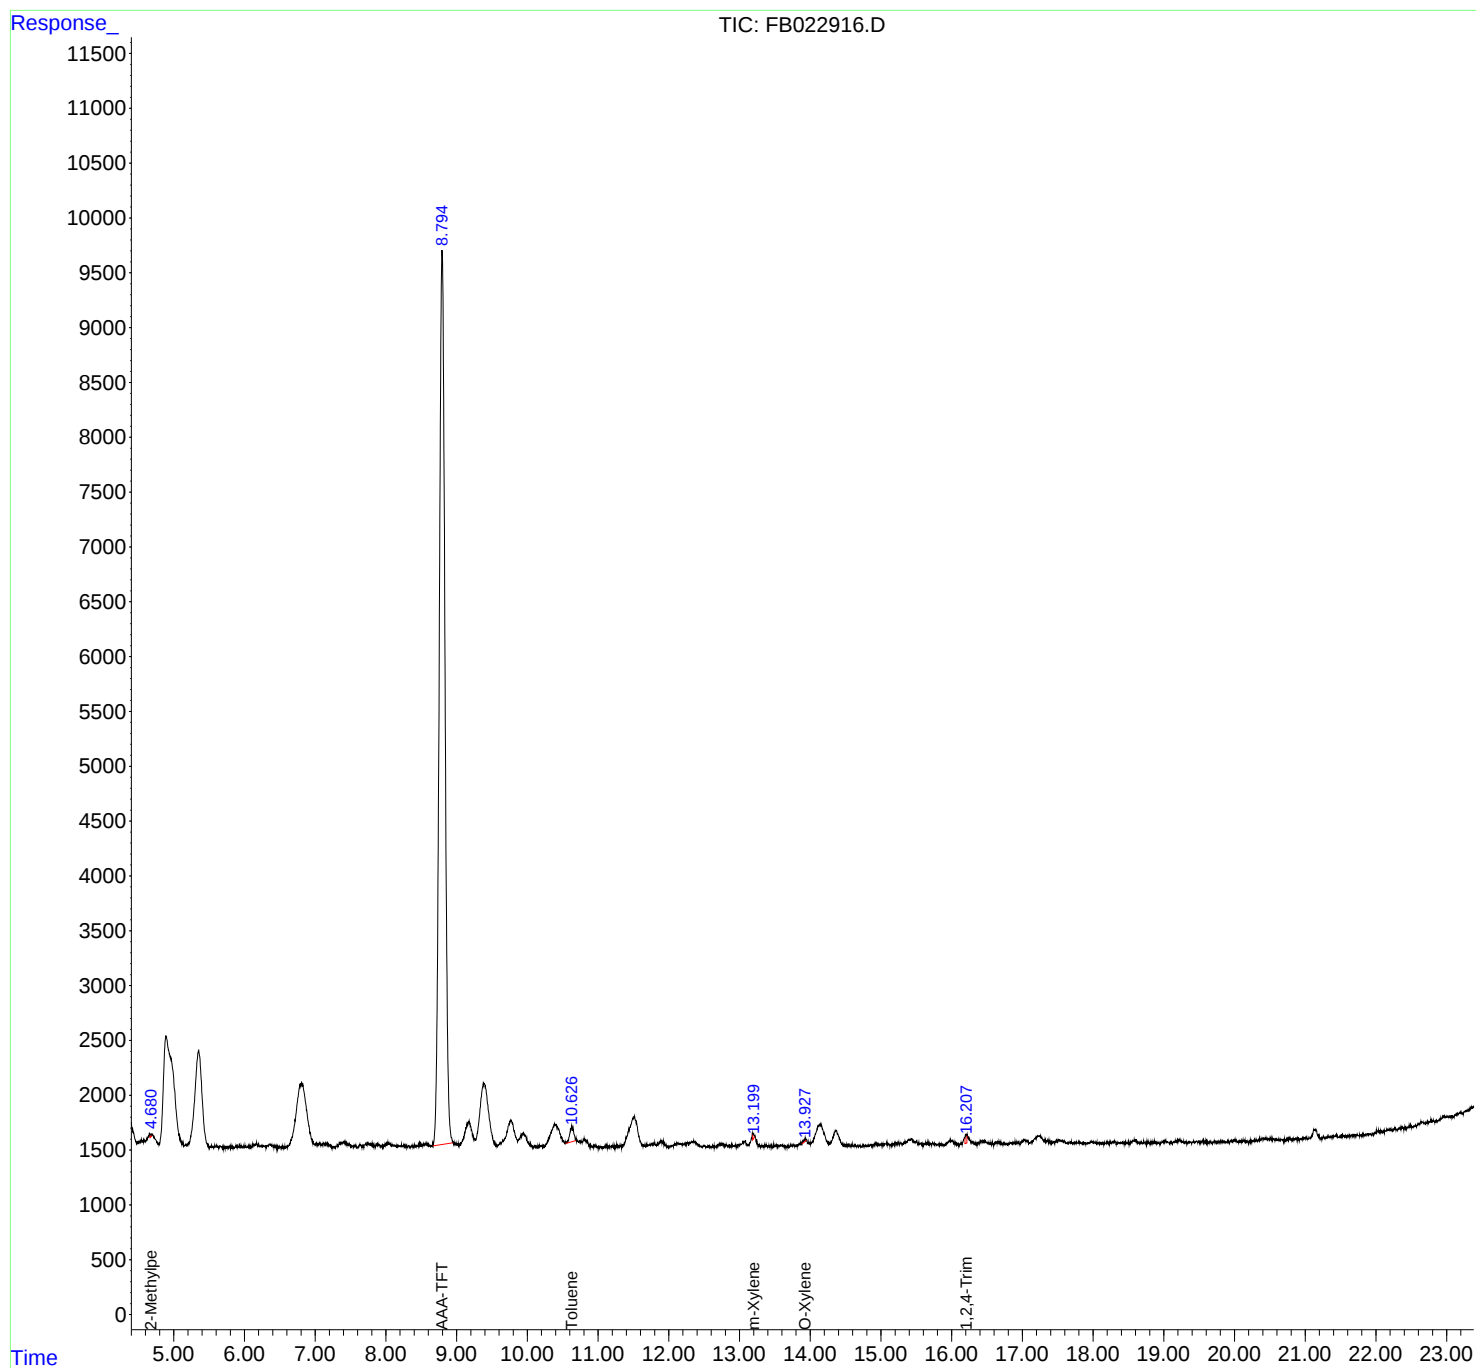


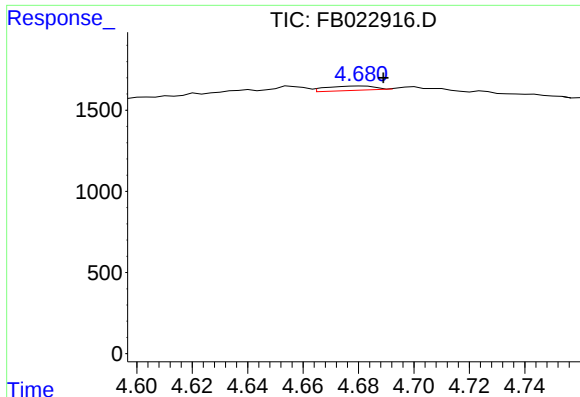

#1 2-Methylpentane


R.T.: 4.682 min
Delta R.T.: -0.007 min
Response: 322
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-110619

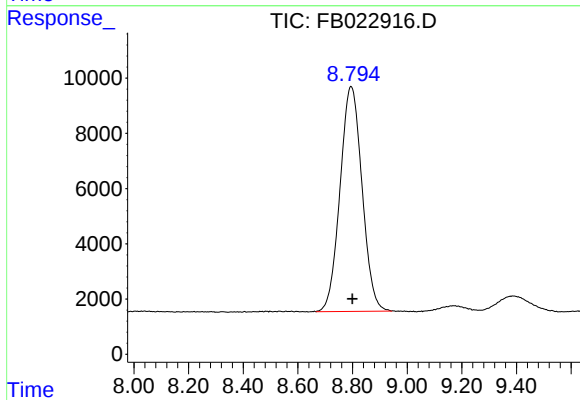


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 455529
Conc: 20.24 ng/ml

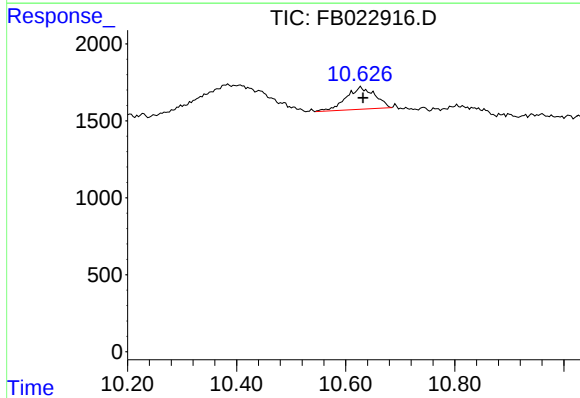


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 5205
Conc: 0.12 ng/ml

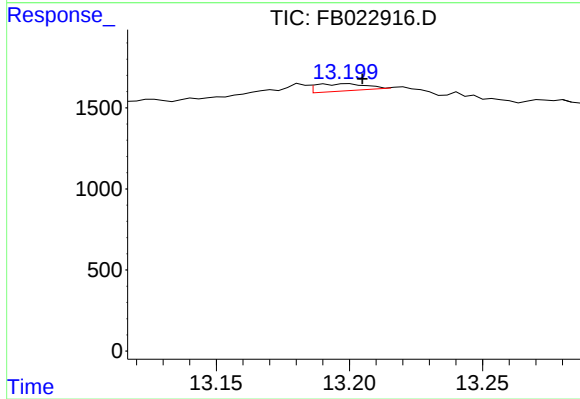

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 580
Conc: 0.02 ng/ml

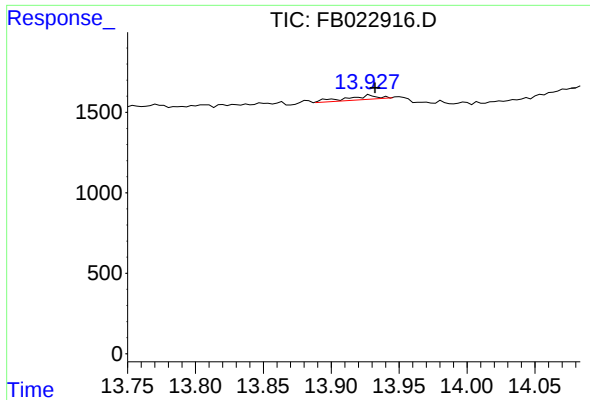

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 394
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-110619

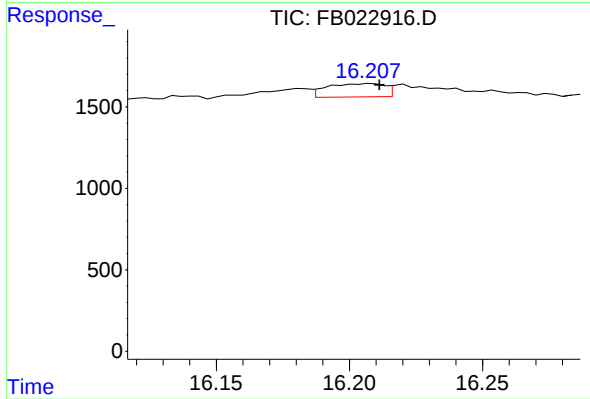

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 1213
Conc: 0.04 ng/ml