

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022917.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 12:18
Operator : DD/AJ
Sample : K5668-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-110619

Integration File: Calibration.e
Quant Time: Nov 07 15:19:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	453860	20.161 ng/ml
Target Compounds			
6) t Toluene	10.628	43615	1.012 ng/ml
7) t Ethylbenzene	13.057	1577	0.040 ng/ml
8) t m-Xylene	13.196	5093	0.135 ng/ml
9) t O-Xylene	13.910	684	0.019 ng/ml
10) t 1,2,4-Trimethylbenzene	16.218	293	0.010 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022917.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 12:18
Operator : DD/AJ
Sample : K5668-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-110619

Integration File: Calibration.e
Quant Time: Nov 07 15:19:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

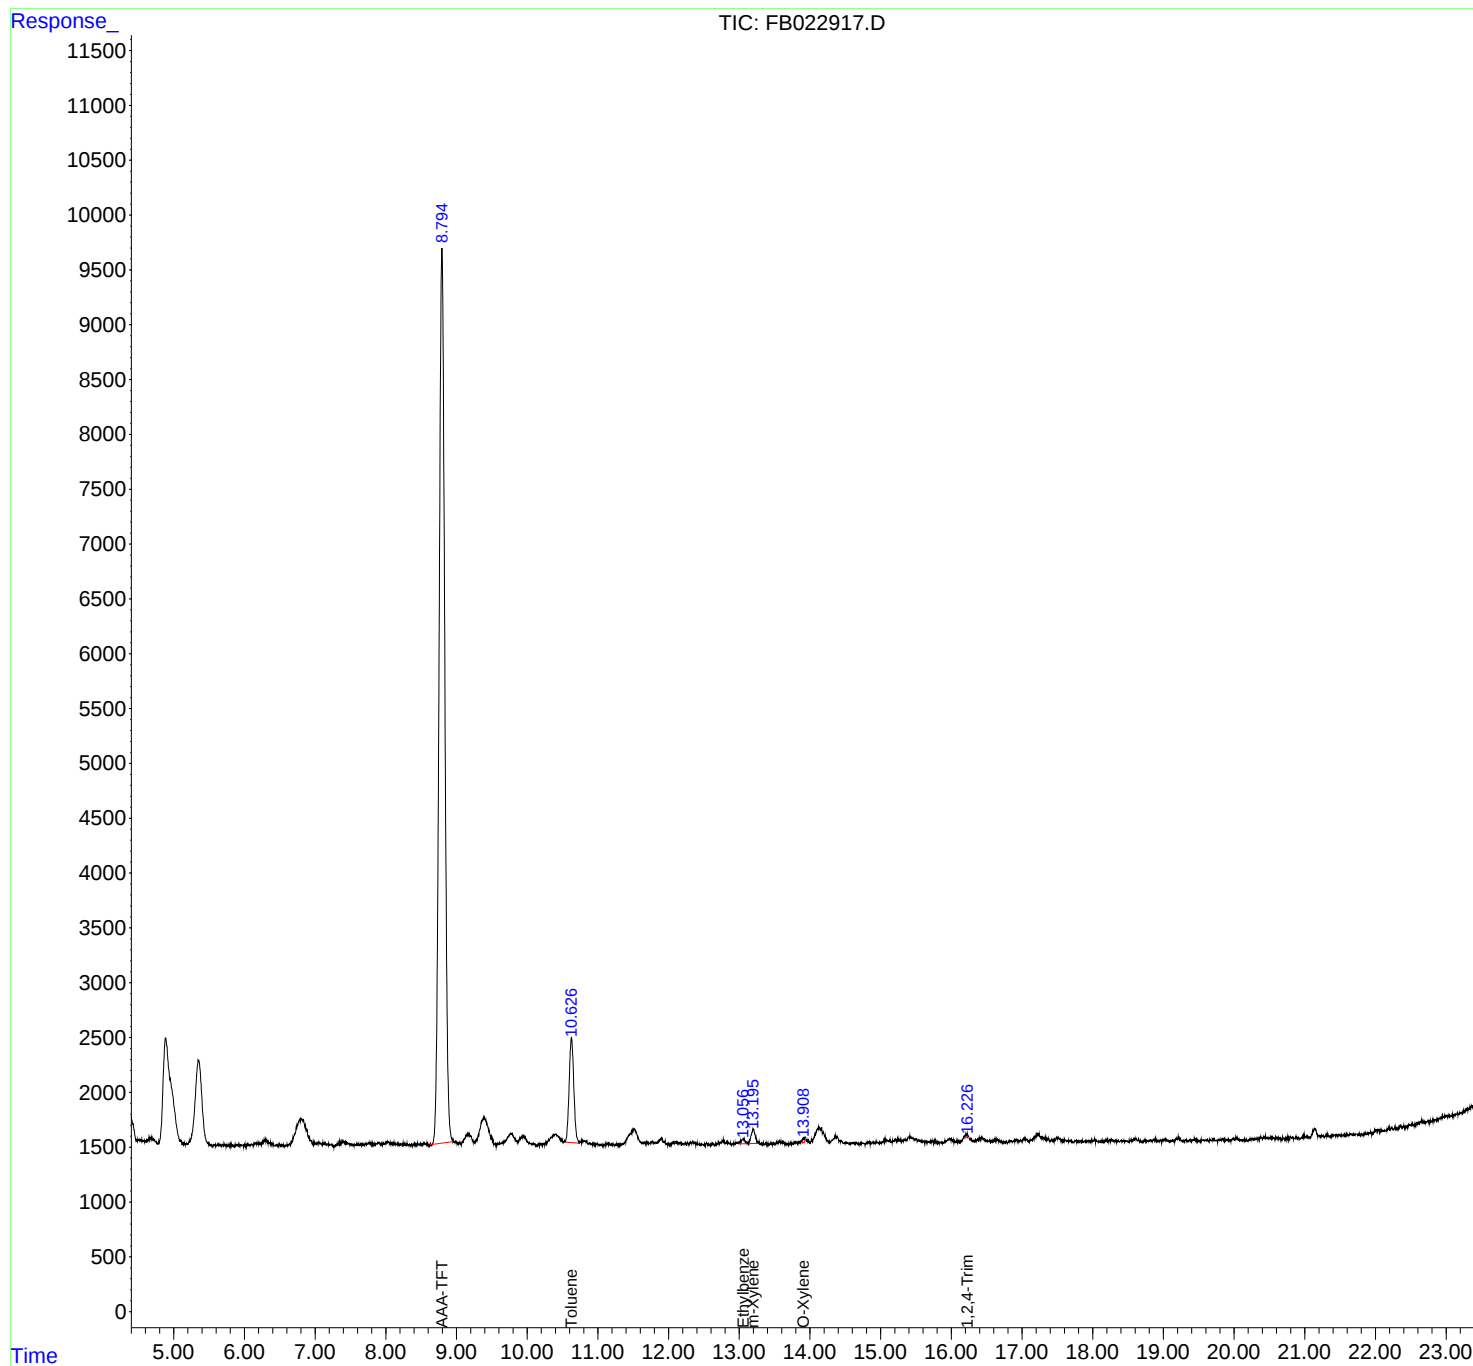


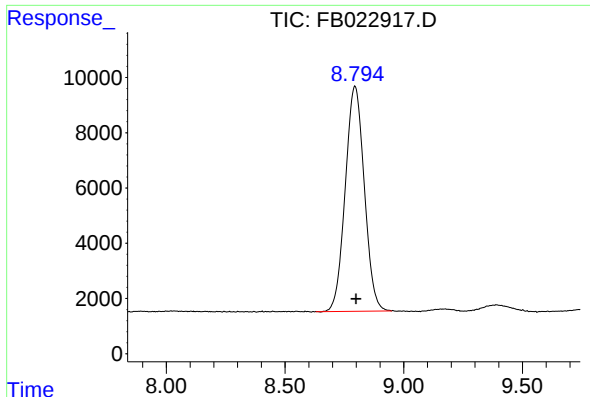

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 453860
Conc: 20.16 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-110619

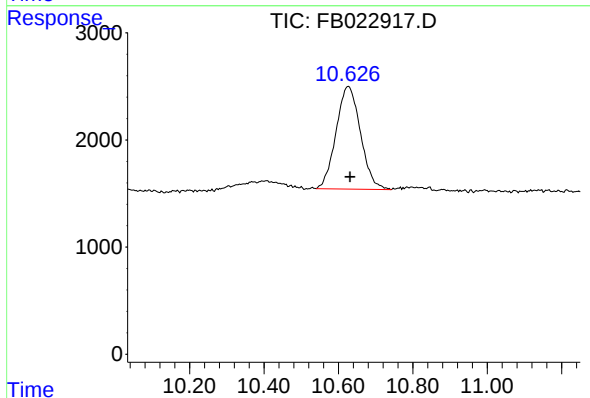


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 43615
Conc: 1.01 ng/ml

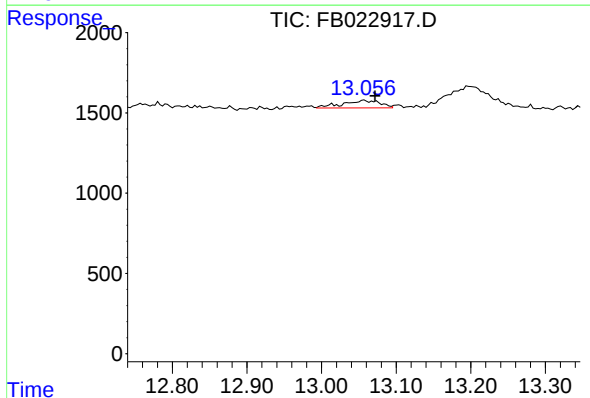


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.014 min
Response: 1577
Conc: 0.04 ng/ml

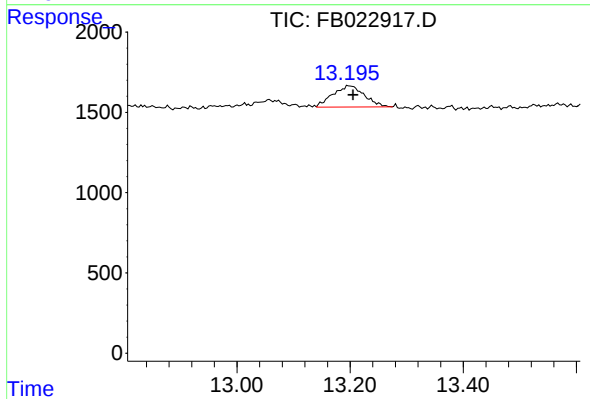

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.008 min
Response: 5093
Conc: 0.13 ng/ml

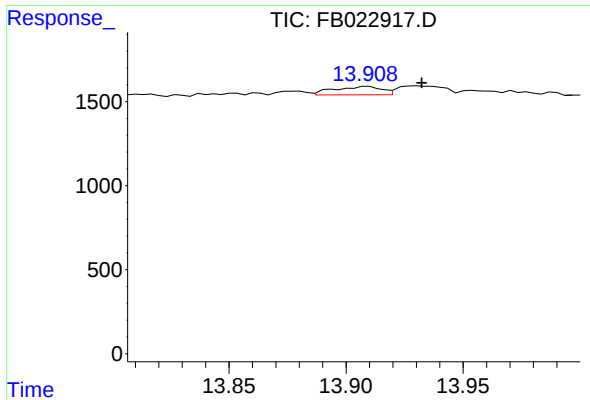

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.023 min
Response: 684
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-110619

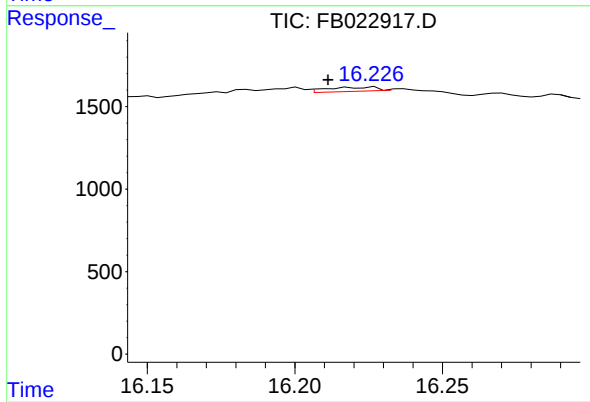

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.007 min
Response: 293
Conc: 0.01 ng/ml