

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022918.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 12:48
 Operator : DD/AJ
 Sample : K5676-07
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-04-110619

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	449721	19.977 ng/ml
Target Compounds			
6) t Toluene	10.619	5125	0.119 ng/ml
7) t Ethylbenzene	13.061	860	0.022 ng/ml
8) t m-Xylene	13.210	2779	0.074 ng/ml
9) t O-Xylene	13.931	2195	0.062 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	3220	0.114 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022918.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 12:48
Operator : DD/AJ
Sample : K5676-07
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-04-110619

Integration File: Calibration.e
Quant Time: Nov 07 15:19:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

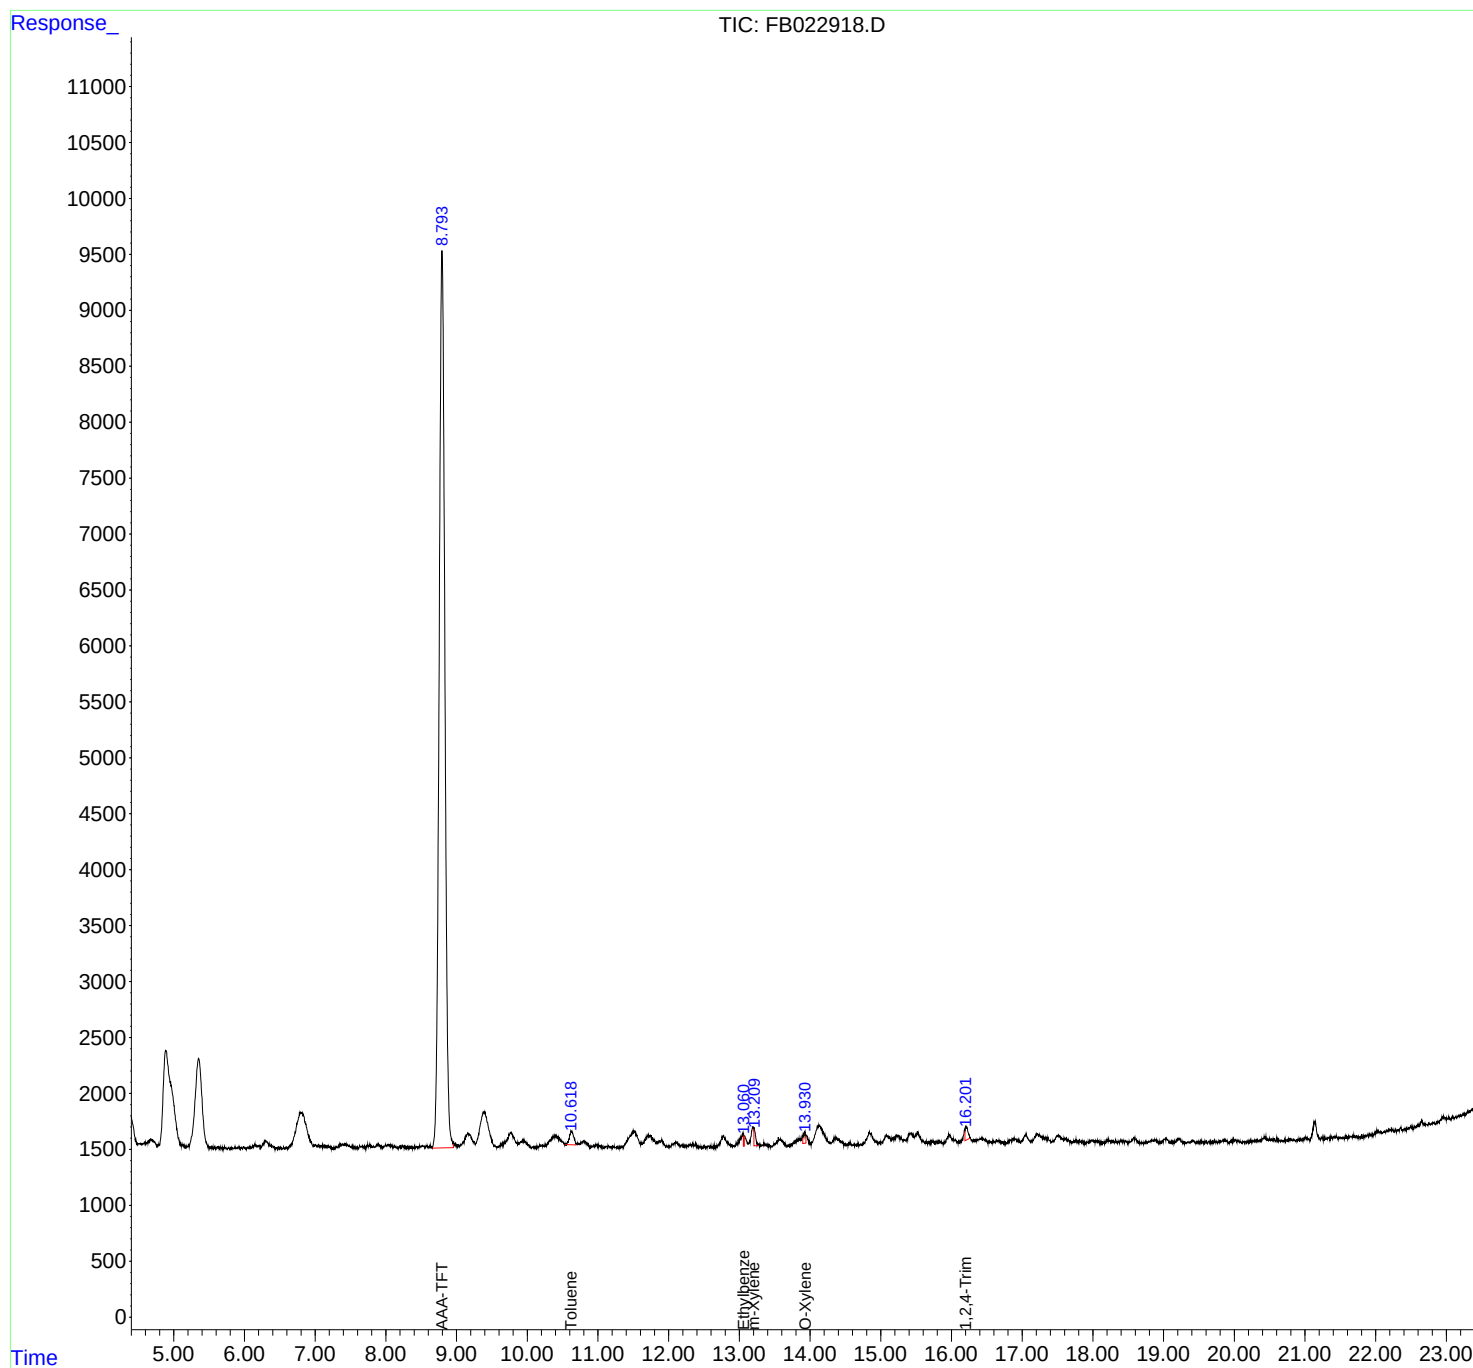


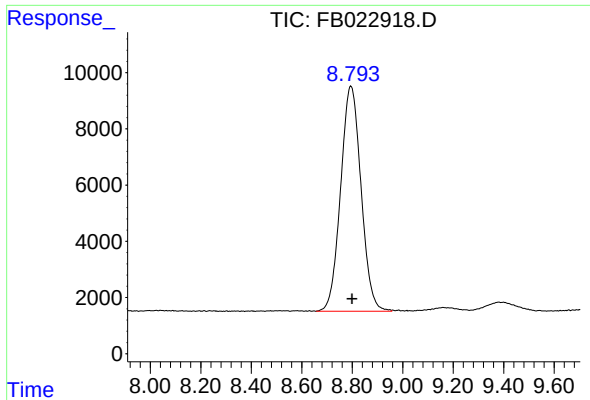

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 449721
Conc: 19.98 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619

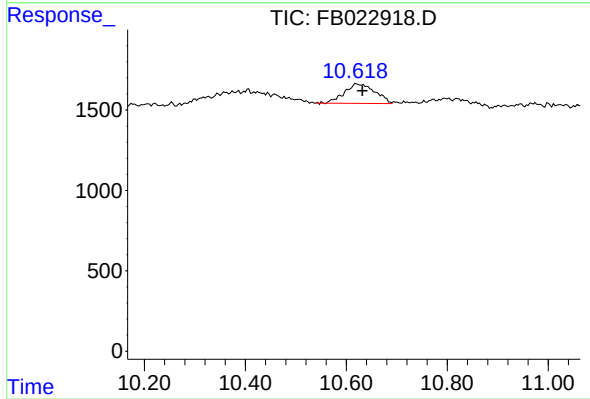


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.012 min
Response: 5125
Conc: 0.12 ng/ml

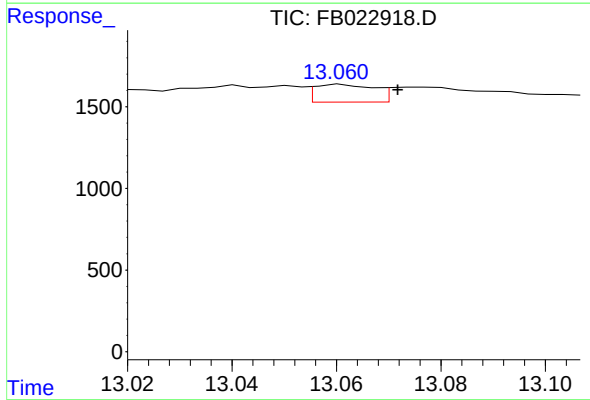


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.010 min
Response: 860
Conc: 0.02 ng/ml

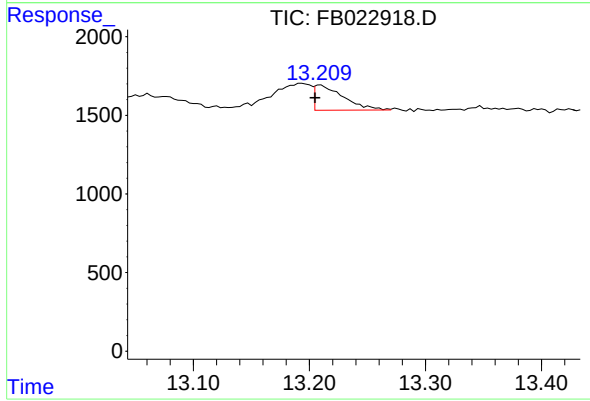

#8 m-Xylene


R.T.: 13.210 min
Delta R.T.: 0.005 min
Response: 2779
Conc: 0.07 ng/ml

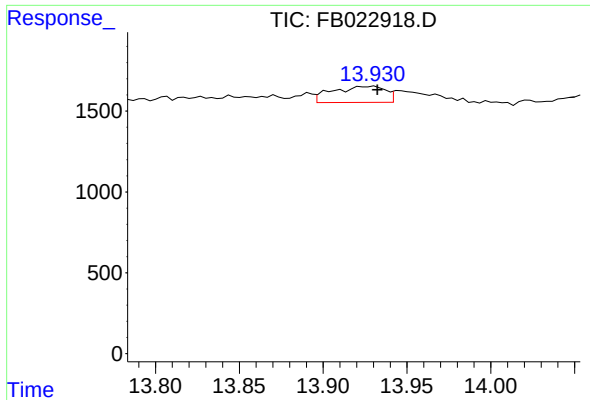

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 2195
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619

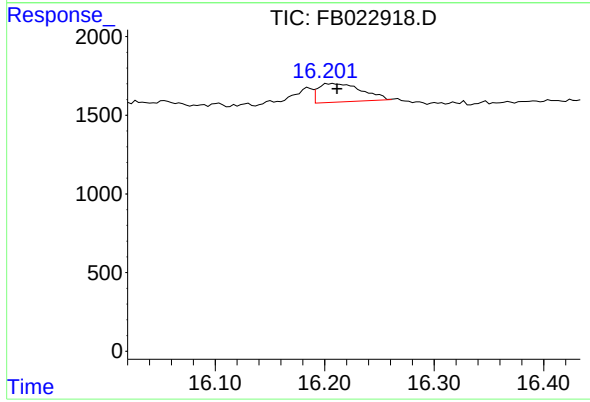

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.009 min
Response: 3220
Conc: 0.11 ng/ml