

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022920.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 13:48
 Operator : DD/AJ
 Sample : K5676-07MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-04-110619MSD

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	460448	20.454 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	796288	24.754 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	767281	21.736 ng/ml
3) t n-Heptane	7.755	251385	7.227 ng/ml
4) t Benzene	7.889	403642	9.319 ng/ml
6) t Toluene	10.627	1154147	26.772 ng/ml
7) t Ethylbenzene	13.067	353065	8.844 ng/ml
8) t m-Xylene	13.200	662603	17.544 ng/ml
9) t O-Xylene	13.928	626825	17.587 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	476669	16.809 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022920.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 13:48
Operator : DD/AJ
Sample : K5676-07MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-04-110619MSD

Integration File: Calibration.e
Quant Time: Nov 07 15:19:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

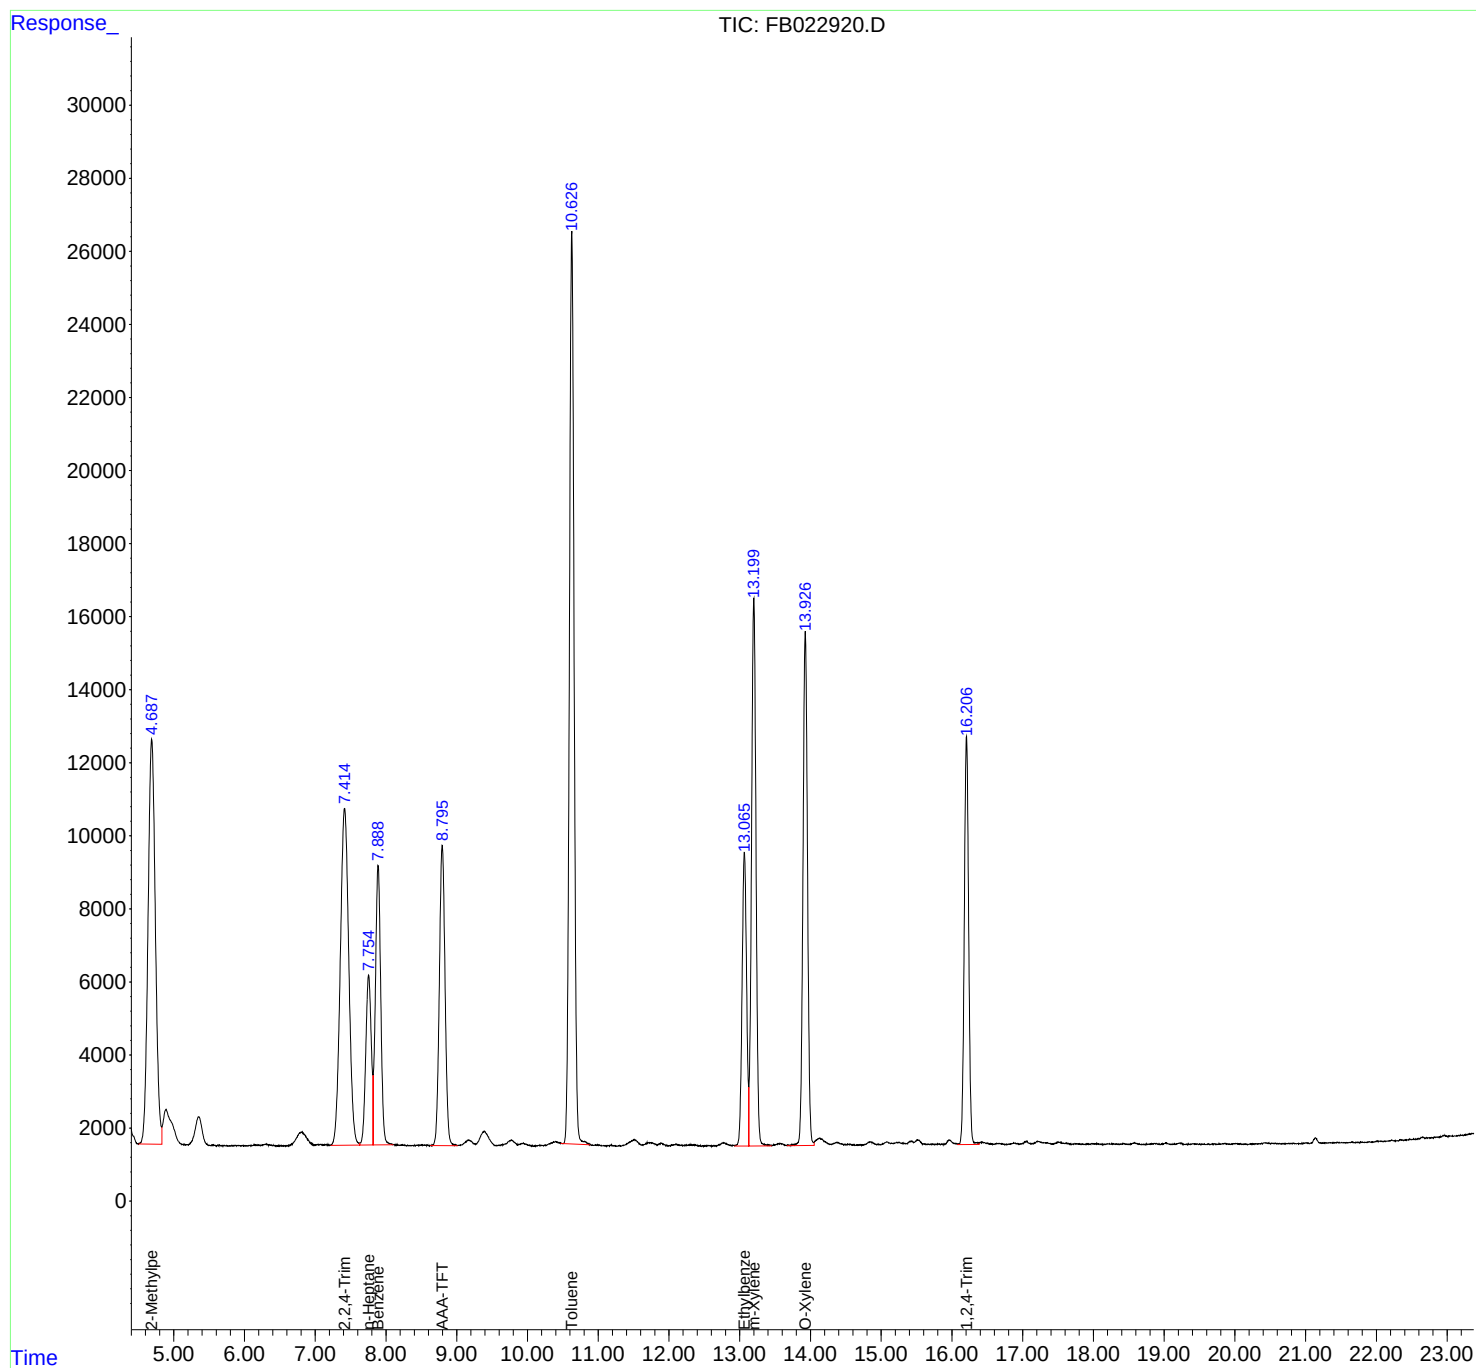


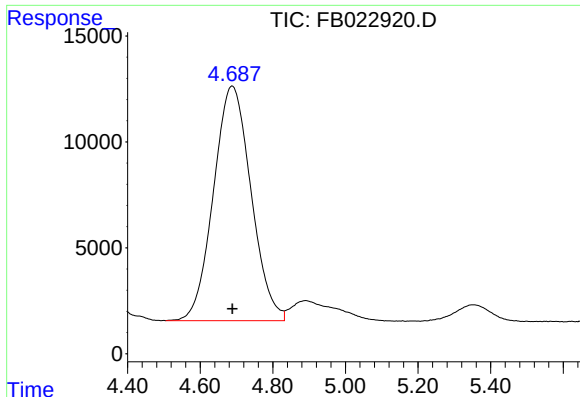

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 796288
Conc: 24.75 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MSD

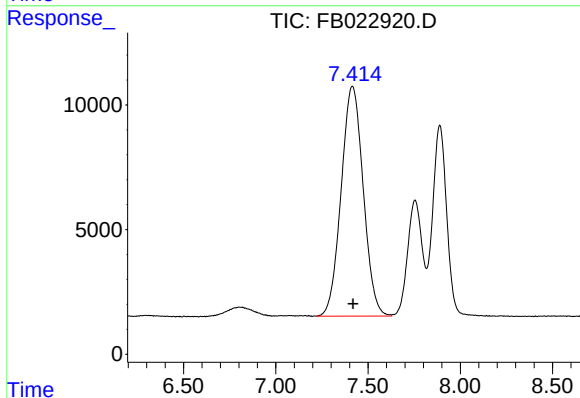


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 767281
Conc: 21.74 ng/ml

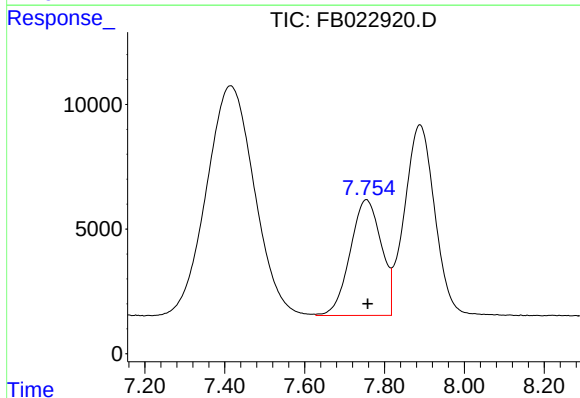


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 251385
Conc: 7.23 ng/ml

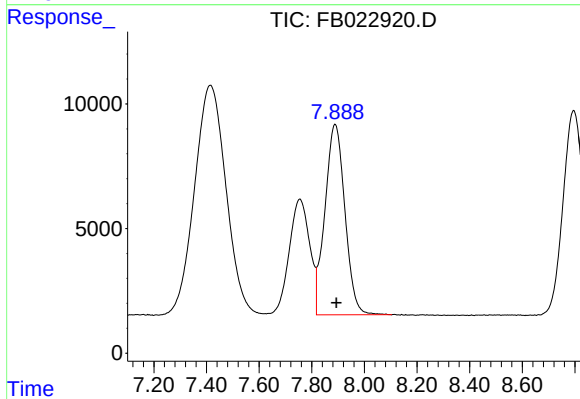

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 403642
Conc: 9.32 ng/ml

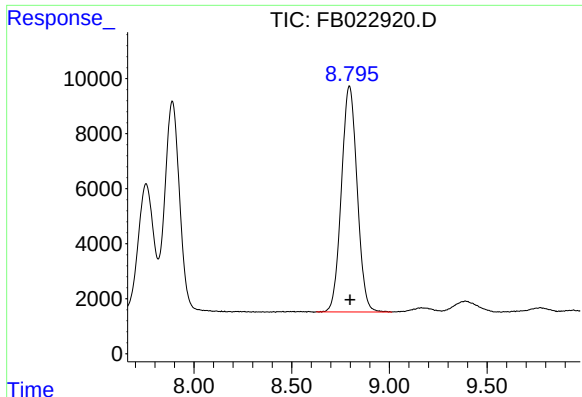

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 460448
Conc: 20.45 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MSD

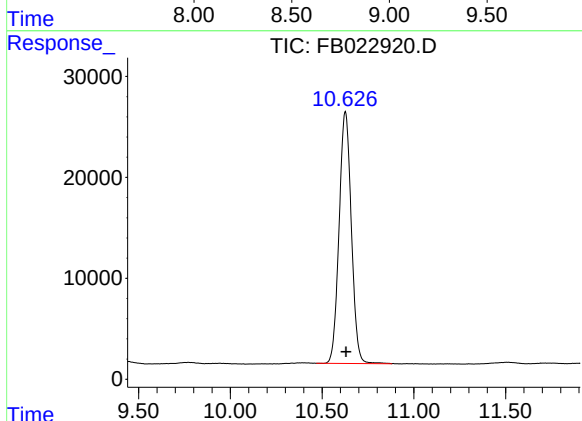


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1154147
Conc: 26.77 ng/ml

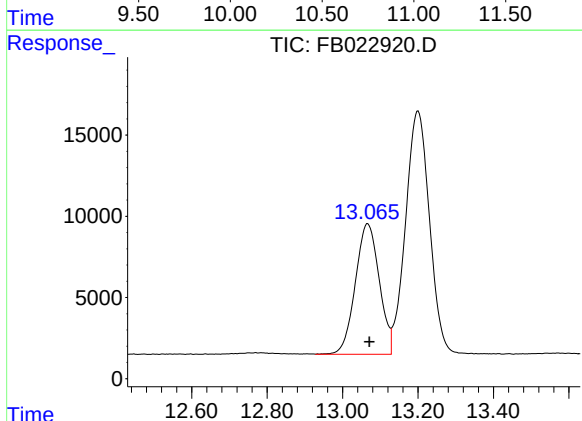


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 353065
Conc: 8.84 ng/ml

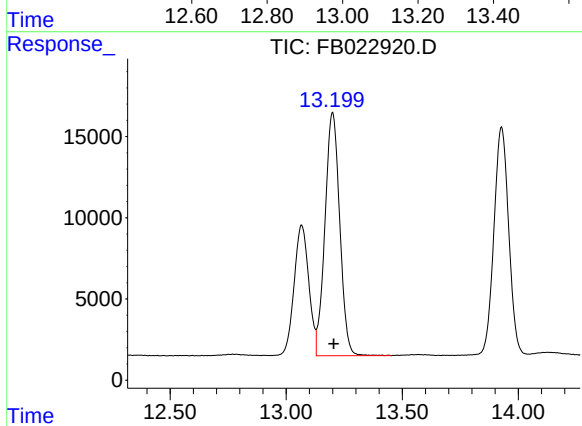

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 662603
Conc: 17.54 ng/ml

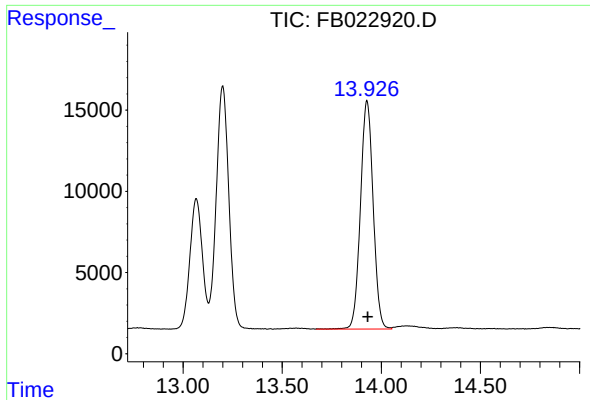

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 626825
Conc: 17.59 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MSD

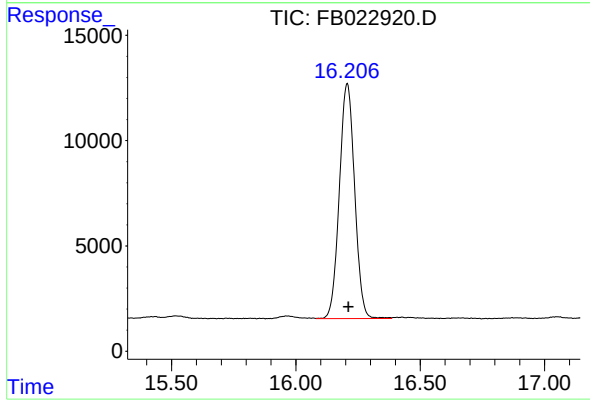

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 476669
Conc: 16.81 ng/ml