

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022923.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 17:06
 Operator : DD/AJ
 Sample : K5742-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-10-(4-6)

Integration File: Calibration.e
 Quant Time: Nov 08 02:54:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	438427	19.475 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.678	13990	0.435 ng/ml
2) t 2,2,4-Trimethylpentane	7.378	23141	0.656 ng/ml
3) t n-Heptane	7.758	27199	0.782 ng/ml
4) t Benzene	7.885	15992	0.369 ng/ml
6) t Toluene	10.627	87677	2.034 ng/ml
7) t Ethylbenzene	13.040	160140	4.011 ng/ml
8) t m-Xylene	13.196	127311	3.371 ng/ml
9) t O-Xylene	13.933	55517	1.558 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	174237	6.144 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022923.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 17:06
Operator : DD/AJ
Sample : K5742-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-10-(4-6)

Integration File: Calibration.e
Quant Time: Nov 08 02:54:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

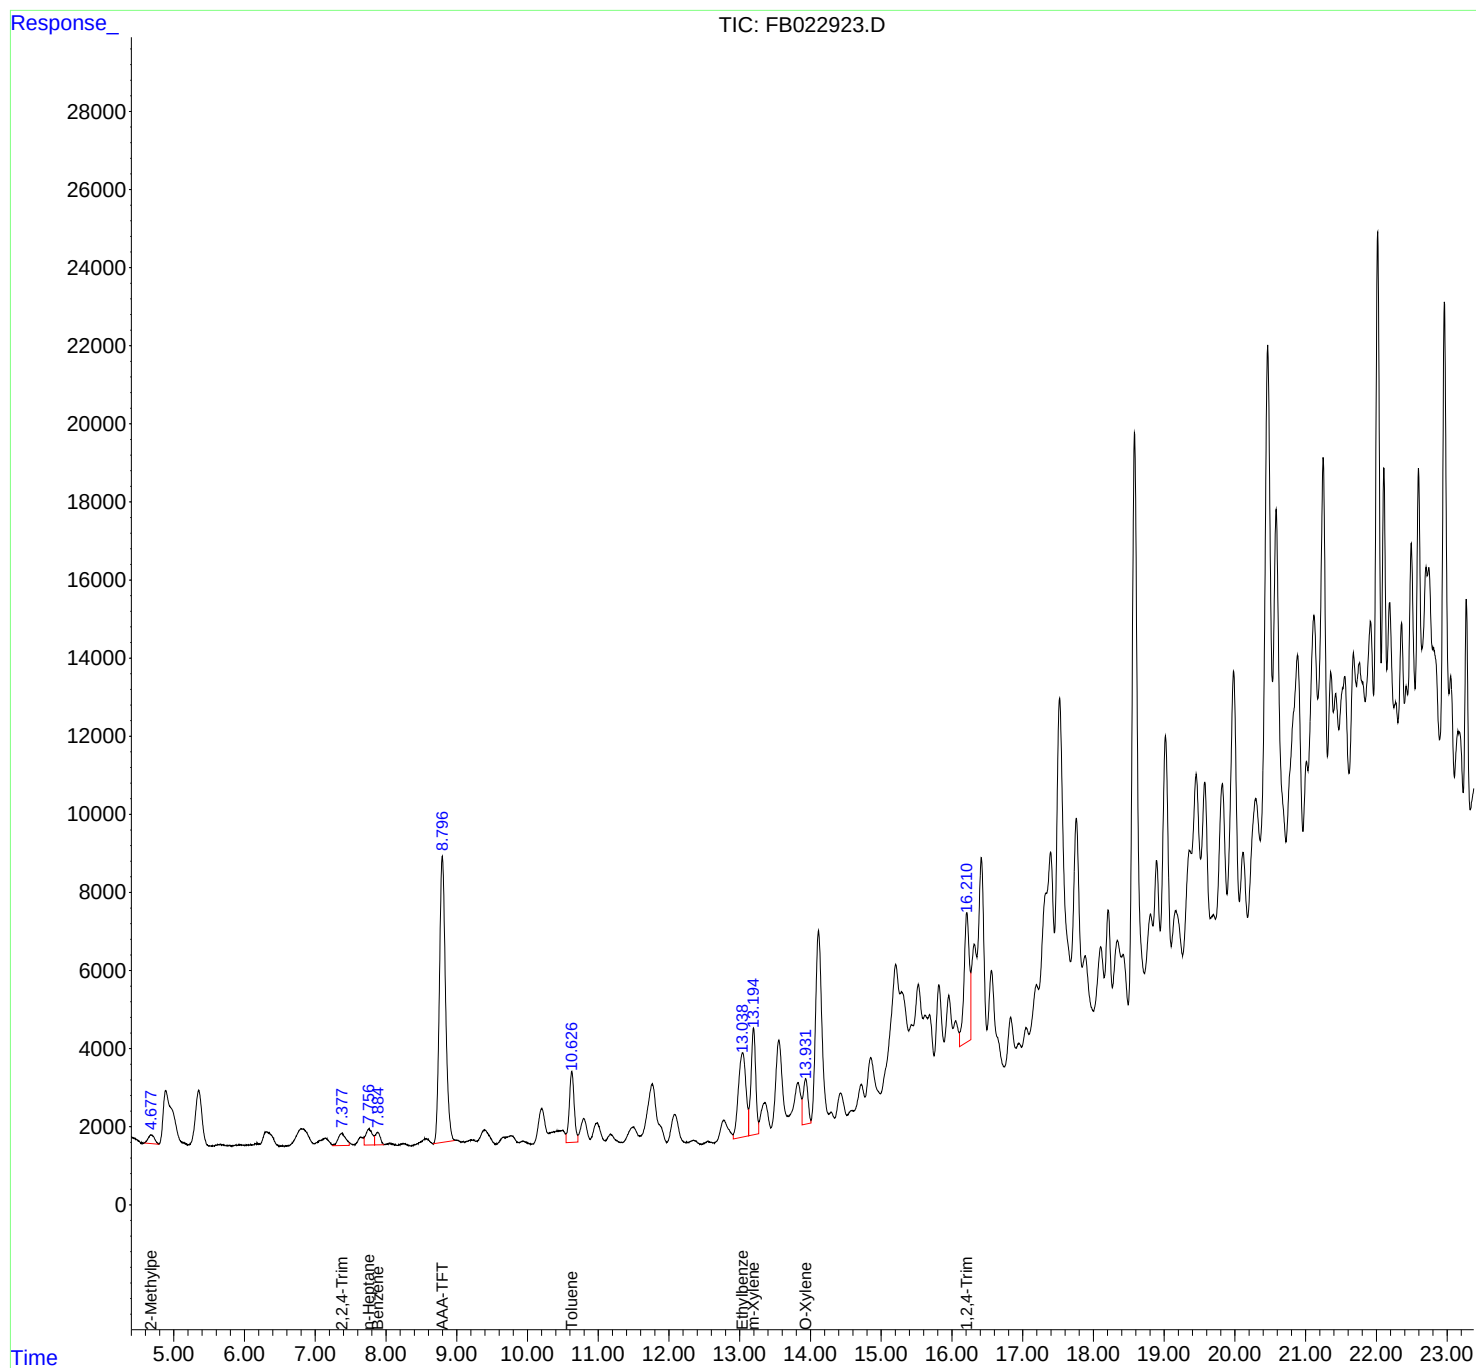


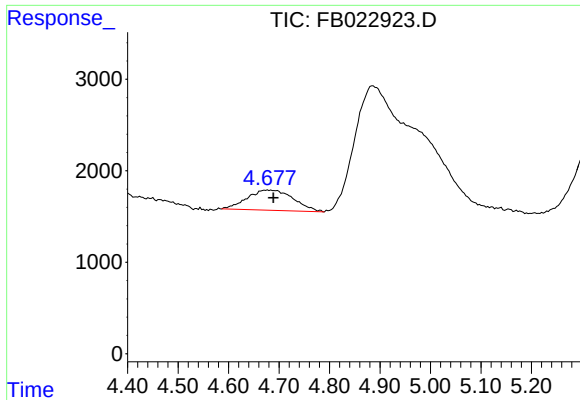

#1 2-Methylpentane


R.T.: 4.678 min
Delta R.T.: -0.011 min
Response: 13990
Conc: 0.43 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-10-(4-6)

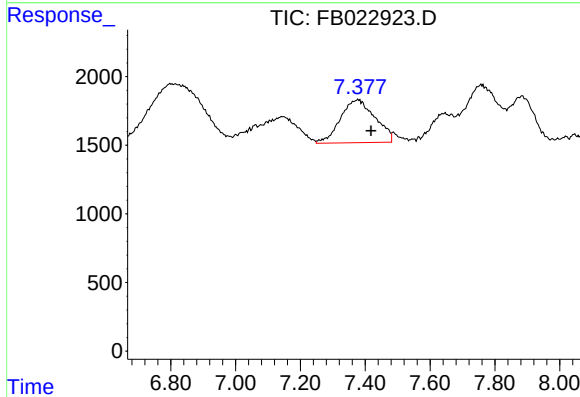


#2 2,2,4-Trimethylpentane

R.T.: 7.378 min
Delta R.T.: -0.040 min
Response: 23141
Conc: 0.66 ng/ml

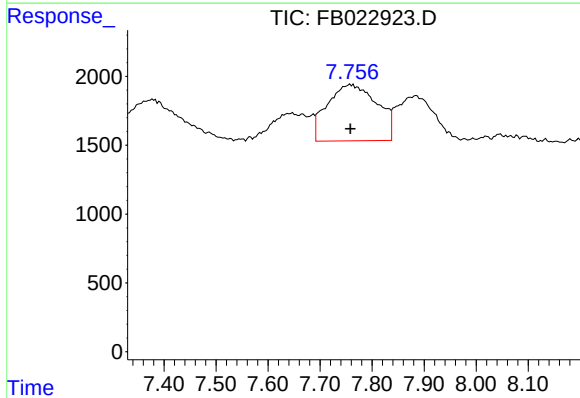


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 27199
Conc: 0.78 ng/ml

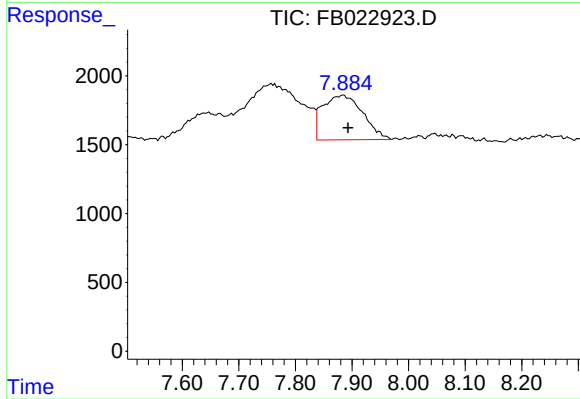

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 15992
Conc: 0.37 ng/ml

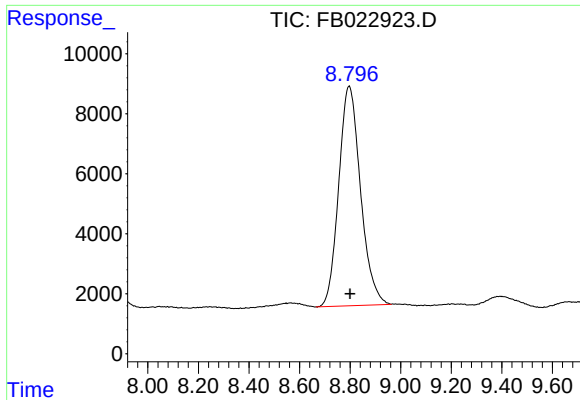

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 438427
Conc: 19.48 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-10-(4-6)

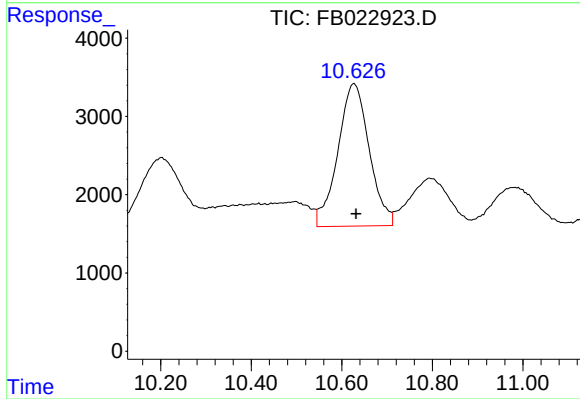


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 87677
Conc: 2.03 ng/ml

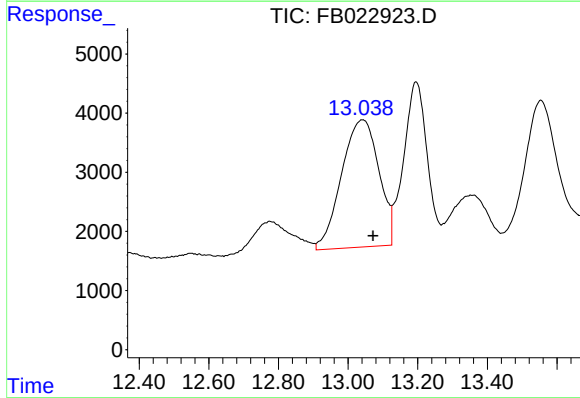


#7 Ethylbenzene

R.T.: 13.040 min
Delta R.T.: -0.032 min
Response: 160140
Conc: 4.01 ng/ml

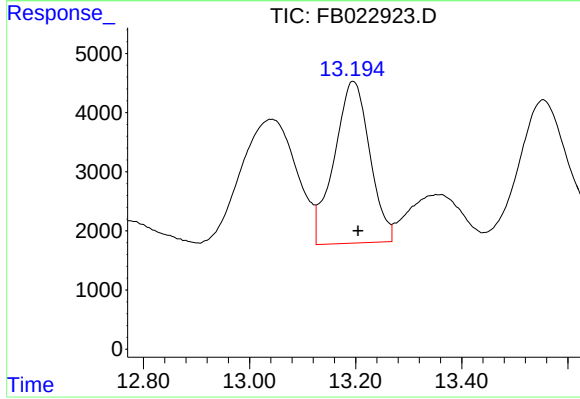

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.009 min
Response: 127311
Conc: 3.37 ng/ml

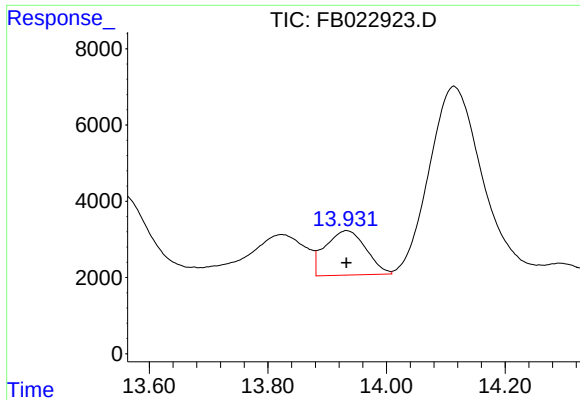

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 55517
Conc: 1.56 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-10-(4-6)

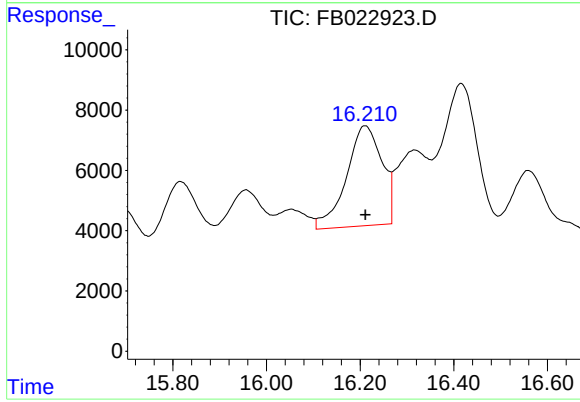

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 174237
Conc: 6.14 ng/ml