

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022925.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 18:06
 Operator : DD/AJ
 Sample : K5742-03
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-17-(6-8)

Integration File: Calibration.e
 Quant Time: Nov 08 02:55:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	452336	20.093 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.677	262	0.008 ng/ml
2) t 2,2,4-Trimethylpentane	7.375	935	0.026 ng/ml
4) t Benzene	7.895	2121	0.049 ng/ml
6) t Toluene	10.630	26052	0.604 ng/ml
7) t Ethylbenzene	13.063	11521	0.289 ng/ml
8) t m-Xylene	13.198	33163	0.878 ng/ml
9) t O-Xylene	13.926	9450	0.265 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	18408	0.649 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022925.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 18:06
Operator : DD/AJ
Sample : K5742-03
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-17-(6-8)

Integration File: Calibration.e
Quant Time: Nov 08 02:55:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

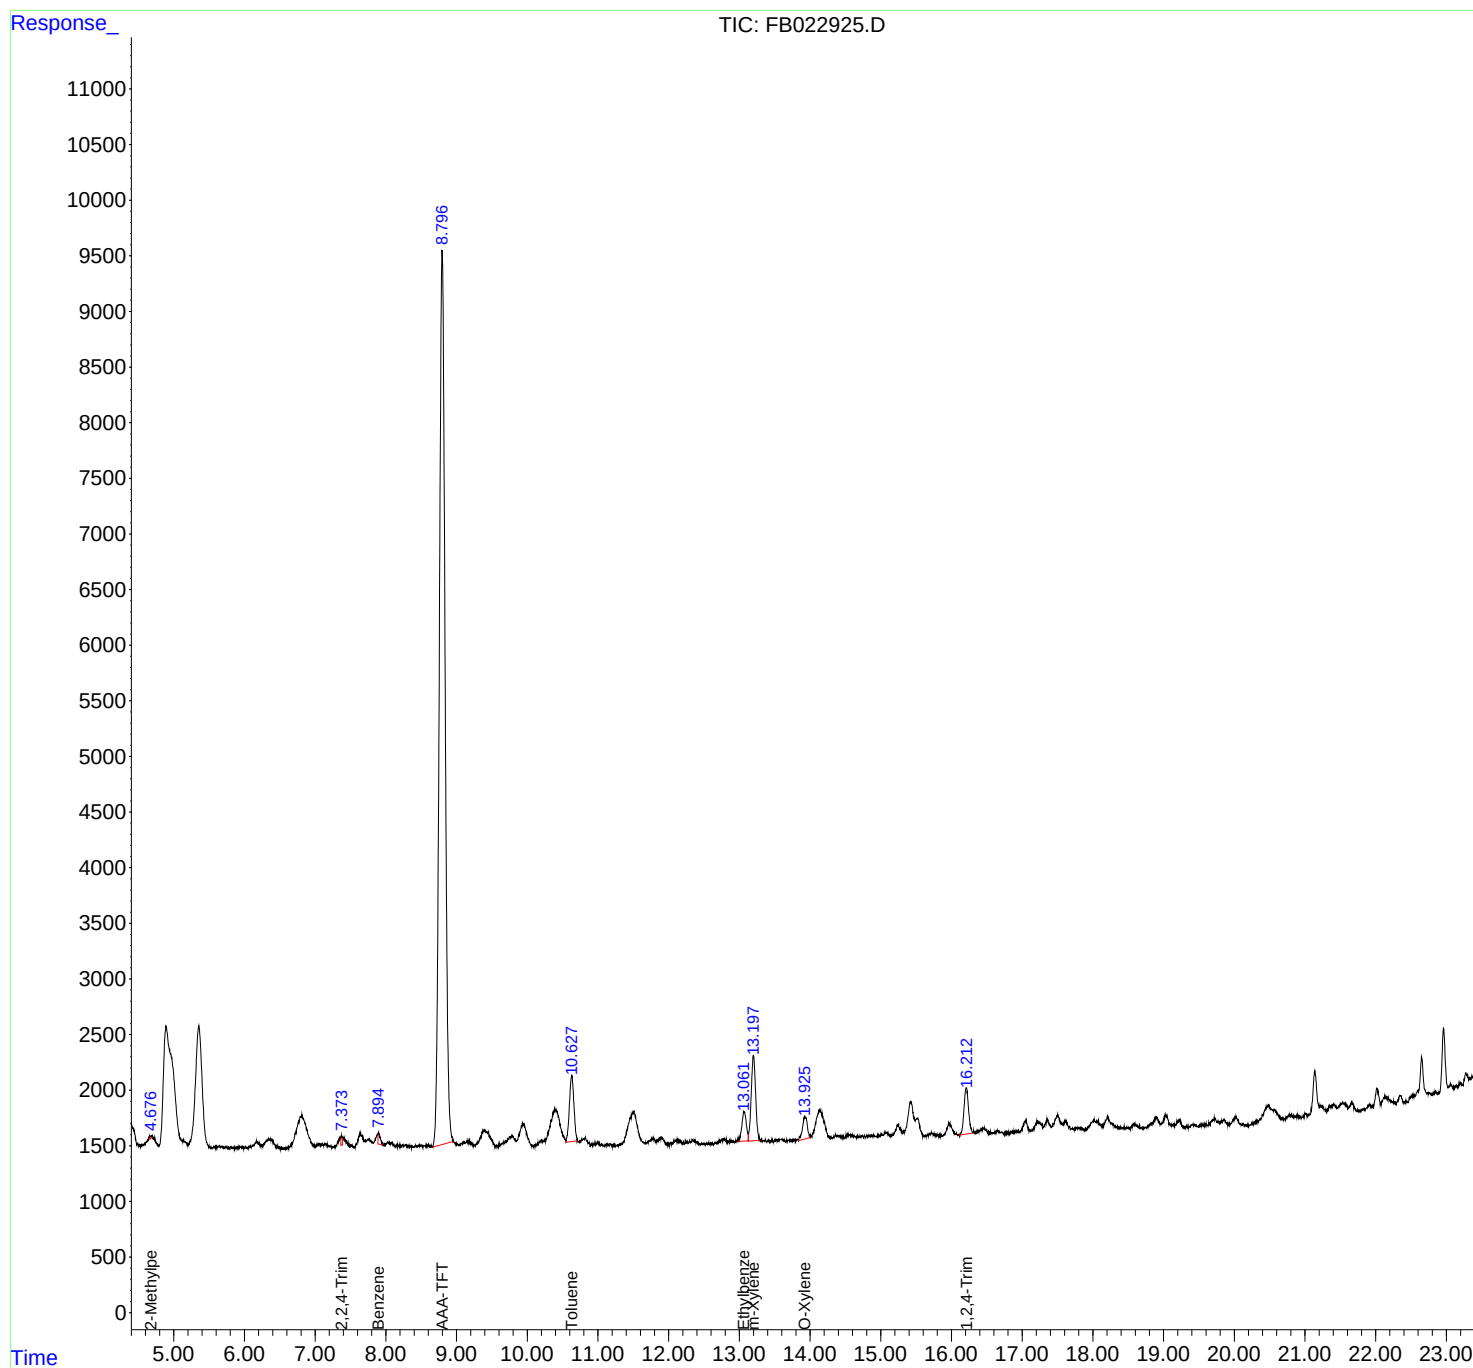


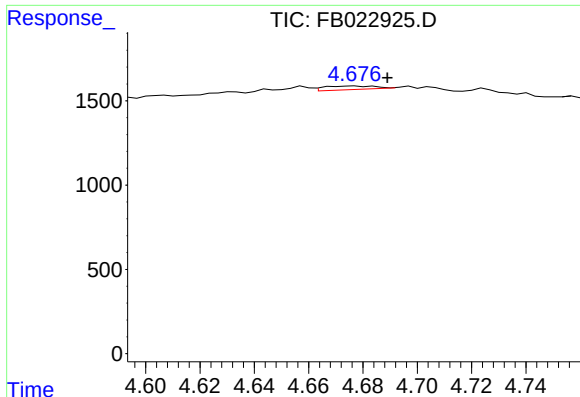

#1 2-Methylpentane


R.T.: 4.677 min
Delta R.T.: -0.012 min
Response: 262
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-17-(6-8)

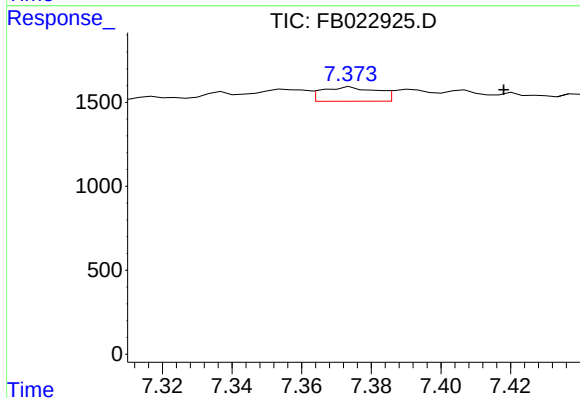


#2 2,2,4-Trimethylpentane

R.T.: 7.375 min
Delta R.T.: -0.043 min
Response: 935
Conc: 0.03 ng/ml

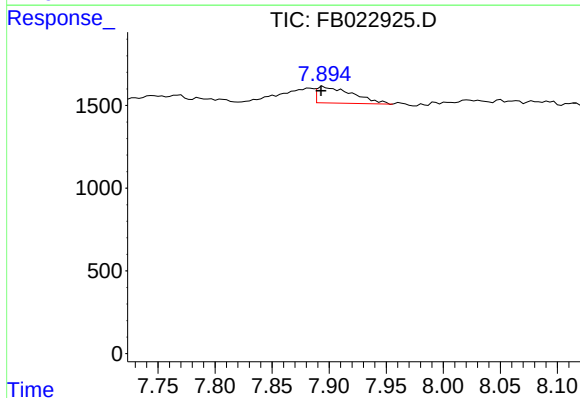


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 2121
Conc: 0.05 ng/ml

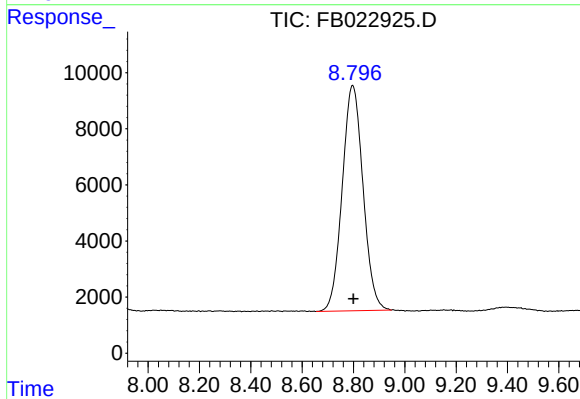

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 452336
Conc: 20.09 ng/ml

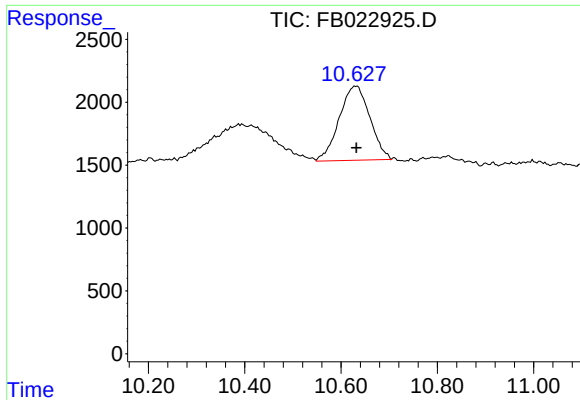

#6 Toluene


R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 26052
Conc: 0.60 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-17-(6-8)

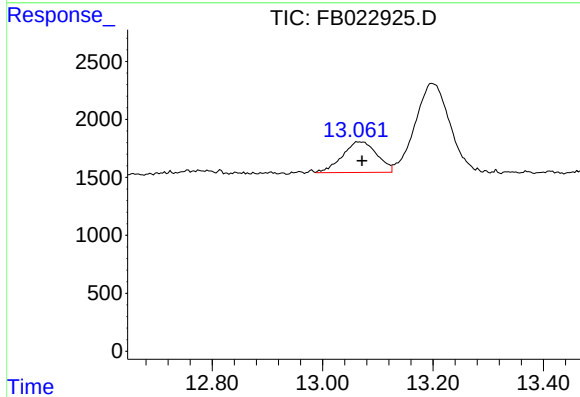


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.009 min
Response: 11521
Conc: 0.29 ng/ml

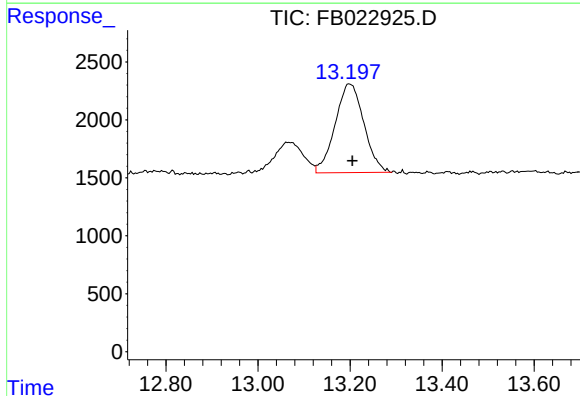


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.006 min
Response: 33163
Conc: 0.88 ng/ml

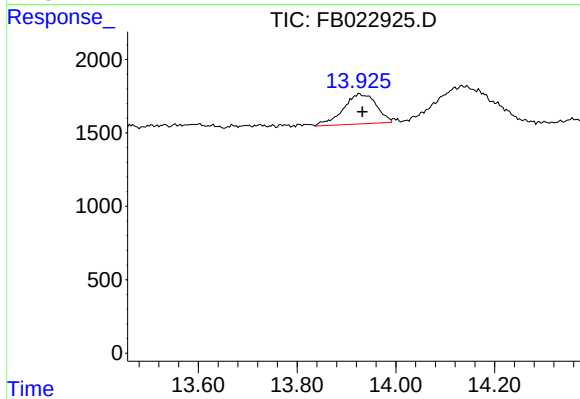

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.006 min
Response: 9450
Conc: 0.27 ng/ml

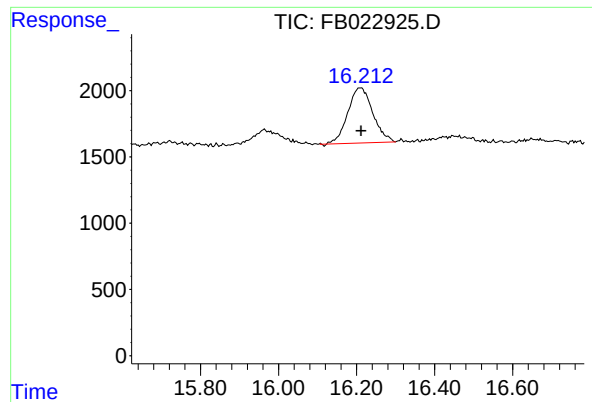

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 18408
Conc: 0.65 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-17-(6-8)