

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022928.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 19:37
 Operator : DD/AJ
 Sample : K5742-06
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-30-(6-8)

Integration File: Calibration.e
 Quant Time: Nov 08 02:55:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	453145	20.129 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	9450	0.294 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	305	0.009 ng/ml
3) t n-Heptane	7.757	24268	0.698 ng/ml
6) t Toluene	10.637	12694	0.294 ng/ml
7) t Ethylbenzene	13.064	39527	0.990 ng/ml
8) t m-Xylene	13.199	75092	1.988 ng/ml
9) t O-Xylene	13.942	7549	0.212 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	90567	3.194 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022928.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 19:37
Operator : DD/AJ
Sample : K5742-06
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-30-(6-8)

Integration File: Calibration.e
Quant Time: Nov 08 02:55:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

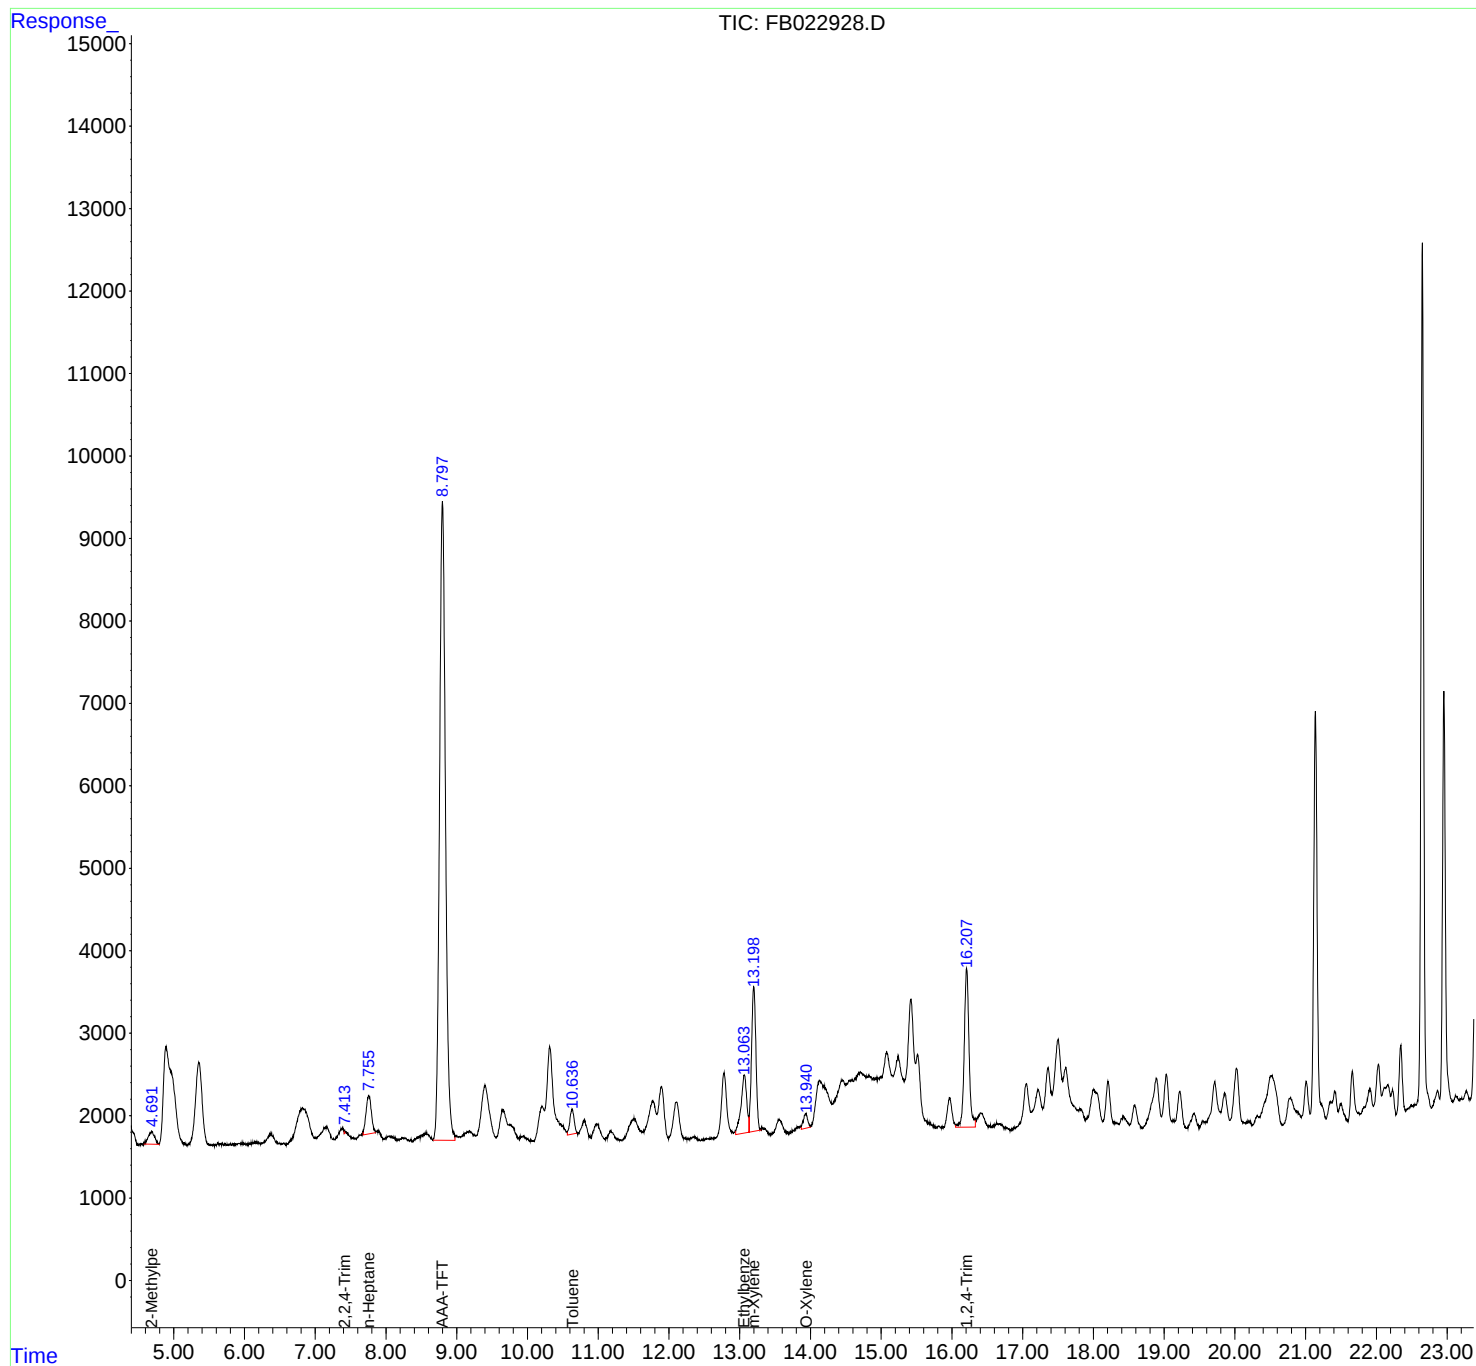


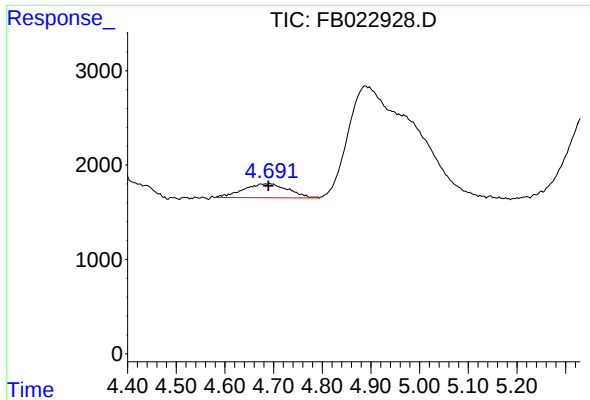

#1 2-Methylpentane


R.T.: 4.692 min
Delta R.T.: 0.003 min
Response: 9450
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-30-(6-8)

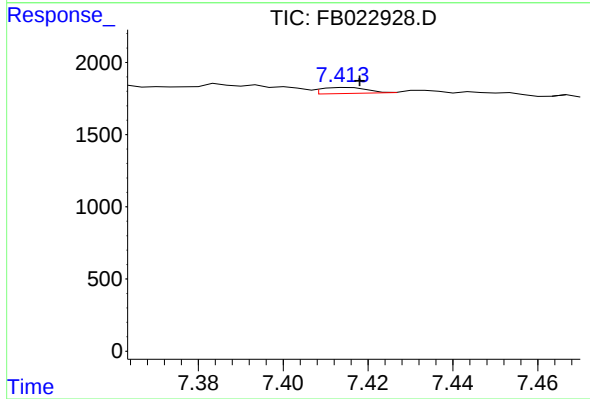


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 305
Conc: 0.01 ng/ml

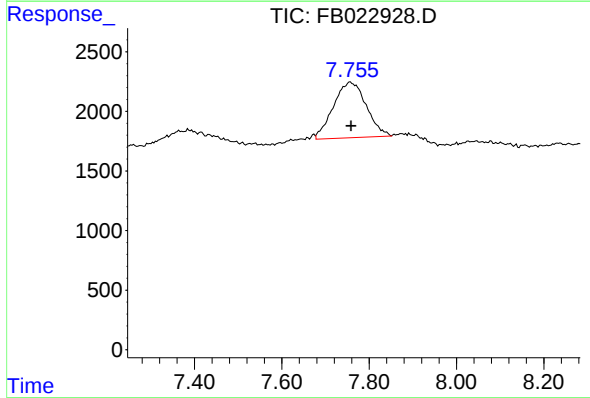


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 24268
Conc: 0.70 ng/ml

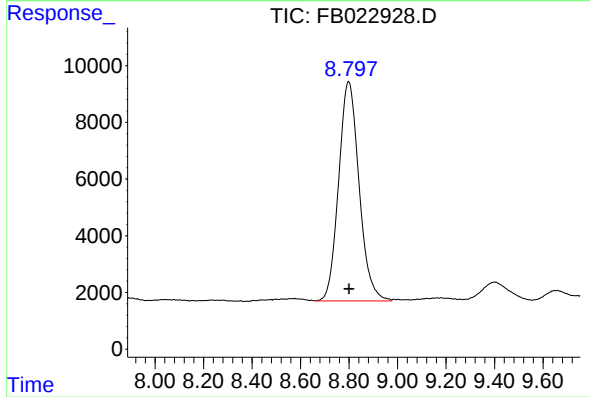

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 453145
Conc: 20.13 ng/ml

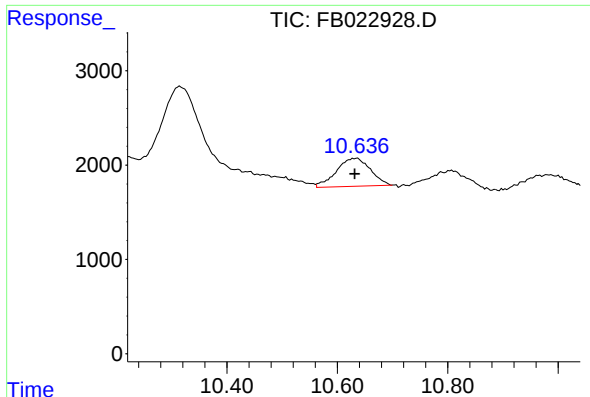

#6 Toluene


R.T.: 10.637 min
Delta R.T.: 0.005 min
Response: 12694
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-30-(6-8)

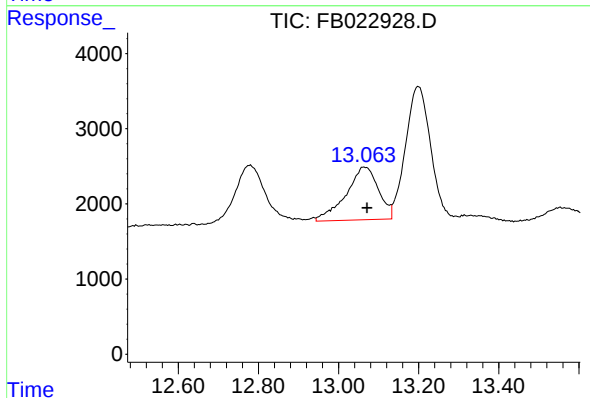


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.008 min
Response: 39527
Conc: 0.99 ng/ml

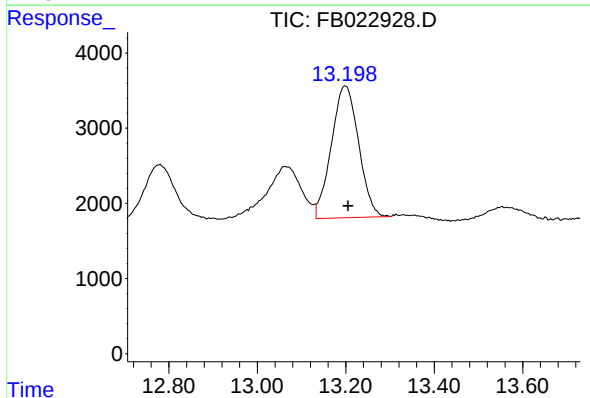


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 75092
Conc: 1.99 ng/ml

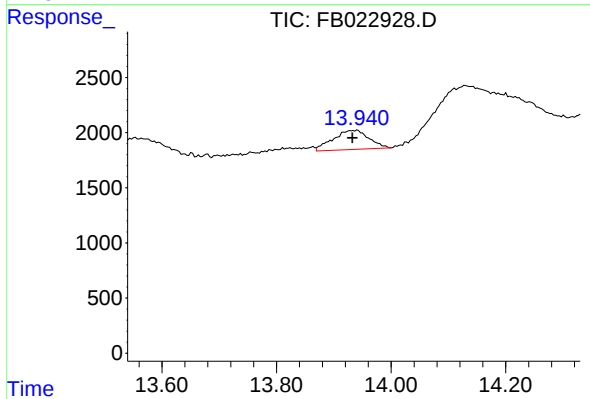

#9 O-Xylene

R.T.: 13.942 min
Delta R.T.: 0.009 min
Response: 7549
Conc: 0.21 ng/ml

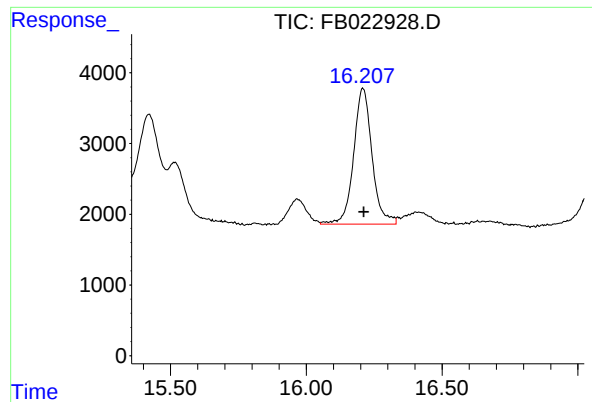

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 90567
Conc: 3.19 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-30-(6-8)