

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022915.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 11:19
 Operator : DD/AJ
 Sample : BSF1107S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1107S1

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	436849	19.405 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	949611	29.521 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1074670	30.444 ng/ml
3) t n-Heptane	7.753	348070	10.006 ng/ml
4) t Benzene	7.887	424851	9.809 ng/ml
6) t Toluene	10.626	1255427	29.121 ng/ml
7) t Ethylbenzene	13.065	397513	9.957 ng/ml
8) t m-Xylene	13.199	760325	20.132 ng/ml
9) t O-Xylene	13.927	710436	19.933 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	567417	20.009 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022915.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 11:19
Operator : DD/AJ
Sample : BSF1107S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1107S1

Integration File: Calibration.e
Quant Time: Nov 07 15:19:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

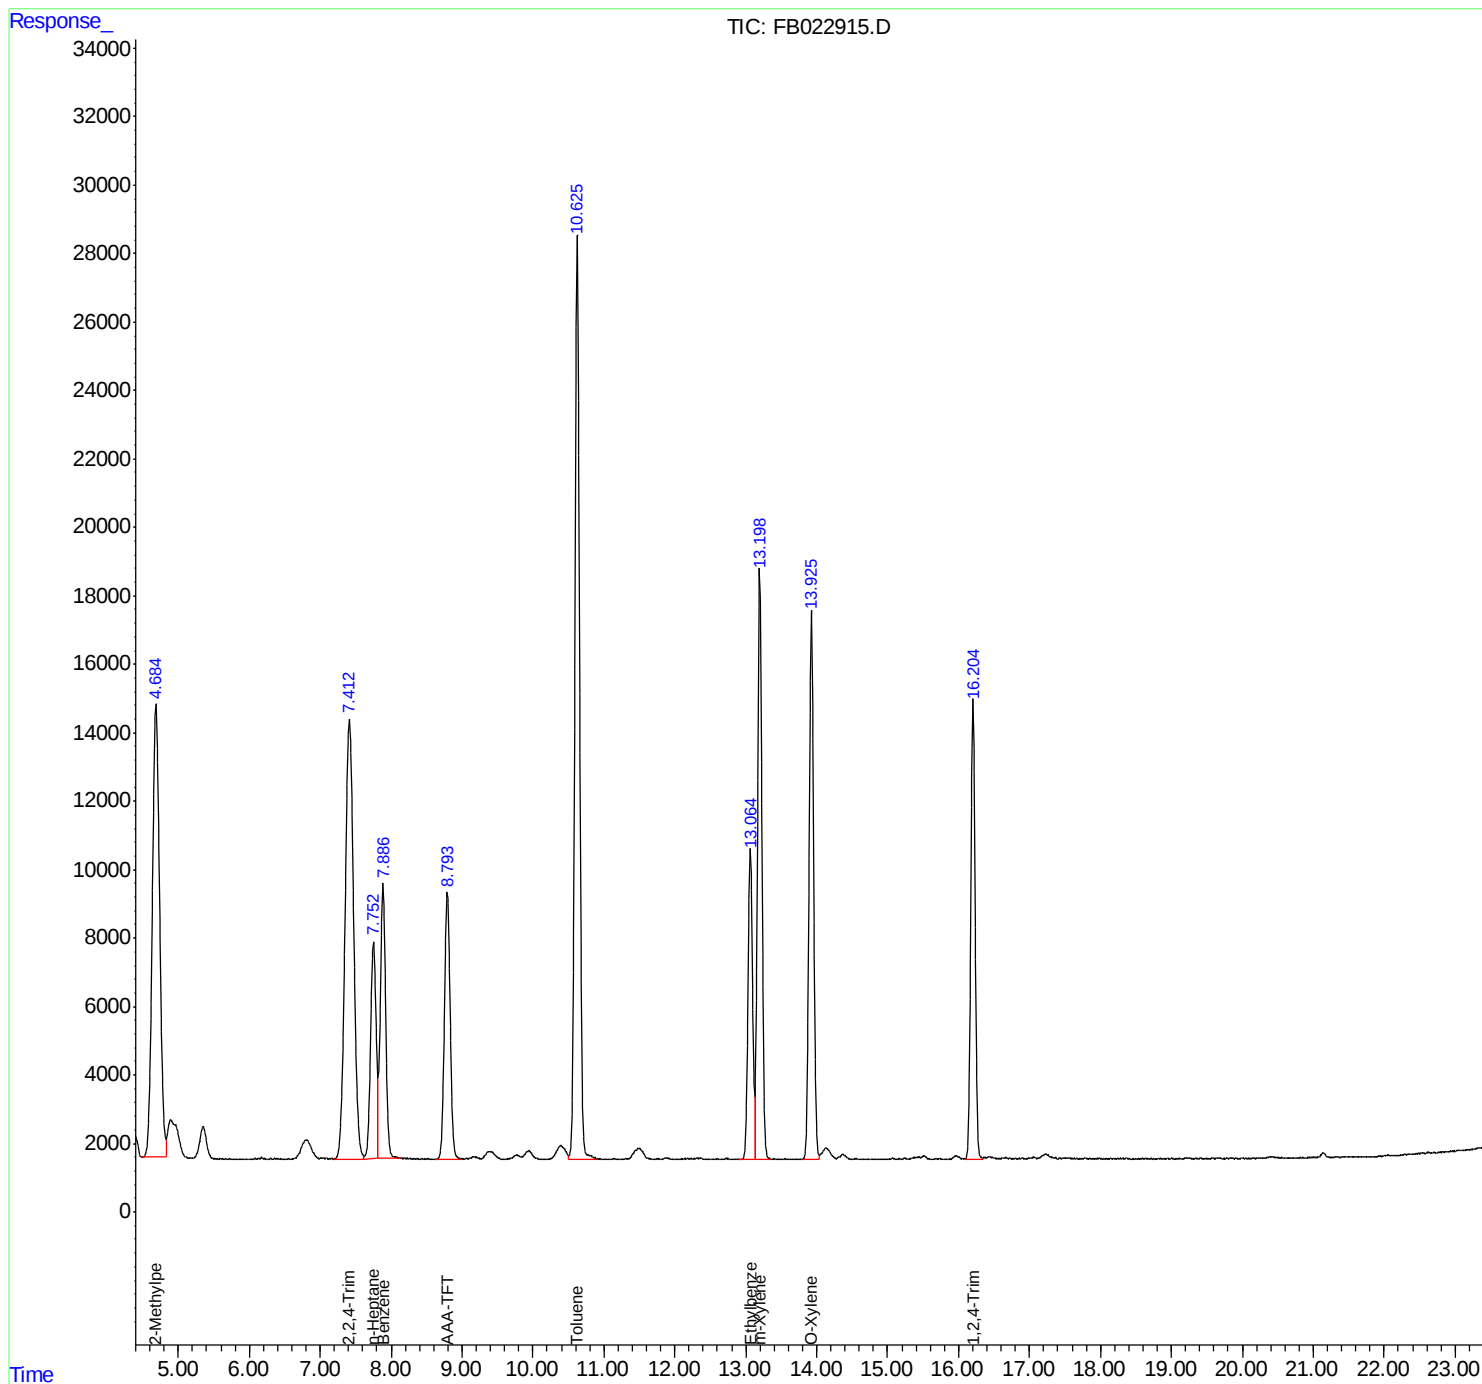


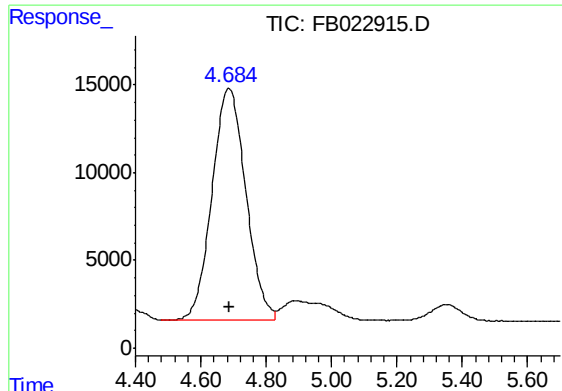

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 949611
Conc: 29.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S1

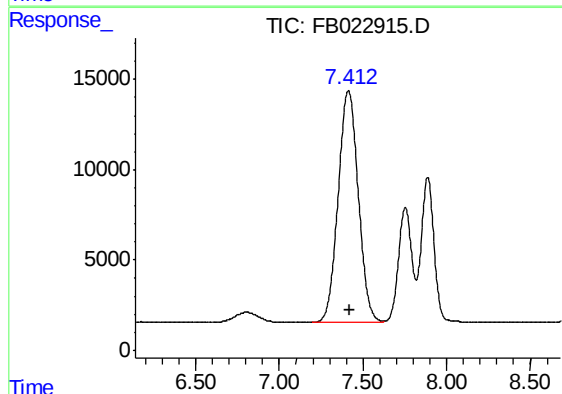


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 1074670
Conc: 30.44 ng/ml

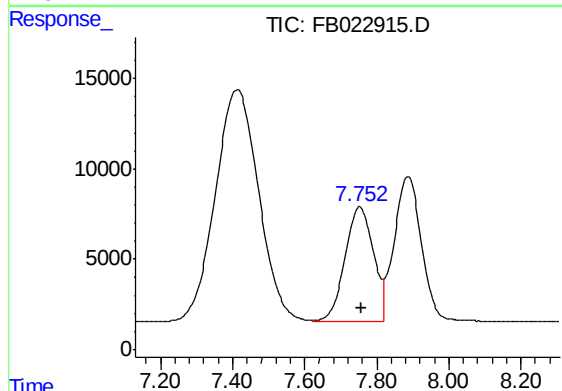


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 348070
Conc: 10.01 ng/ml

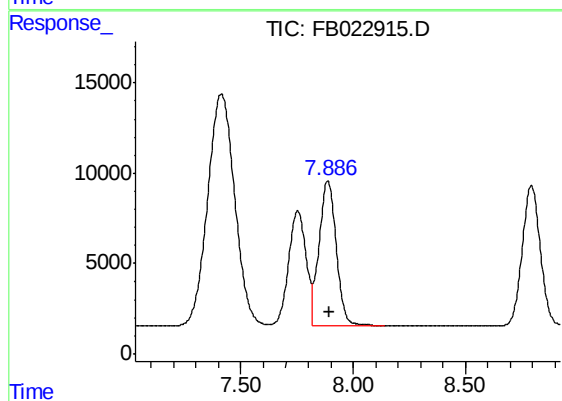

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 424851
Conc: 9.81 ng/ml

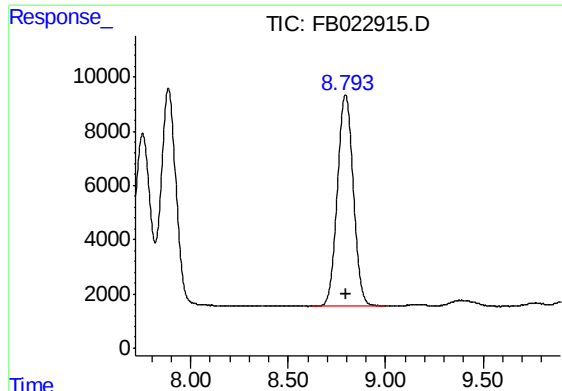

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 436849
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S1

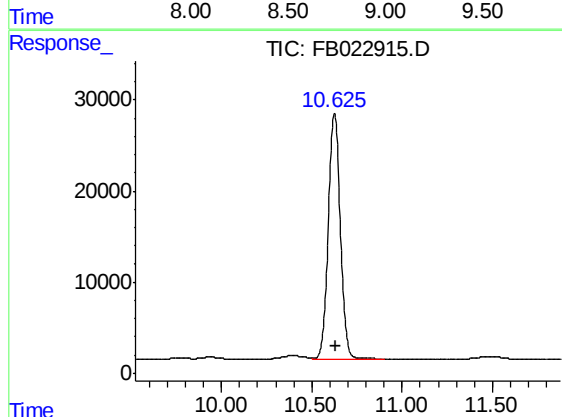


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.006 min
Response: 1255427
Conc: 29.12 ng/ml

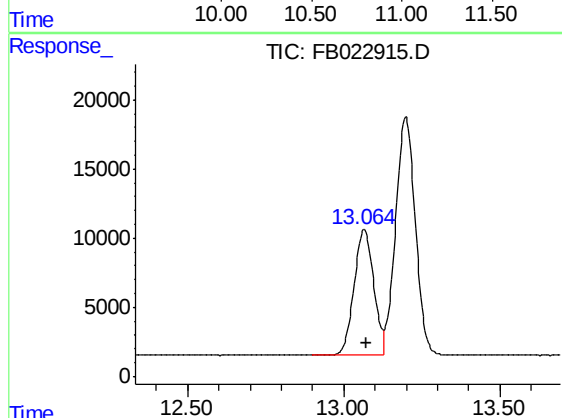


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.006 min
Response: 397513
Conc: 9.96 ng/ml

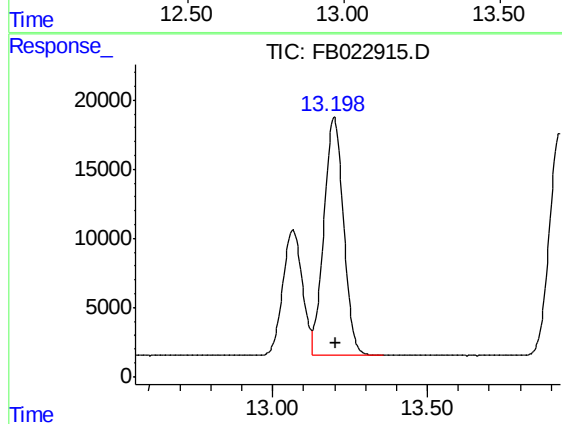

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 760325
Conc: 20.13 ng/ml

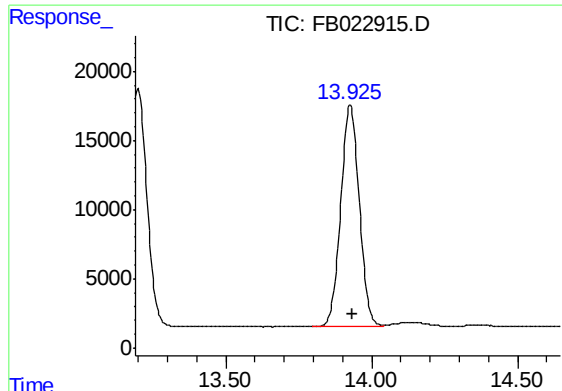

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 710436
Conc: 19.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S1

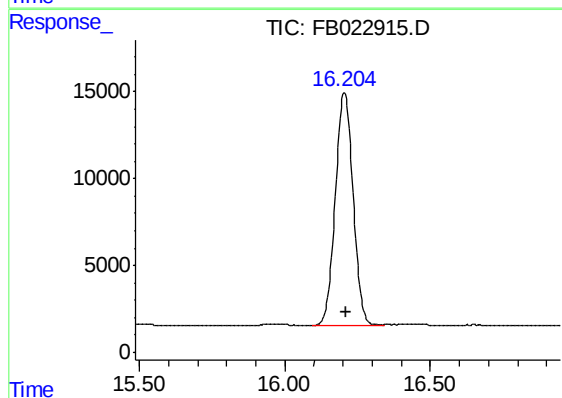

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 567417
Conc: 20.01 ng/ml