

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
 Data File : FB022919.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2019 13:18
 Operator : DD/AJ
 Sample : K5676-07MS
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-04-110619MS

Integration File: Calibration.e
 Quant Time: Nov 07 15:19:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	443154	19.685 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	833764	25.919 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	836557	23.698 ng/ml
3) t n-Heptane	7.754	272140	7.823 ng/ml
4) t Benzene	7.888	404518	9.339 ng/ml
6) t Toluene	10.627	1173666	27.225 ng/ml
7) t Ethylbenzene	13.067	362711	9.085 ng/ml
8) t m-Xylene	13.200	687402	18.201 ng/ml
9) t O-Xylene	13.928	648375	18.192 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	492509	17.367 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110719\
Data File : FB022919.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2019 13:18
Operator : DD/AJ
Sample : K5676-07MS
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-04-110619MS

Integration File: Calibration.e
Quant Time: Nov 07 15:19:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

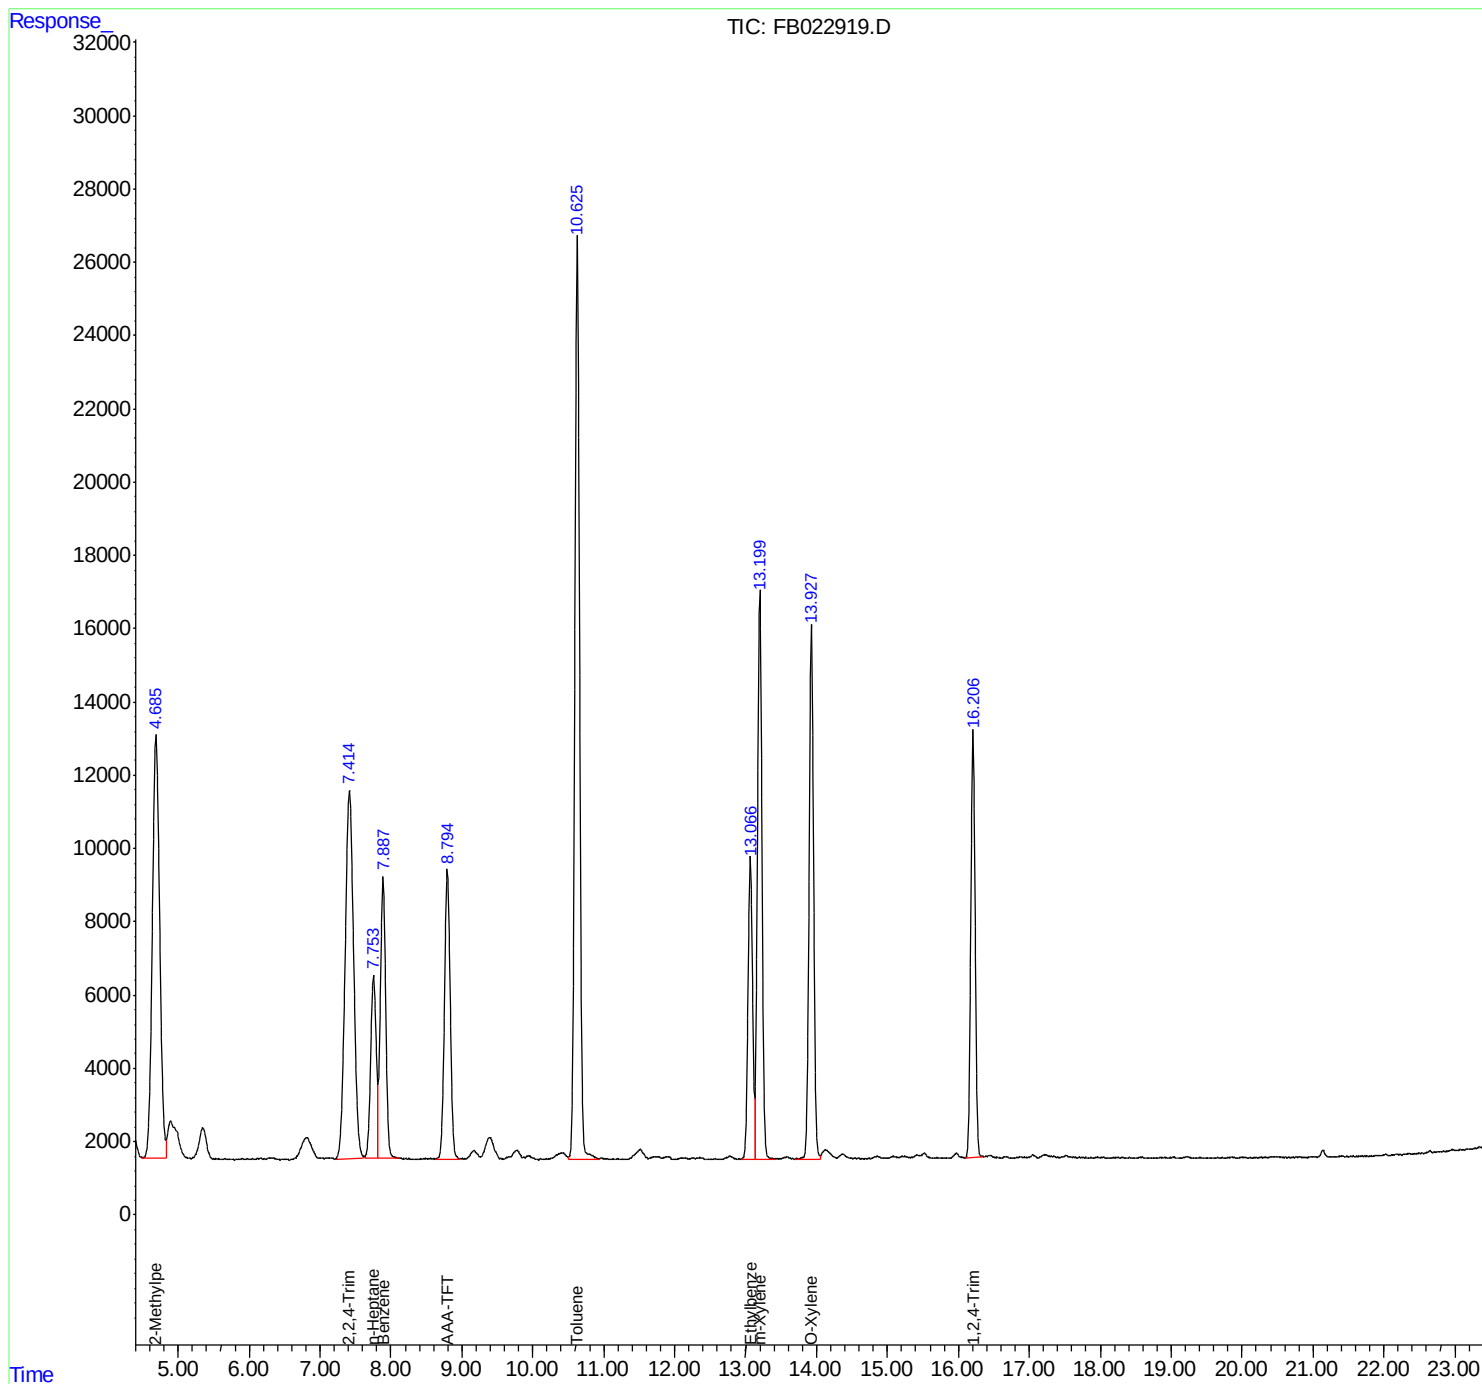


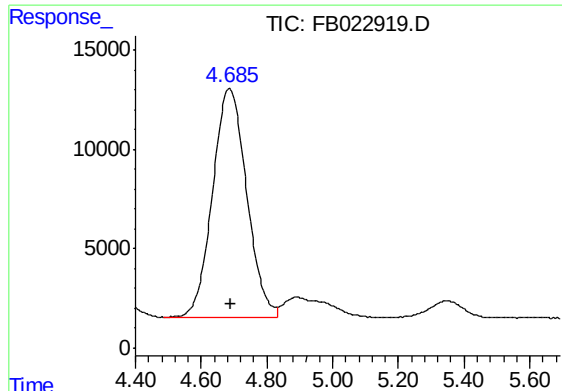

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 833764
Conc: 25.92 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MS

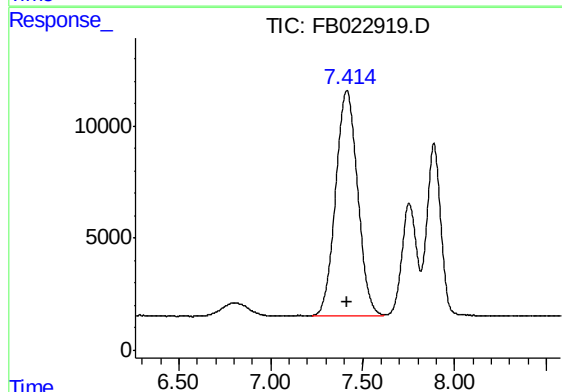


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 836557
Conc: 23.70 ng/ml

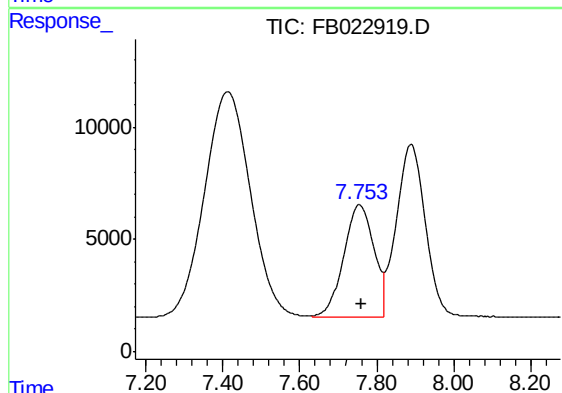


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 272140
Conc: 7.82 ng/ml

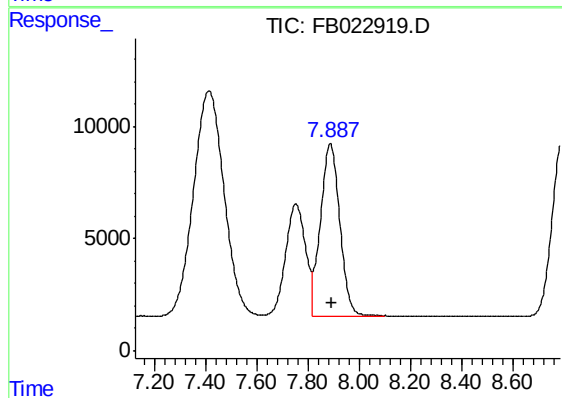

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.005 min
Response: 404518
Conc: 9.34 ng/ml

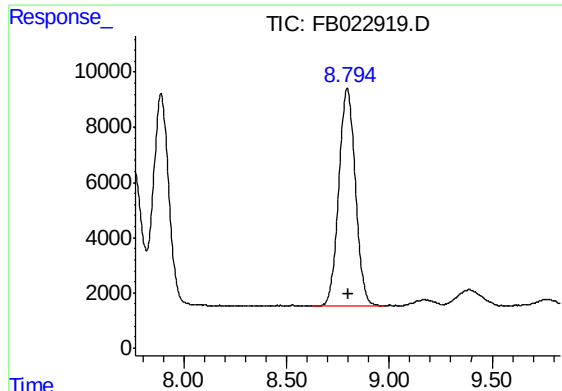

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 443154
Conc: 19.69 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MS

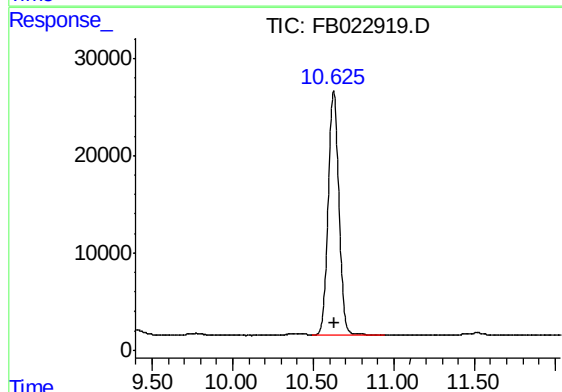


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.005 min
Response: 1173666
Conc: 27.22 ng/ml

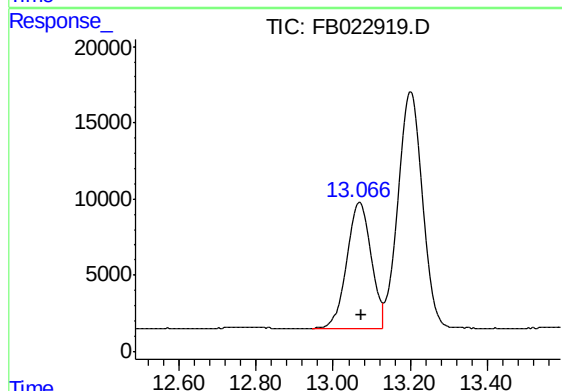


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 362711
Conc: 9.09 ng/ml

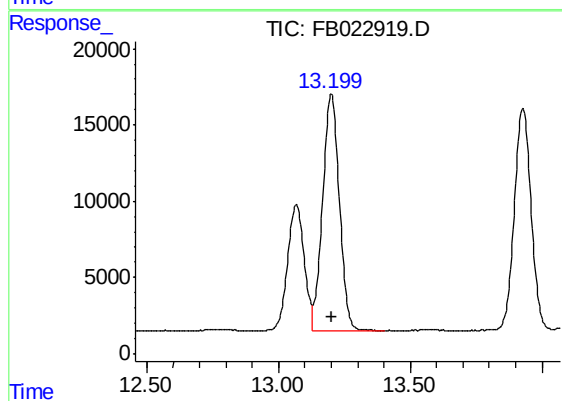

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 687402
Conc: 18.20 ng/ml

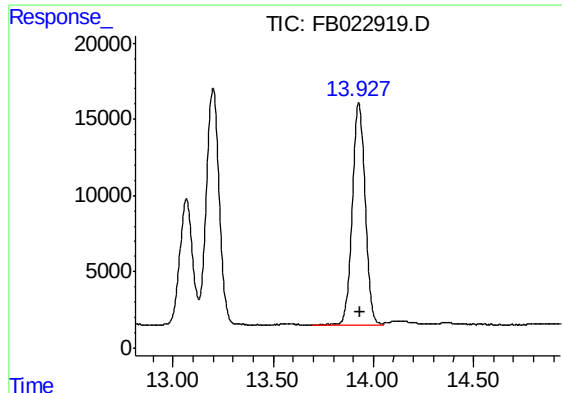

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 648375
Conc: 18.19 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-04-110619MS

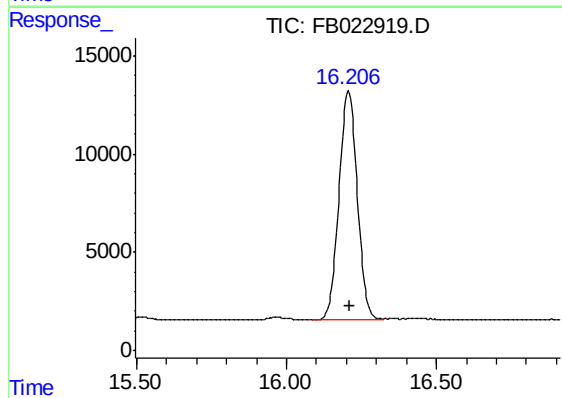

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 492509
Conc: 17.37 ng/ml