

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
 Data File : FB028845.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2022 10:29
 Operator : AJ/MA
 Sample : VBF1107S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 08 03:12:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	301344	23.714 ng/ml
Target Compounds			
9) t O-Xylene	13.885	22471	1.225 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
Data File : FB028845.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2022 10:29
Operator : AJ/MA
Sample : VBF1107S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 08 03:12:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

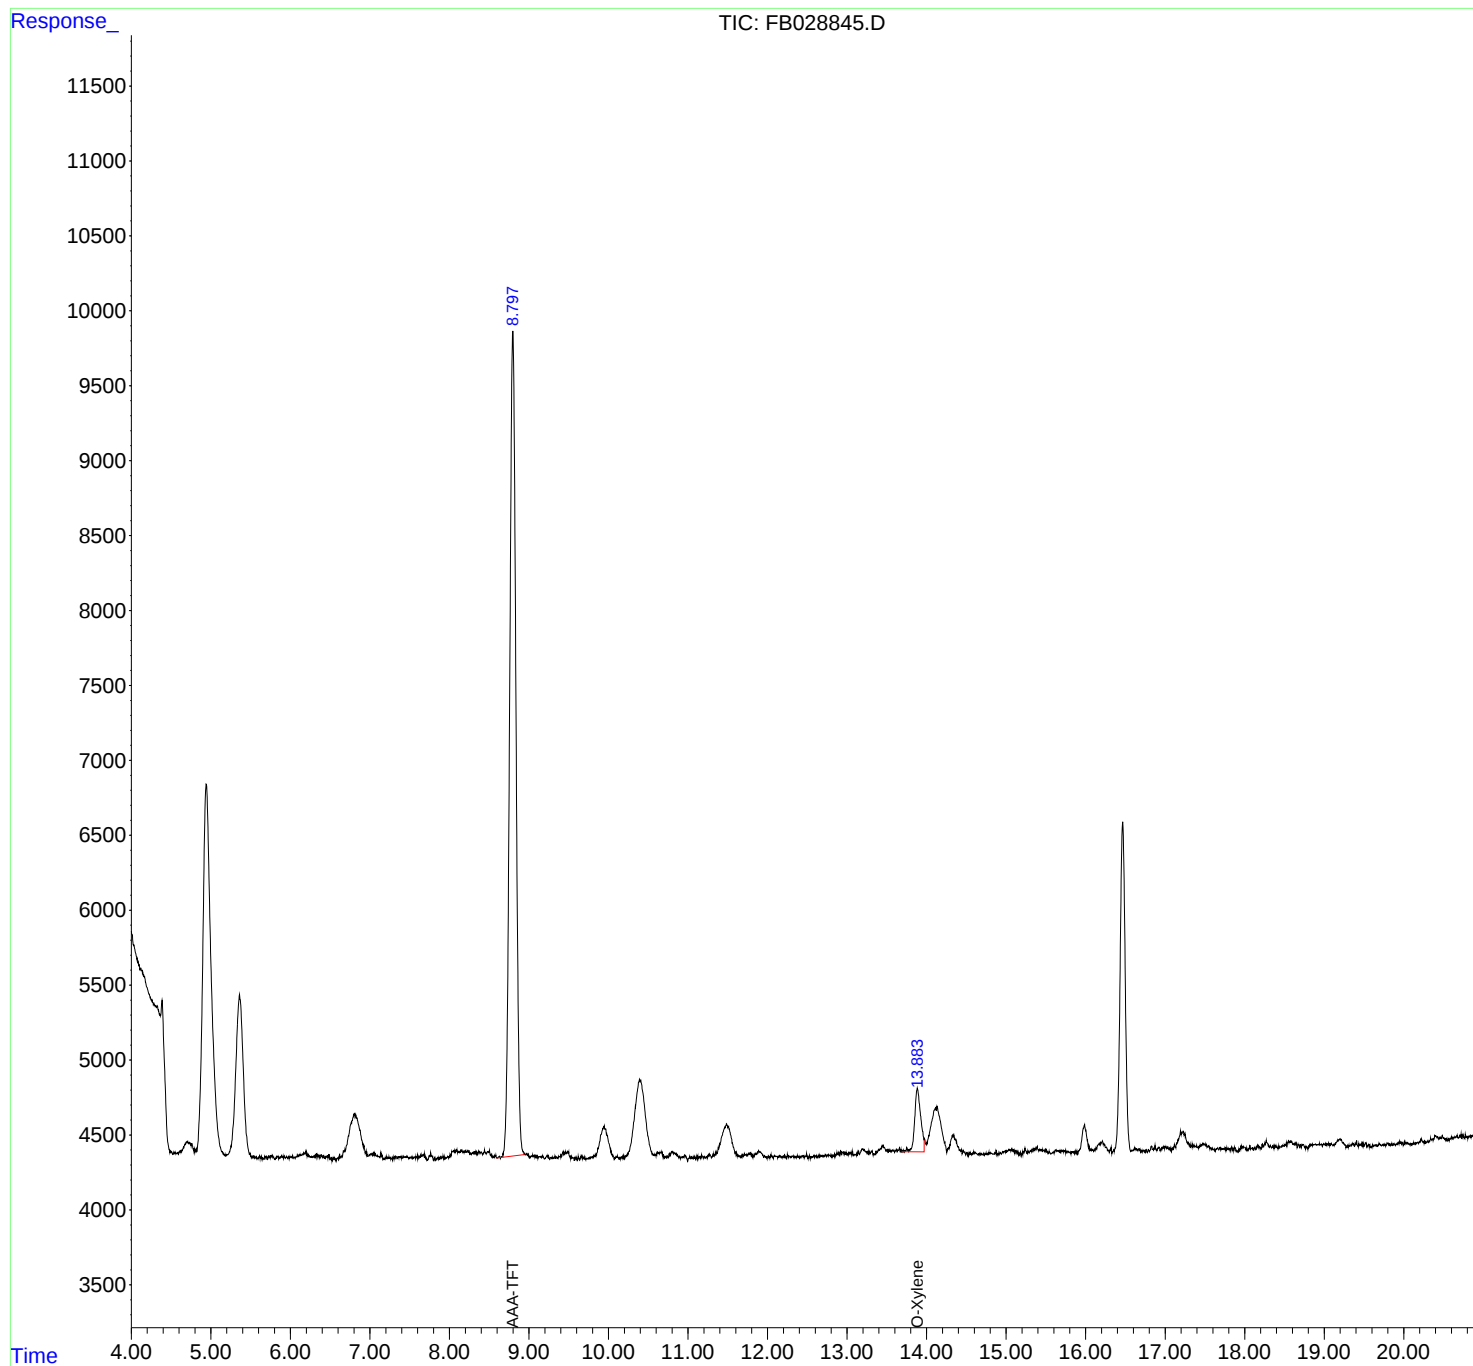


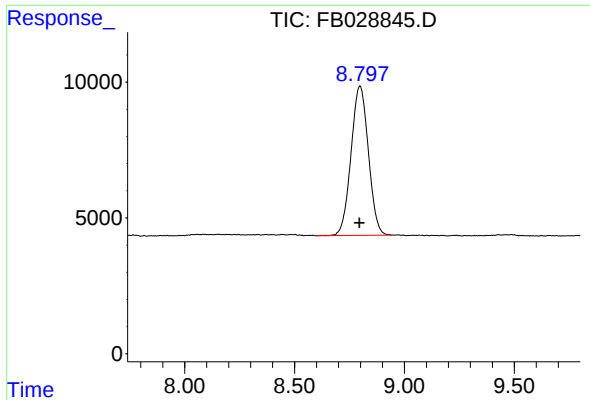

#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.003 min
Response: 301344
Conc: 23.71 ng/ml

Instrument :
FID_B
ClientSampleId :

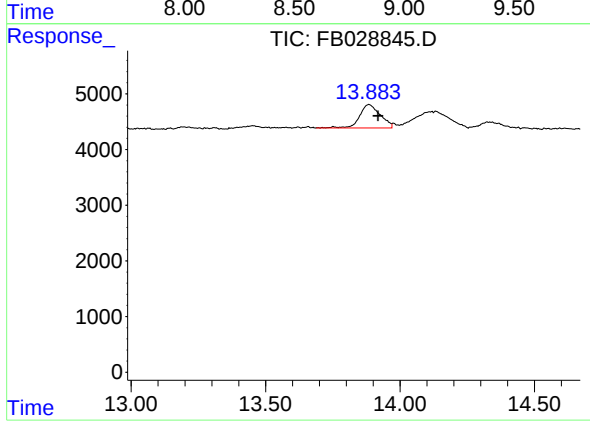

#9 O-Xylene

R.T.: 13.885 min
Delta R.T.: -0.033 min
Response: 22471
Conc: 1.22 ng/ml