

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
 Data File : FB028849.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2022 13:03
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 08 03:13:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.805	335386	26.393 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.424	775	0.044 ng/ml
3) t n-Heptane	7.779	34676	1.972 ng/ml
4) t Benzene	7.896	3702	0.181 ng/ml
6) t Toluene	10.633	151407	7.528 ng/ml
7) t Ethylbenzene	13.069	66690	3.516 ng/ml
8) t m-Xylene	13.199	265374	14.106 ng/ml
9) t O-Xylene	13.932	302611	16.495 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	204846	11.120 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
Data File : FB028849.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2022 13:03
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 08 03:13:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

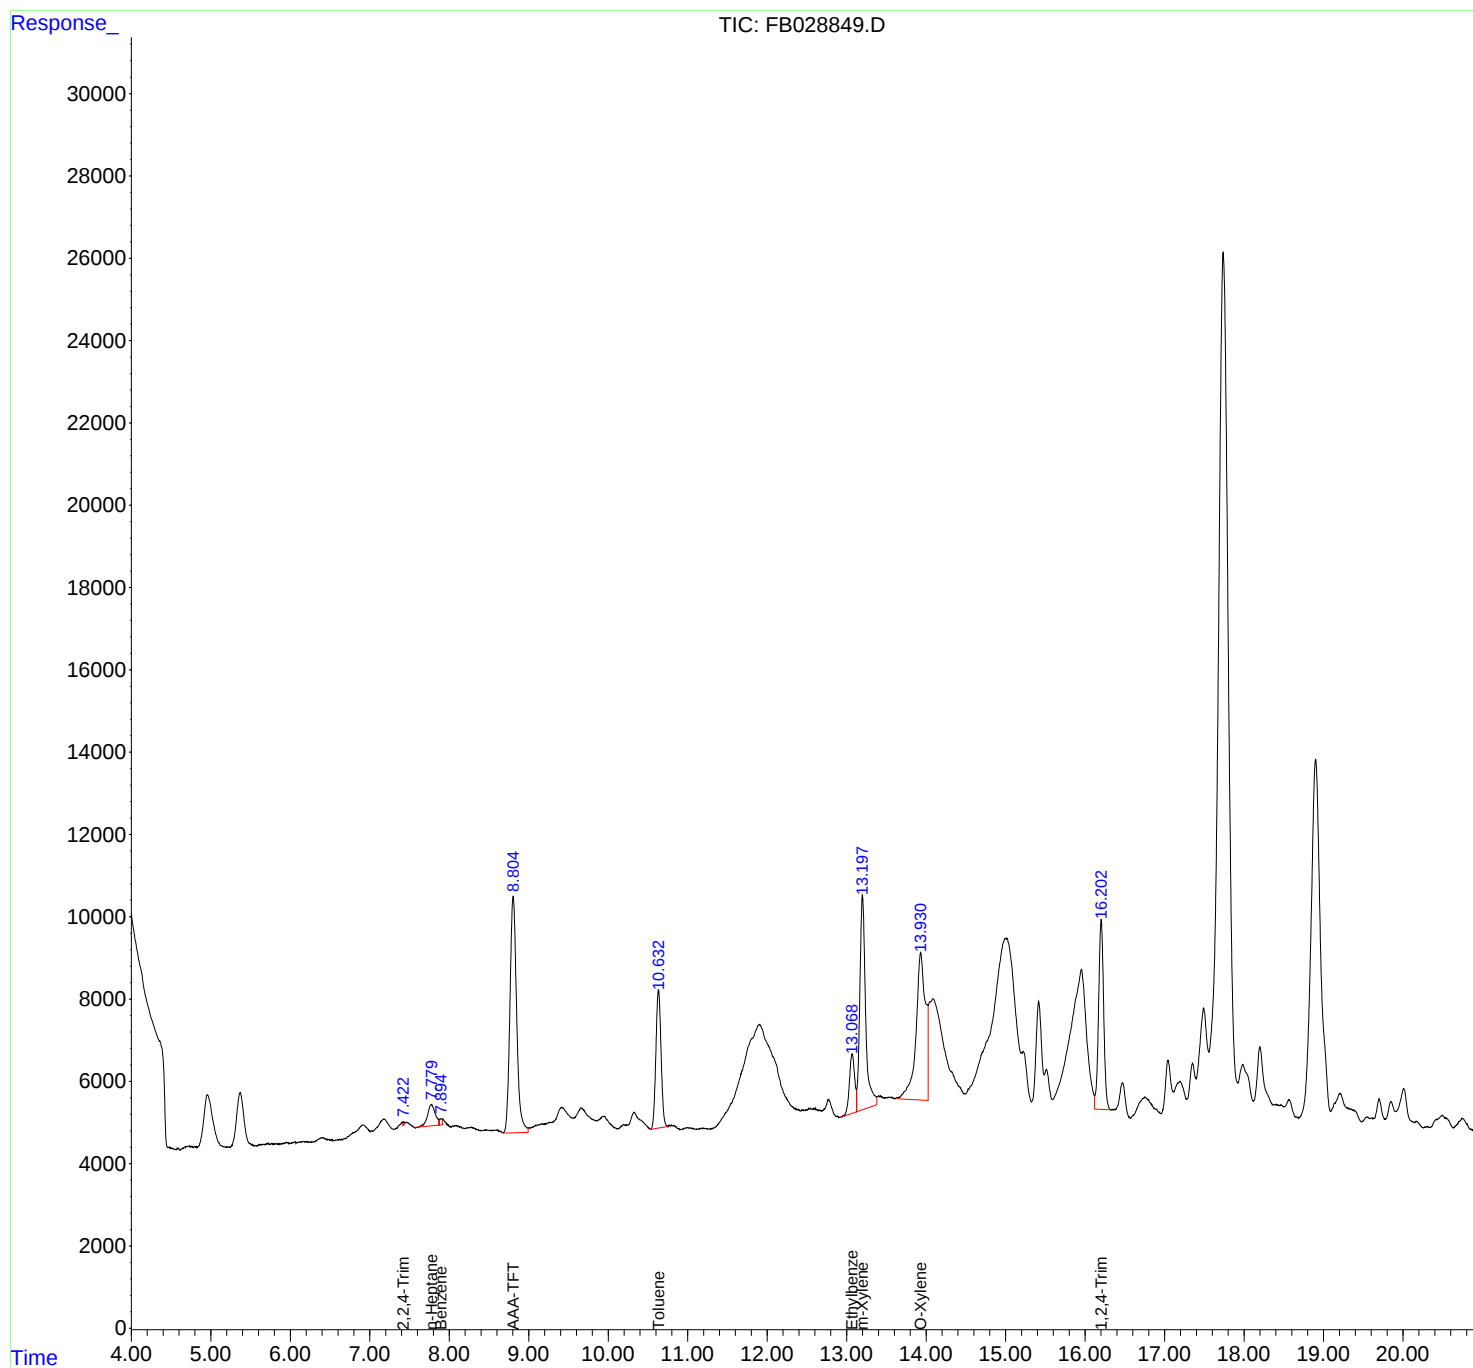


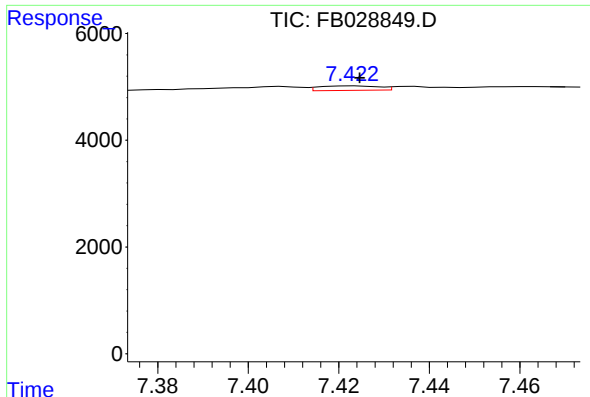

#2 2,2,4-Trimethylpentane


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 775
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :

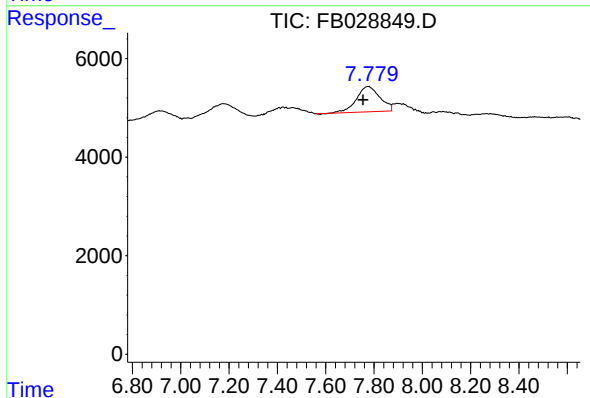


#3 n-Heptane

R.T.: 7.779 min
Delta R.T.: 0.025 min
Response: 34676
Conc: 1.97 ng/ml

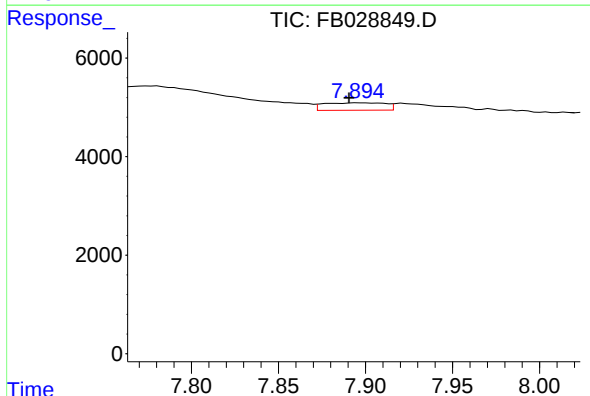


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.006 min
Response: 3702
Conc: 0.18 ng/ml

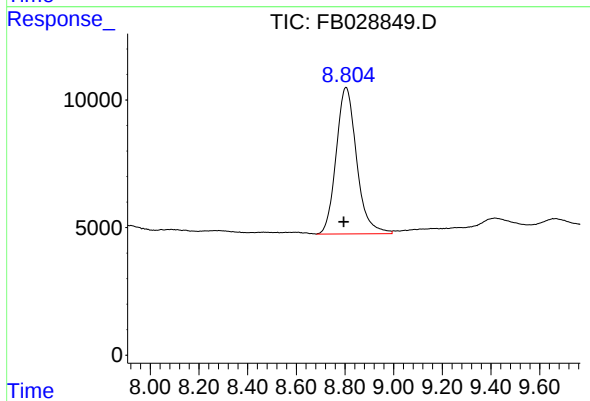

#5 AAA-TFT


R.T.: 8.805 min
Delta R.T.: 0.010 min
Response: 335386
Conc: 26.39 ng/ml

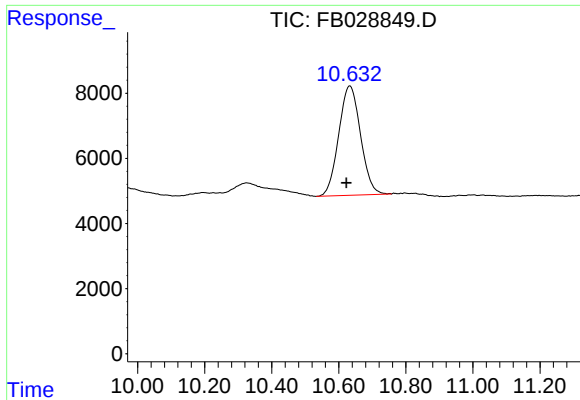

#6 Toluene


R.T.: 10.633 min
Delta R.T.: 0.011 min
Response: 151407
Conc: 7.53 ng/ml

Instrument :
FID_B
ClientSampleId :

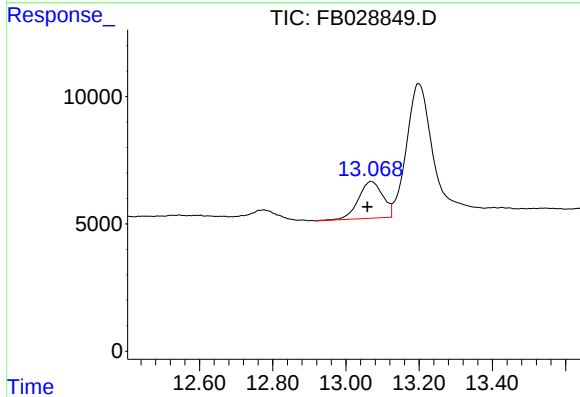


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.011 min
Response: 66690
Conc: 3.52 ng/ml

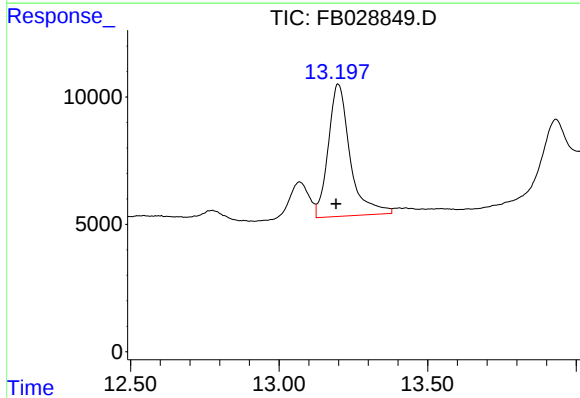


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.007 min
Response: 265374
Conc: 14.11 ng/ml

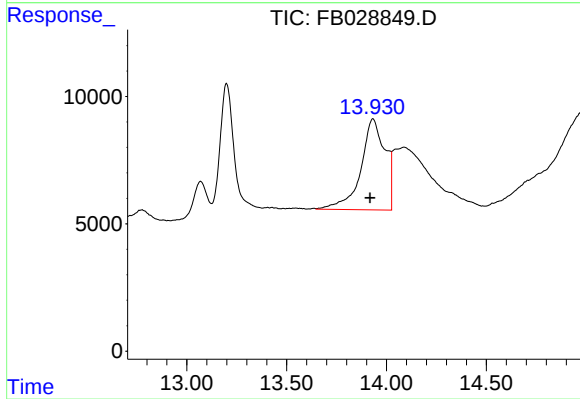

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.014 min
Response: 302611
Conc: 16.50 ng/ml

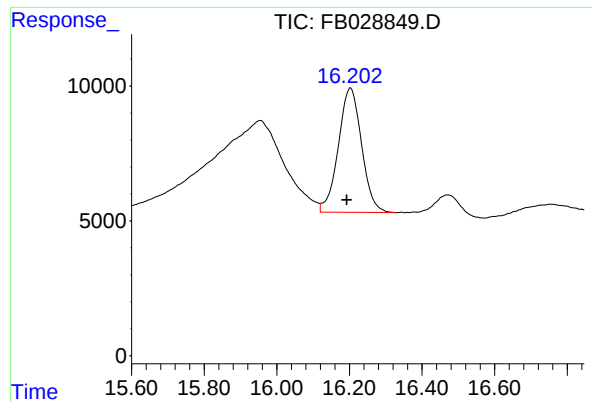

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.011 min
Response: 204846
Conc: 11.12 ng/ml

Instrument :

FID_B

ClientSampleId :