

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
 Data File : FB028850.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2022 13:40
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 08 03:13:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	285676	22.481 ng/ml
Target Compounds			
6) t Toluene	10.633	35331	1.757 ng/ml
7) t Ethylbenzene	13.063	9532	0.503 ng/ml
8) t m-Xylene	13.195	38670	2.055 ng/ml
9) t O-Xylene	13.907	41583	2.267 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	33696	1.829 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
Data File : FB028850.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2022 13:40
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 08 03:13:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

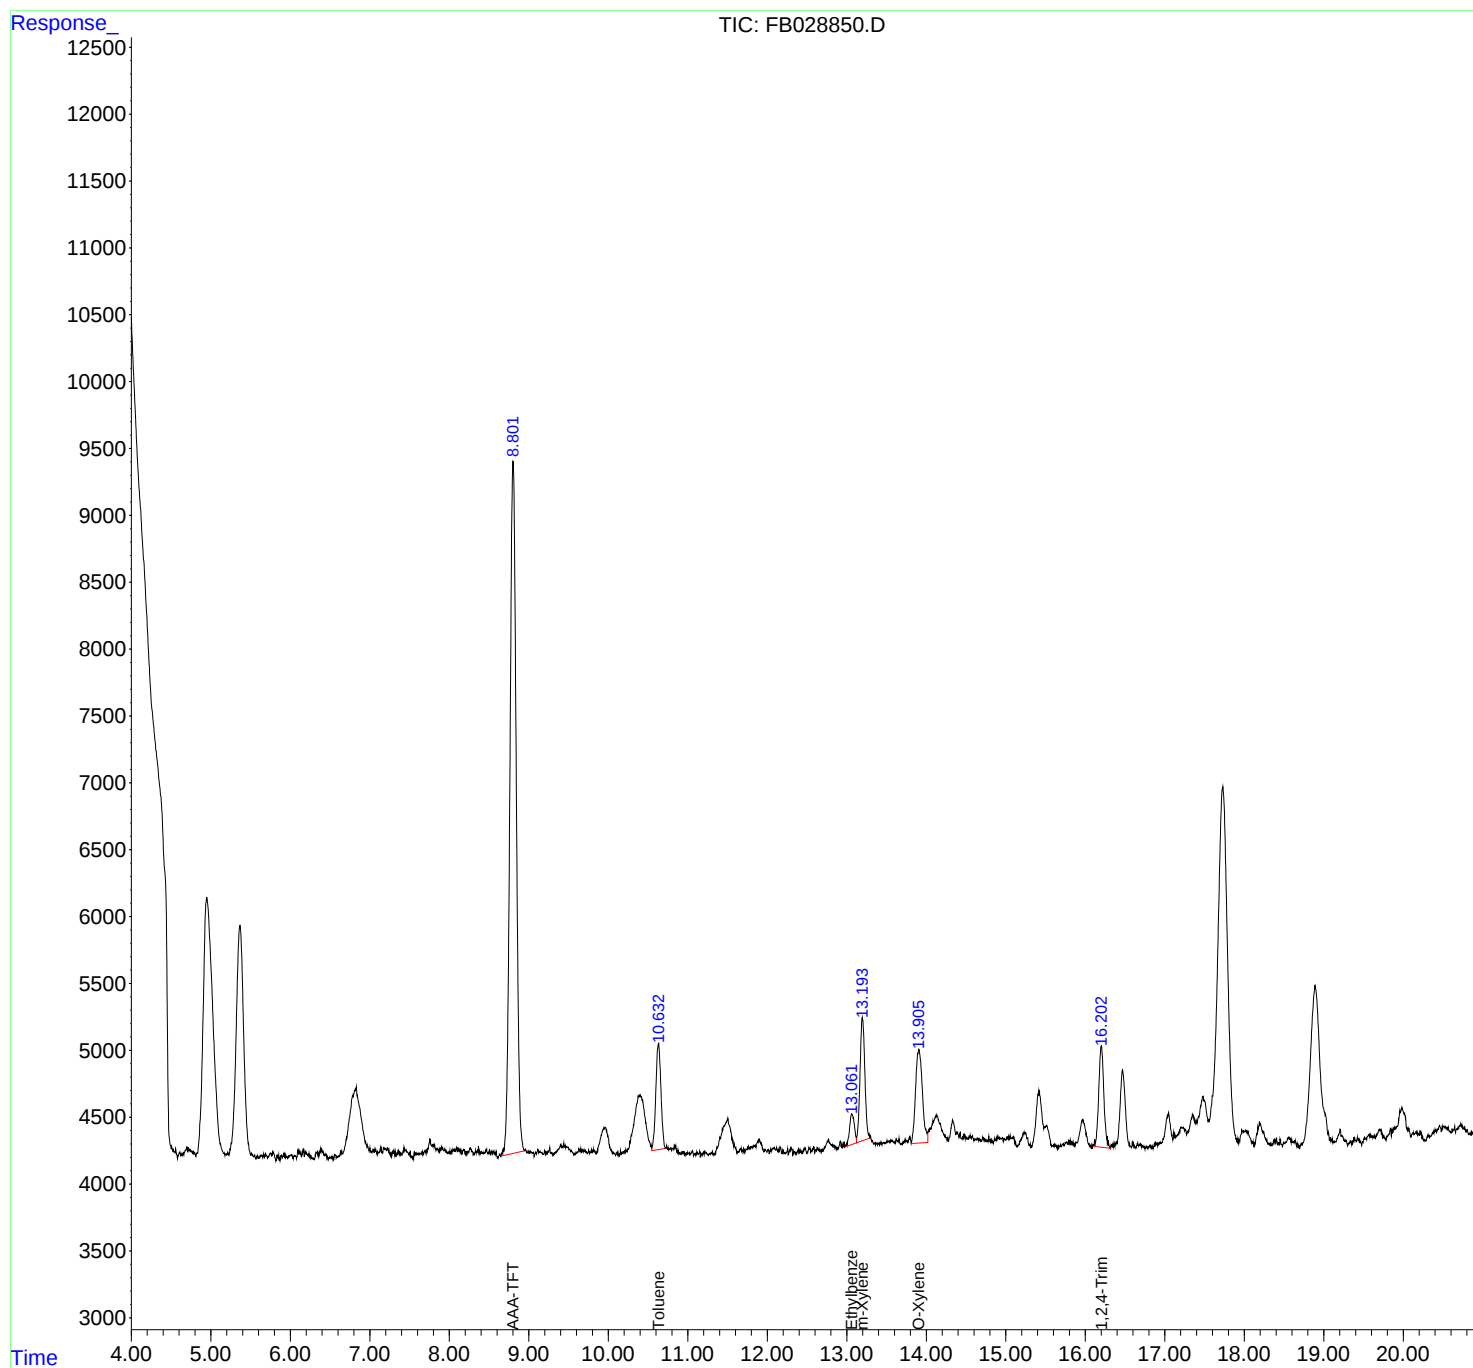


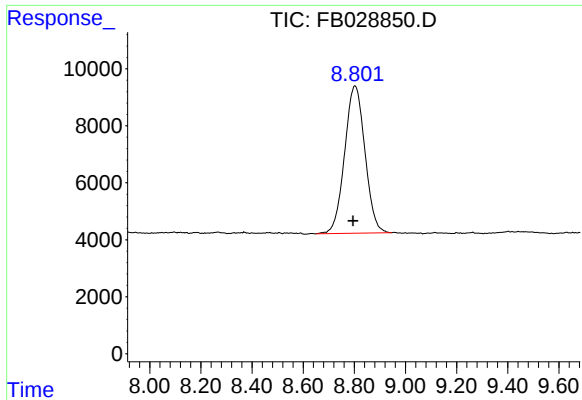

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.008 min
Response: 285676
Conc: 22.48 ng/ml

Instrument :
FID_B
ClientSampleId :

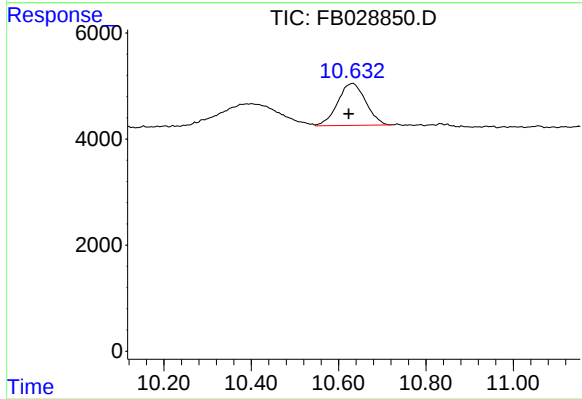


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.010 min
Response: 35331
Conc: 1.76 ng/ml

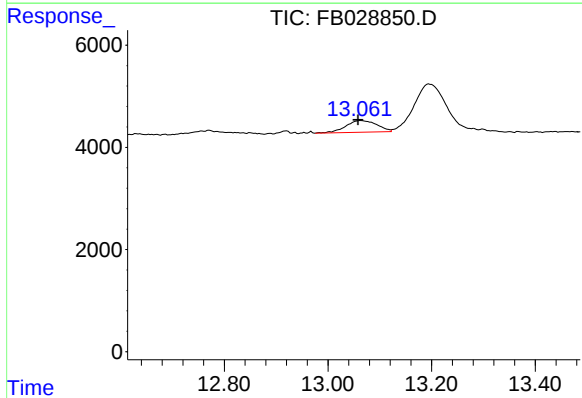


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.005 min
Response: 9532
Conc: 0.50 ng/ml

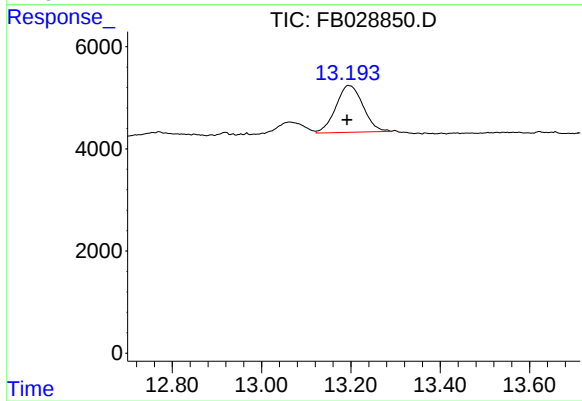

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.003 min
Response: 38670
Conc: 2.06 ng/ml

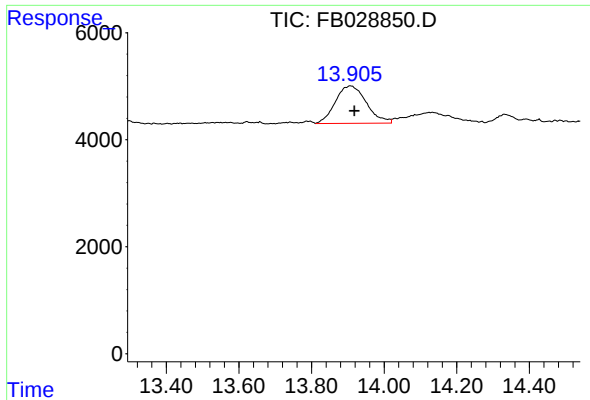

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.011 min
Response: 41583
Conc: 2.27 ng/ml

Instrument :
FID_B
ClientSampleId :

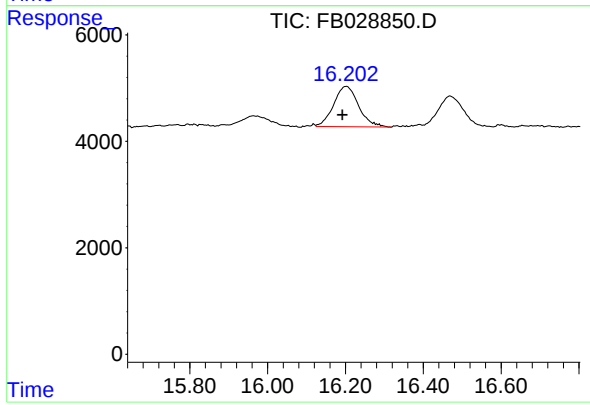

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.011 min
Response: 33696
Conc: 1.83 ng/ml