

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
 Data File : FB028854.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2022 16:12
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 08 03:13:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	263479	20.734 ng/ml
Target Compounds			
6) t Toluene	10.628	8016	0.399 ng/ml
8) t m-Xylene	13.201	9744	0.518 ng/ml
9) t O-Xylene	13.891	26767	1.459 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	8332	0.452 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
Data File : FB028854.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2022 16:12
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 08 03:13:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

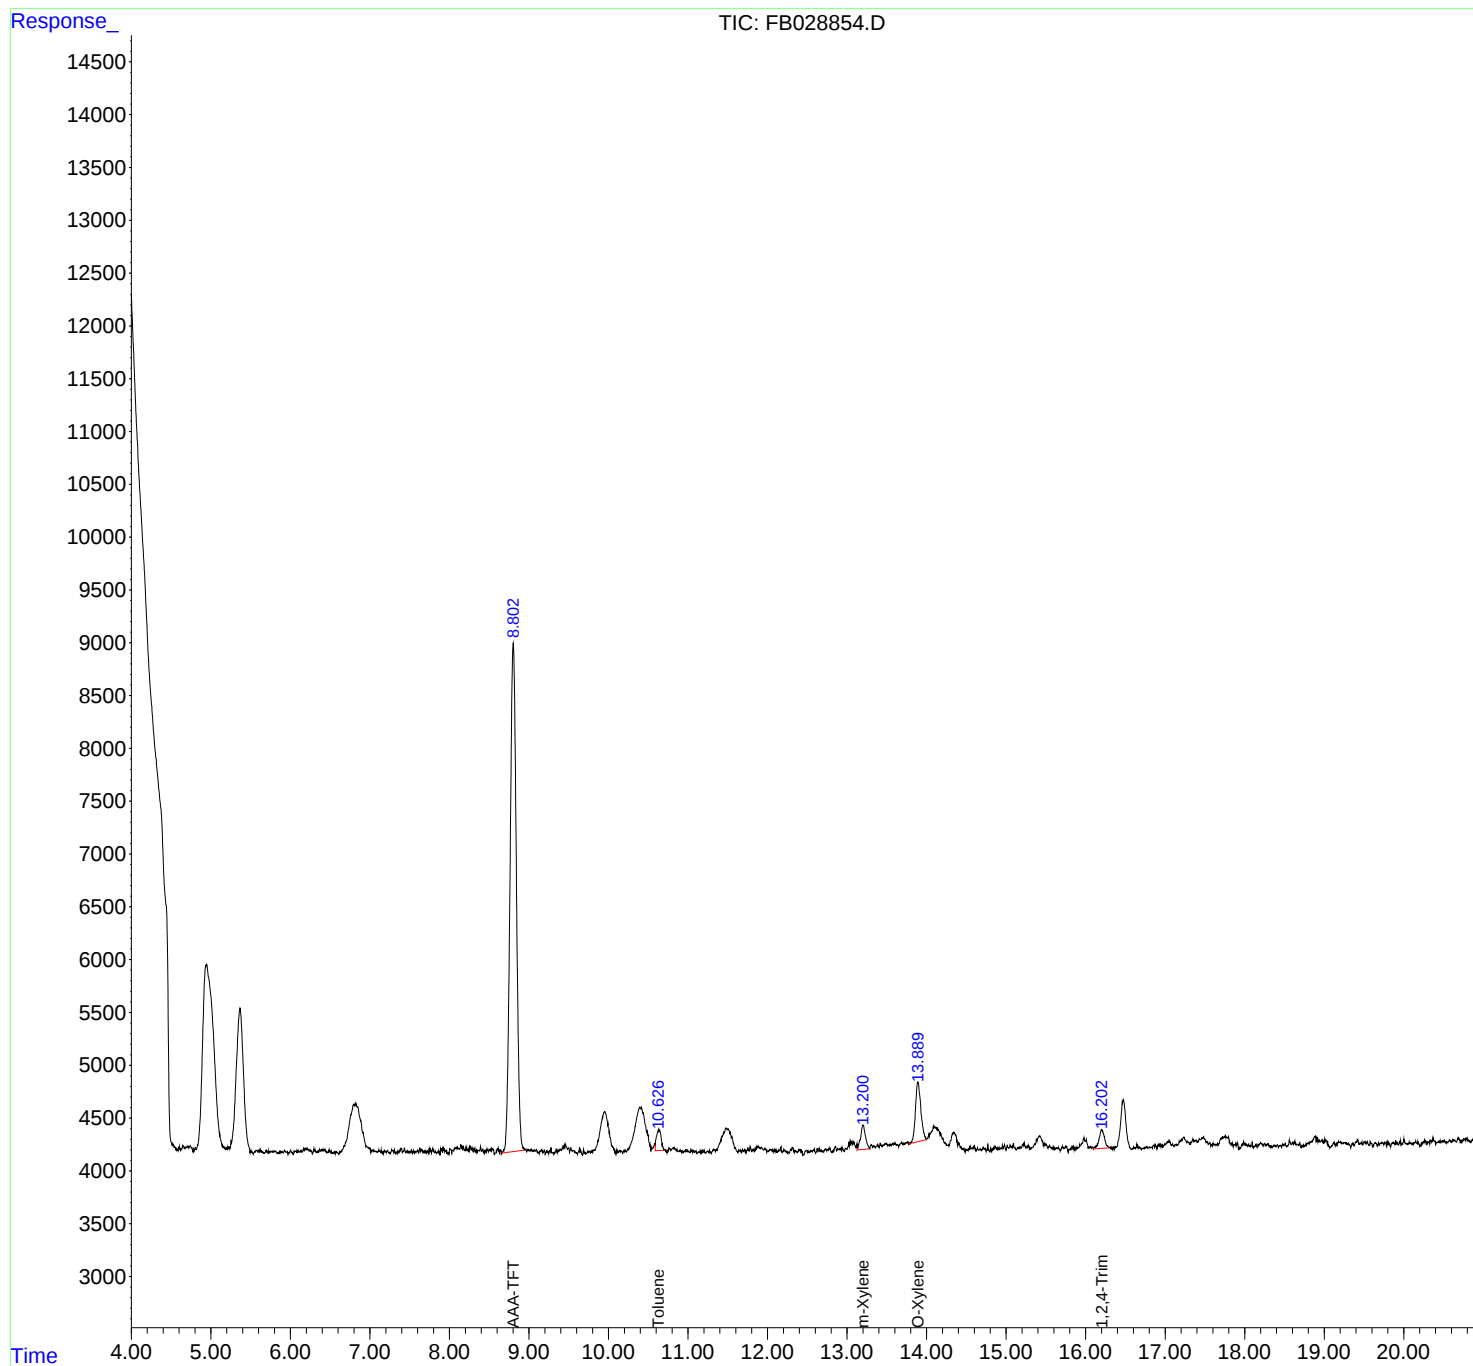


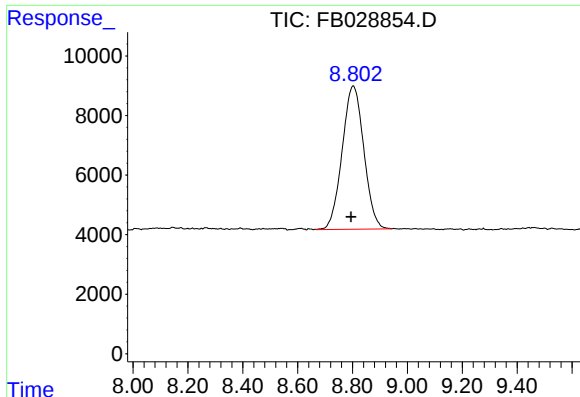

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.008 min
Response: 263479
Conc: 20.73 ng/ml

Instrument :
FID_B
ClientSampleId :

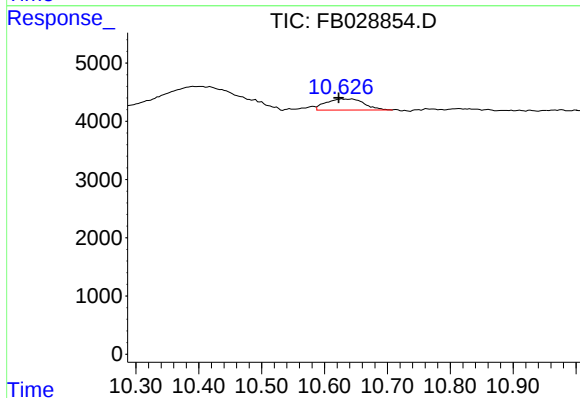


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.005 min
Response: 8016
Conc: 0.40 ng/ml

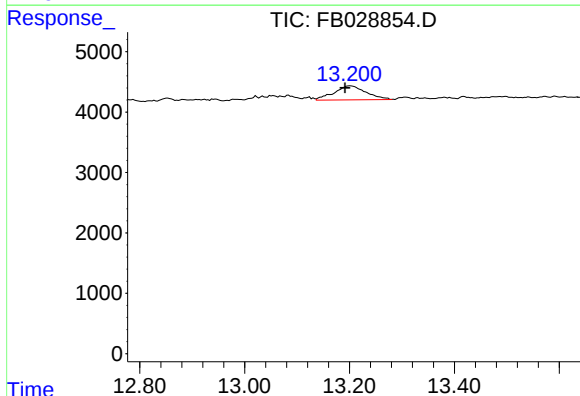


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.010 min
Response: 9744
Conc: 0.52 ng/ml

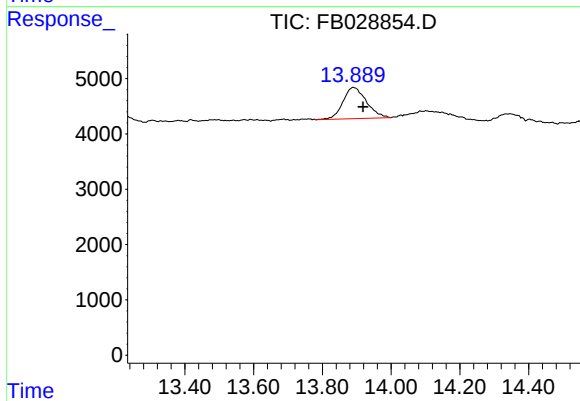

#9 O-Xylene

R.T.: 13.891 min
Delta R.T.: -0.027 min
Response: 26767
Conc: 1.46 ng/ml

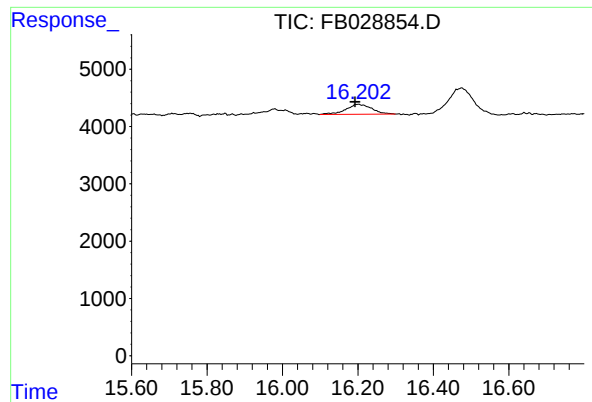

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.011 min
Response: 8332
Conc: 0.45 ng/ml

Instrument :

FID_B

ClientSampleId :