

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
 Data File : FB028847.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2022 11:45
 Operator : AJ/MA
 Sample : BSF1107S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1107S1

Integration File: Calibration.e
 Quant Time: Nov 08 03:12:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	280817	22.099 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	448848	27.537 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	551839	31.406 ng/ml
3) t n-Heptane	7.759	186119	10.586 ng/ml
4) t Benzene	7.896	218350	10.648 ng/ml
6) t Toluene	10.629	632198	31.432 ng/ml
7) t Ethylbenzene	13.064	195846	10.326 ng/ml
8) t m-Xylene	13.197	390098	20.736 ng/ml
9) t O-Xylene	13.923	396527	21.615 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	360860	19.588 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110722\
Data File : FB028847.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2022 11:45
Operator : AJ/MA
Sample : BSF1107S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1107S1

Integration File: Calibration.e
Quant Time: Nov 08 03:12:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

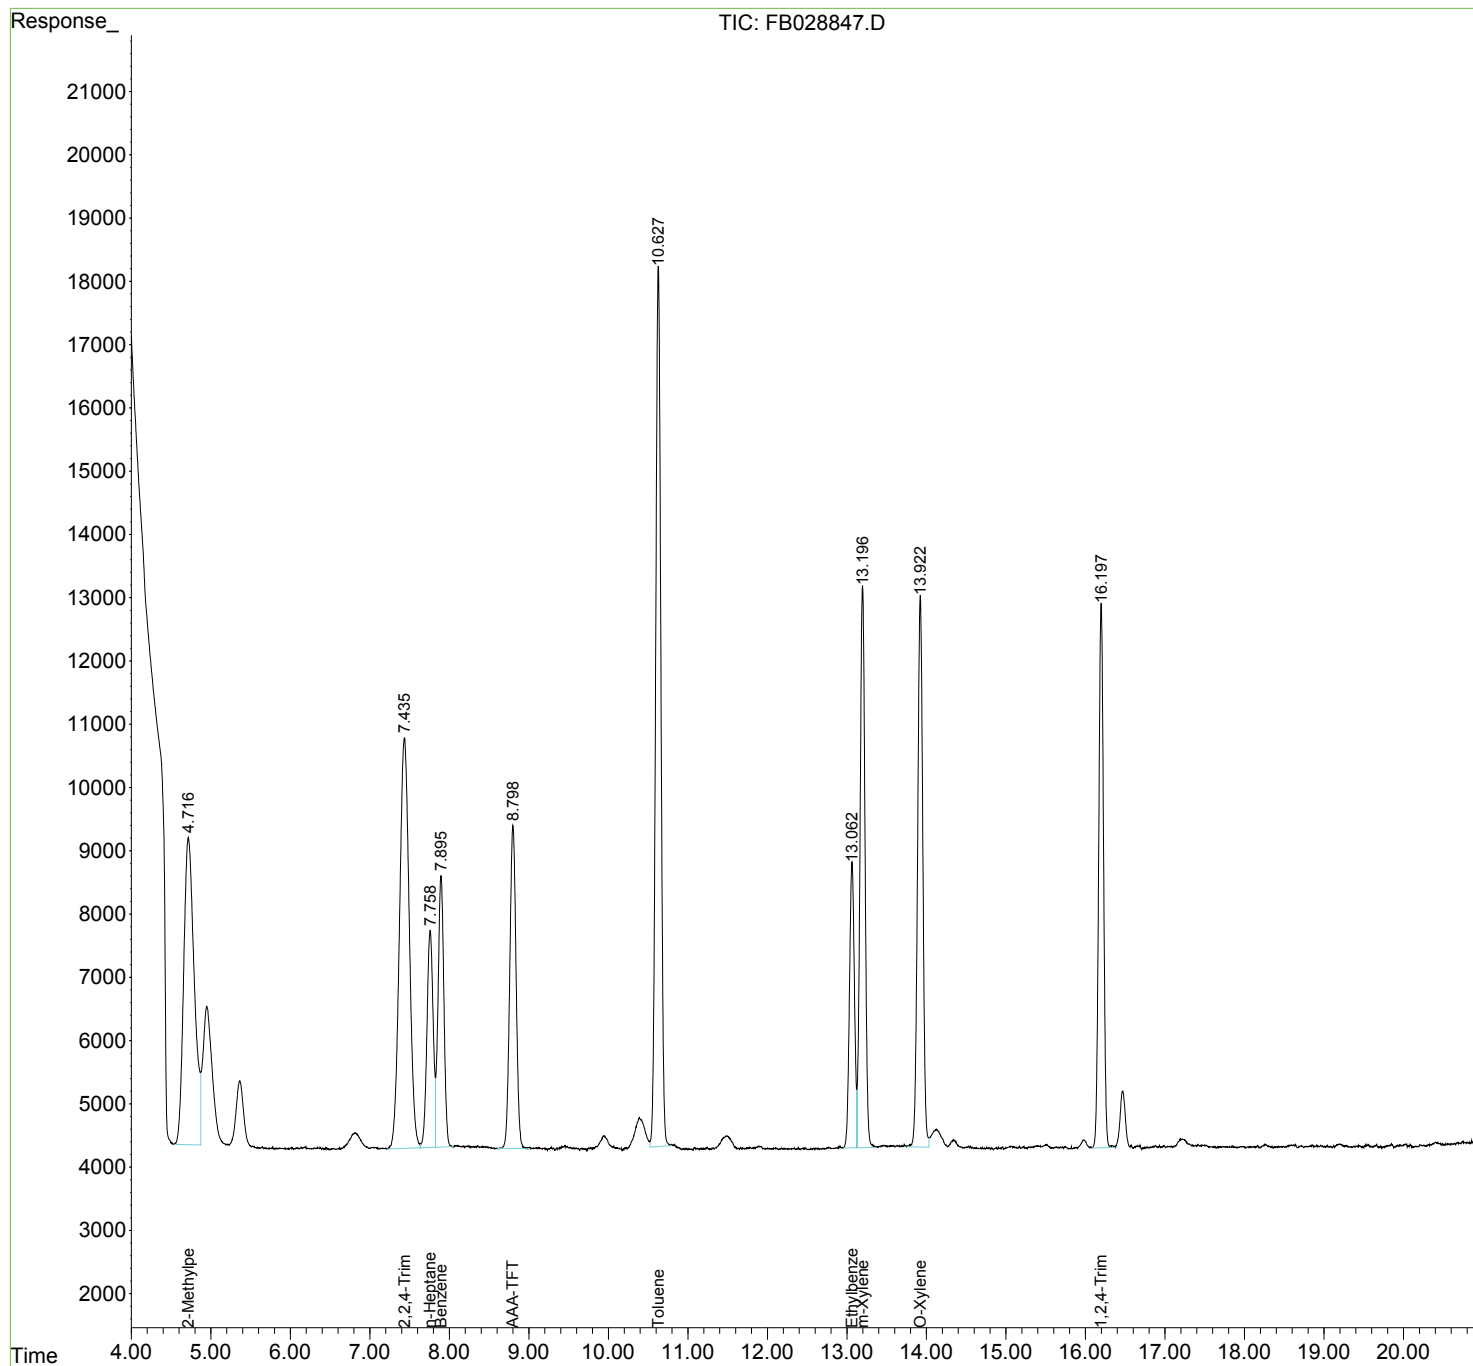


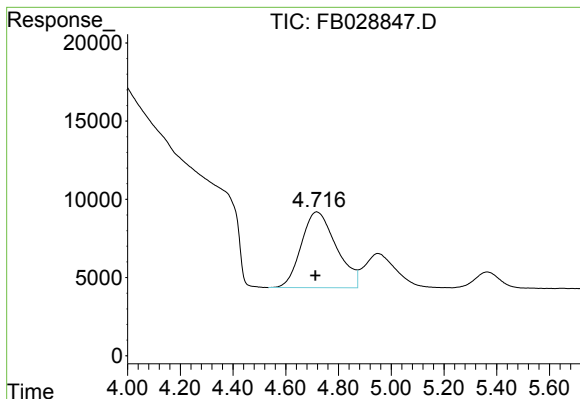

#1 2-Methylpentane


R.T.: 4.718 min
 Delta R.T.: 0.006 min
 Response: 448848
 Conc: 27.54 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 BSF1107S1

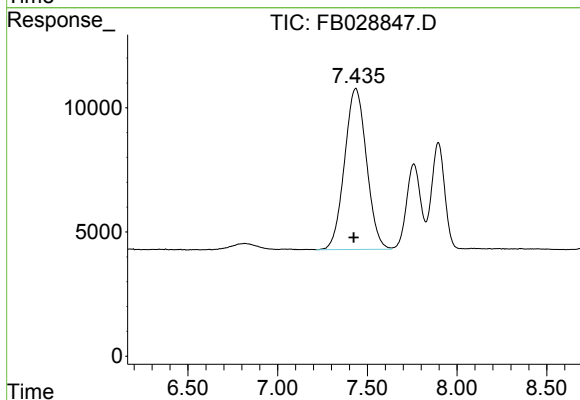


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
 Delta R.T.: 0.012 min
 Response: 551839
 Conc: 31.41 ng/ml

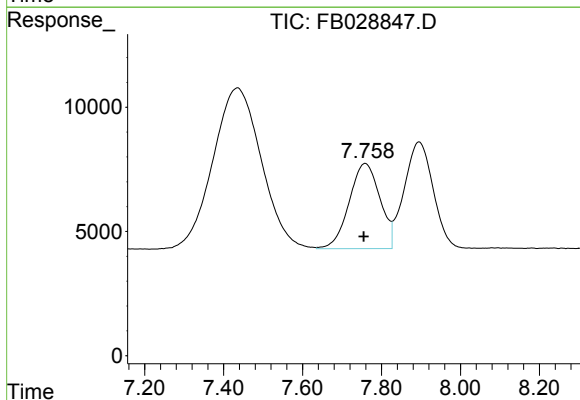


#3 n-Heptane

R.T.: 7.759 min
 Delta R.T.: 0.005 min
 Response: 186119
 Conc: 10.59 ng/ml

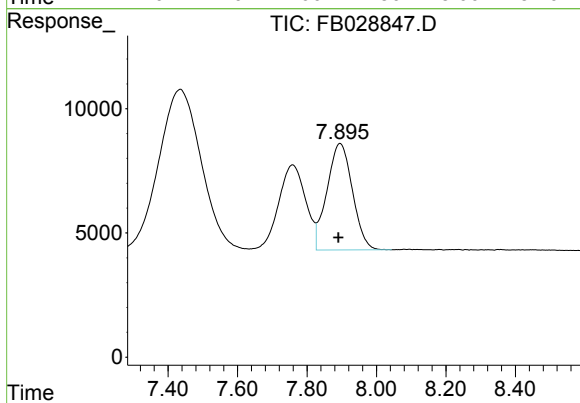

#4 Benzene


R.T.: 7.896 min
 Delta R.T.: 0.005 min
 Response: 218350
 Conc: 10.65 ng/ml

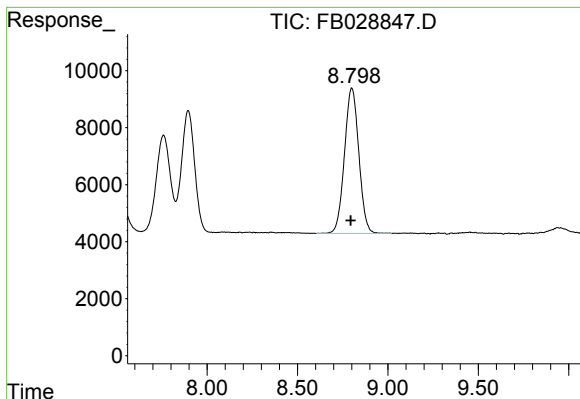

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.005 min
Response: 280817
Conc: 22.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S1

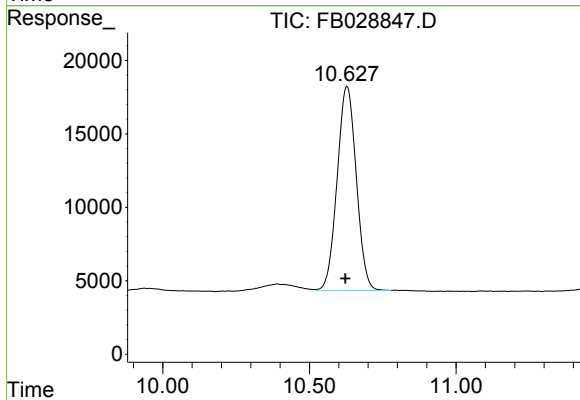


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.006 min
Response: 632198
Conc: 31.43 ng/ml

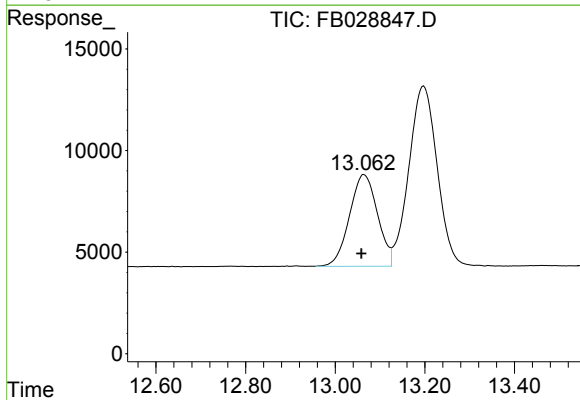


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.006 min
Response: 195846
Conc: 10.33 ng/ml

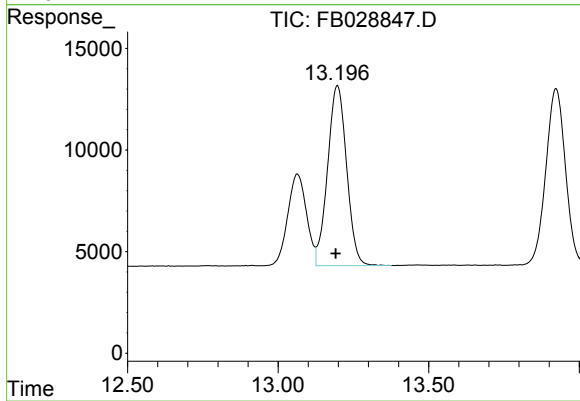

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.006 min
Response: 390098
Conc: 20.74 ng/ml

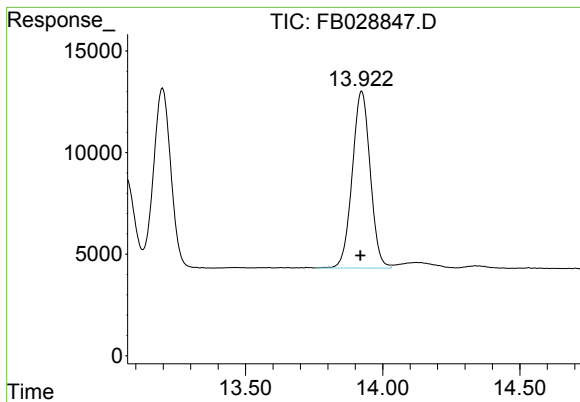

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.005 min
Response: 396527
Conc: 21.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1107S1

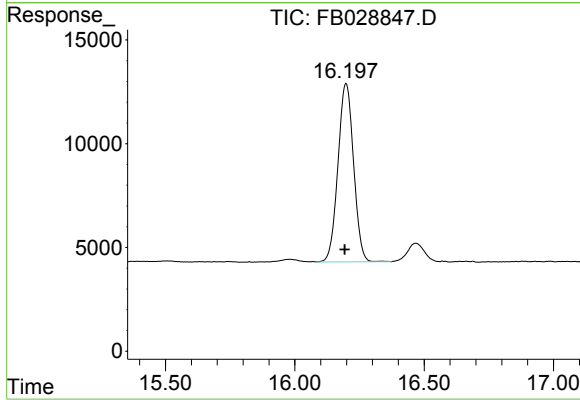

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.006 min
Response: 360860
Conc: 19.59 ng/ml