

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
 Data File : FB030450.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2023 14:43
 Operator : YP/AJ
 Sample : 05102-13
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 07 21:55:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.849	1281022	112.195 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	42644	3.048 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	193565	11.724 ng/ml
4) t Benzene	7.841	3868780	188.567 ng/ml
6) t Toluene	10.637	256511	12.705 ng/ml
7) t Ethylbenzene	13.030	3446898	172.686 ng/ml
8) t m-Xylene	13.174	1192723	60.515 ng/ml
9) t O-Xylene	13.912	4995137	253.797 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	180066	8.717 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030450.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 14:43
Operator : YP/AJ
Sample : 05102-13
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 21:55:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

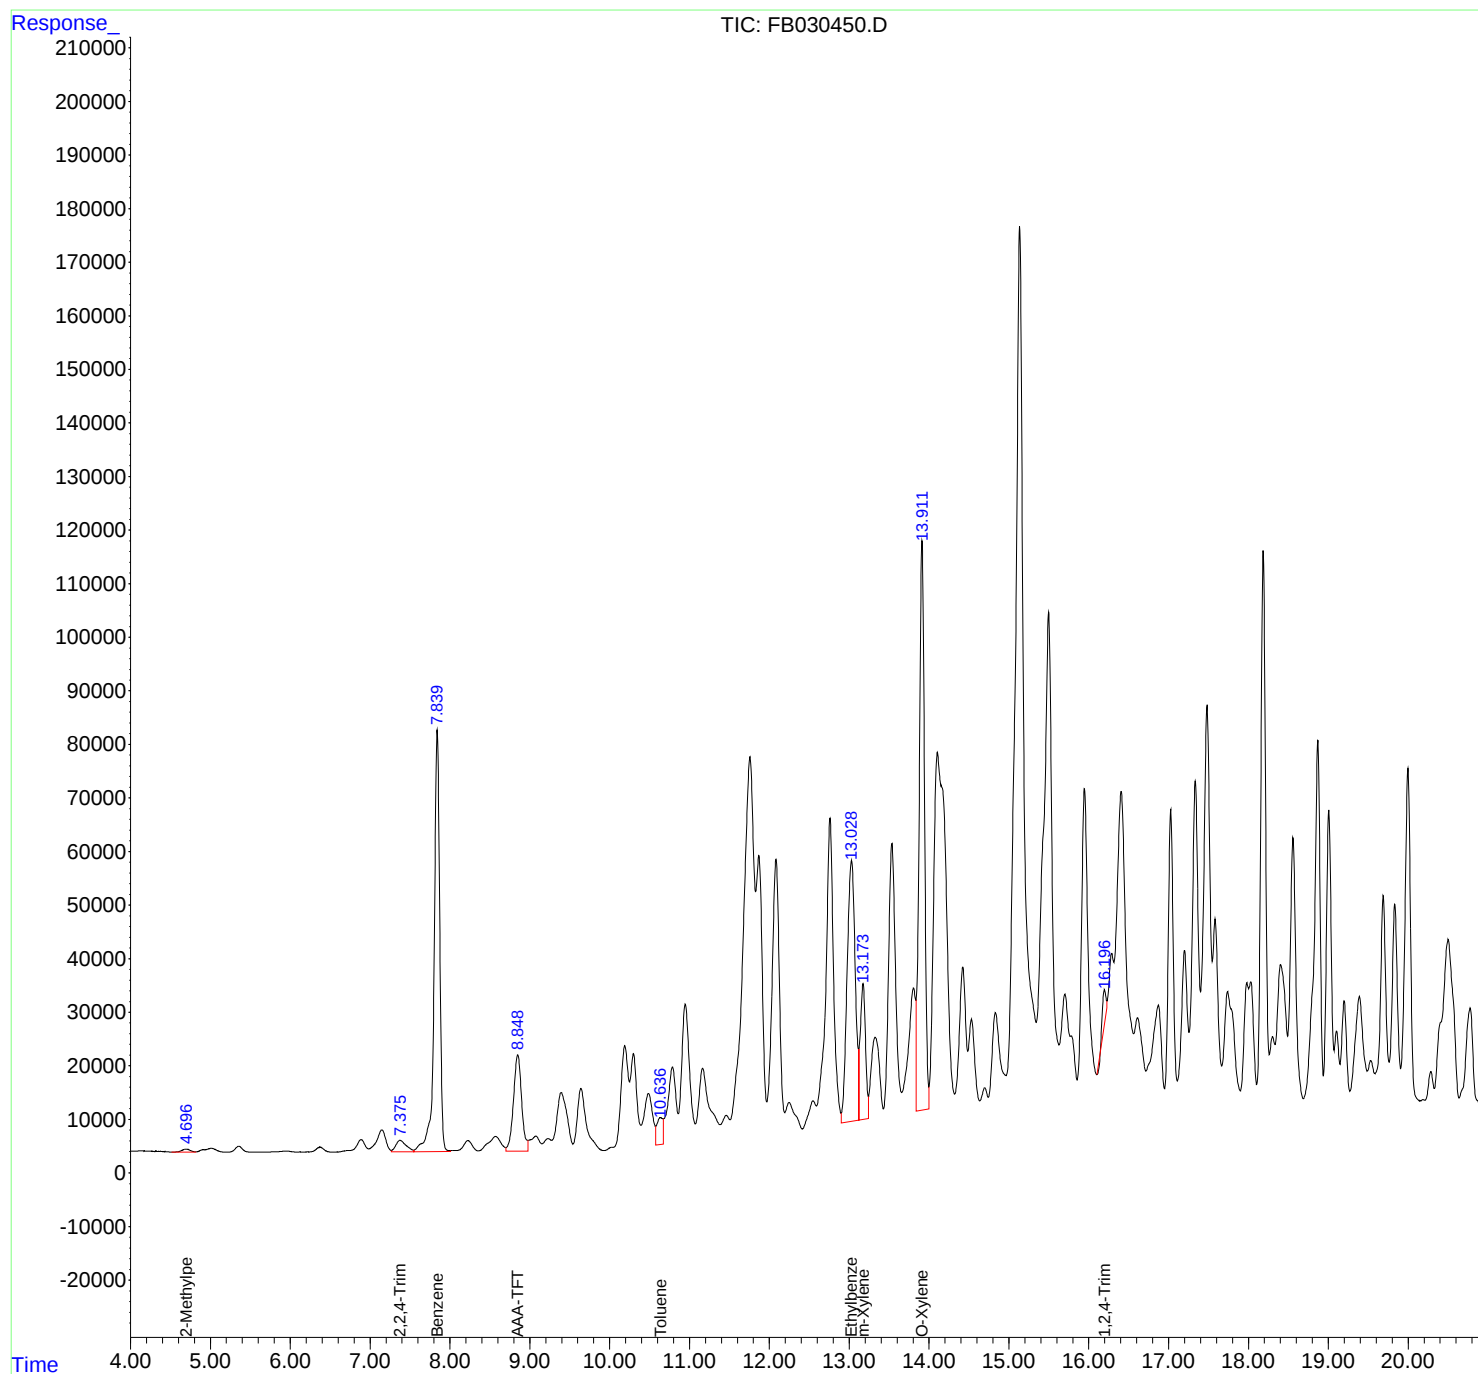


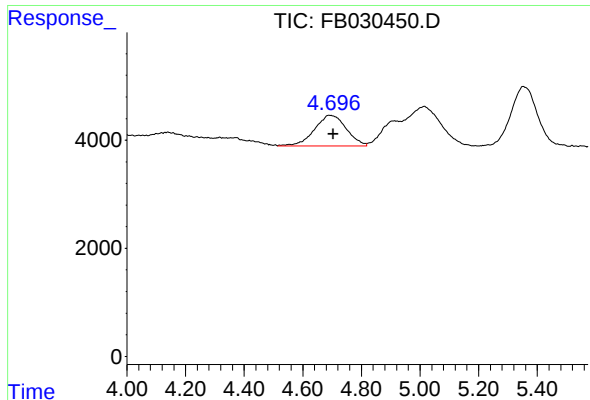

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.006 min
Response: 42644
Conc: 3.05 ng/ml

Instrument :
FID_B
ClientSampleId :

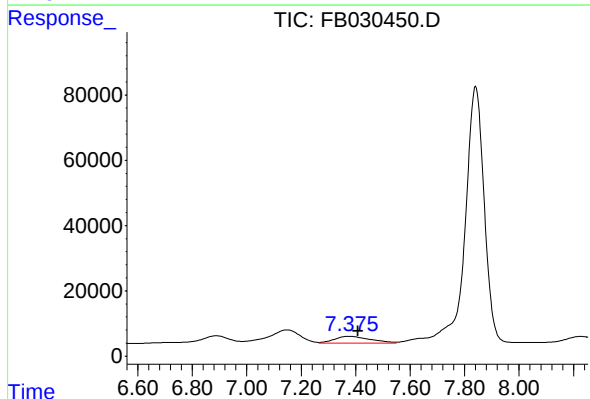


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.033 min
Response: 193565
Conc: 11.72 ng/ml

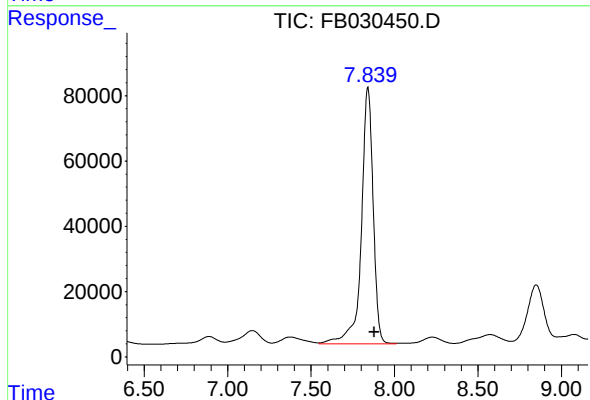


#4 Benzene

R.T.: 7.841 min
Delta R.T.: -0.039 min
Response: 3868780
Conc: 188.57 ng/ml

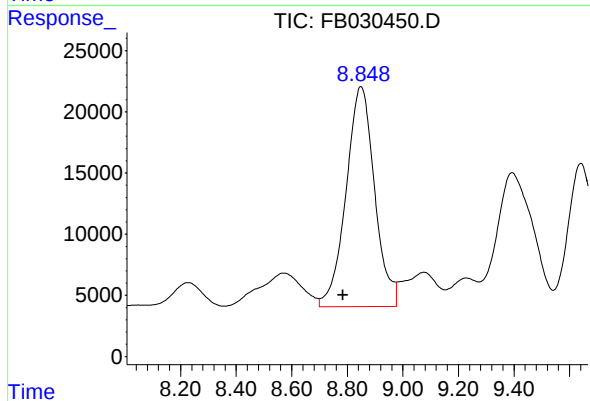

#5 AAA-TFT


R.T.: 8.849 min
Delta R.T.: 0.065 min
Response: 1281022
Conc: 112.20 ng/ml

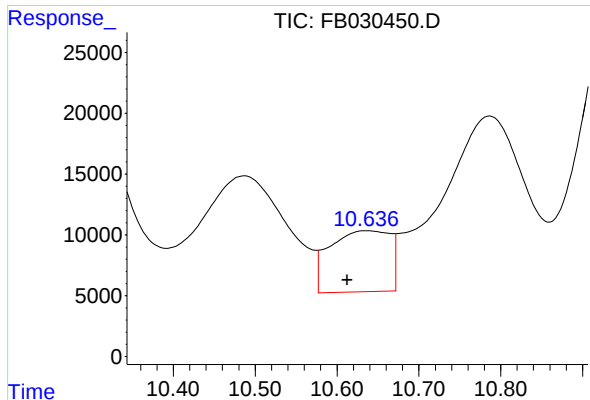

#6 Toluene


R.T.: 10.637 min
Delta R.T.: 0.024 min
Response: 256511
Conc: 12.71 ng/ml

Instrument :
FID_B
ClientSampleId :

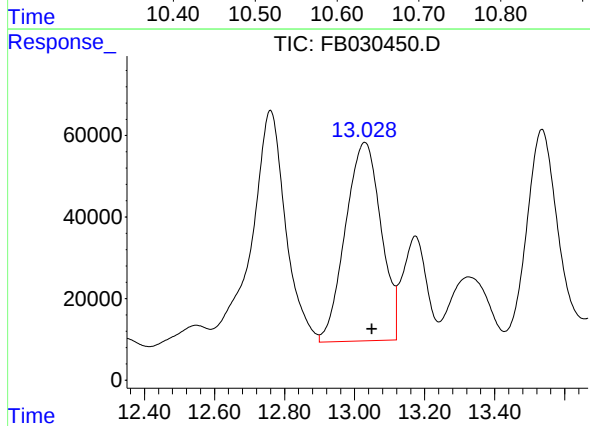


#7 Ethylbenzene

R.T.: 13.030 min
Delta R.T.: -0.020 min
Response: 3446898
Conc: 172.69 ng/ml

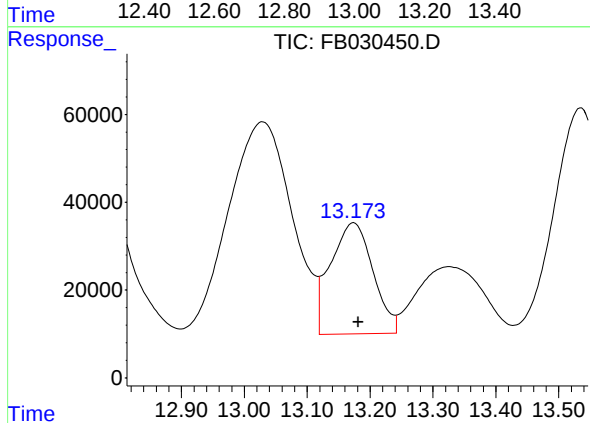


#8 m-Xylene

R.T.: 13.174 min
Delta R.T.: -0.007 min
Response: 1192723
Conc: 60.51 ng/ml

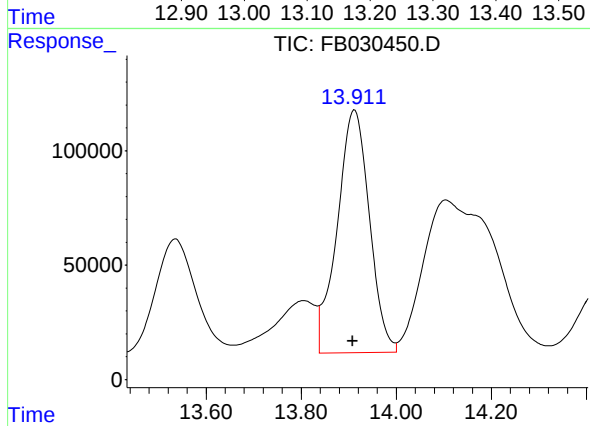

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.004 min
Response: 4995137
Conc: 253.80 ng/ml

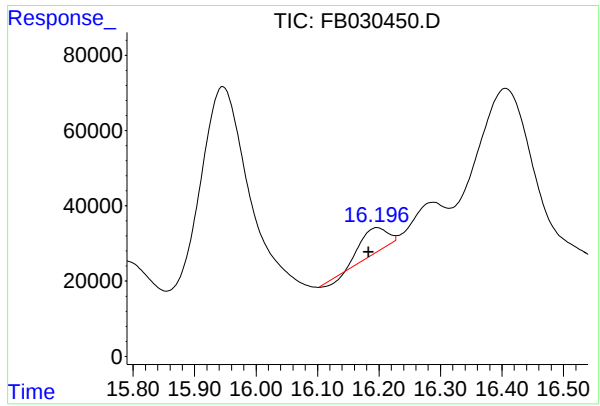

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.015 min
Response: 180066
Conc: 8.72 ng/ml

Instrument :
FID_B
ClientSampleId :