

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
 Data File : FB030451.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2023 15:21
 Operator : YP/AJ
 Sample : 05102-13 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 07 21:56:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	247816	21.704 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.407	222	0.013 ng/ml
4) t Benzene	7.837	98397	4.796 ng/ml
6) t Toluene	10.623	17535	0.869 ng/ml
7) t Ethylbenzene	13.031	368163	18.445 ng/ml
8) t m-Xylene	13.177	196989	9.995 ng/ml
9) t O-Xylene	13.911	606100	30.795 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	166792	8.074 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030451.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 15:21
Operator : YP/AJ
Sample : 05102-13 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 21:56:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

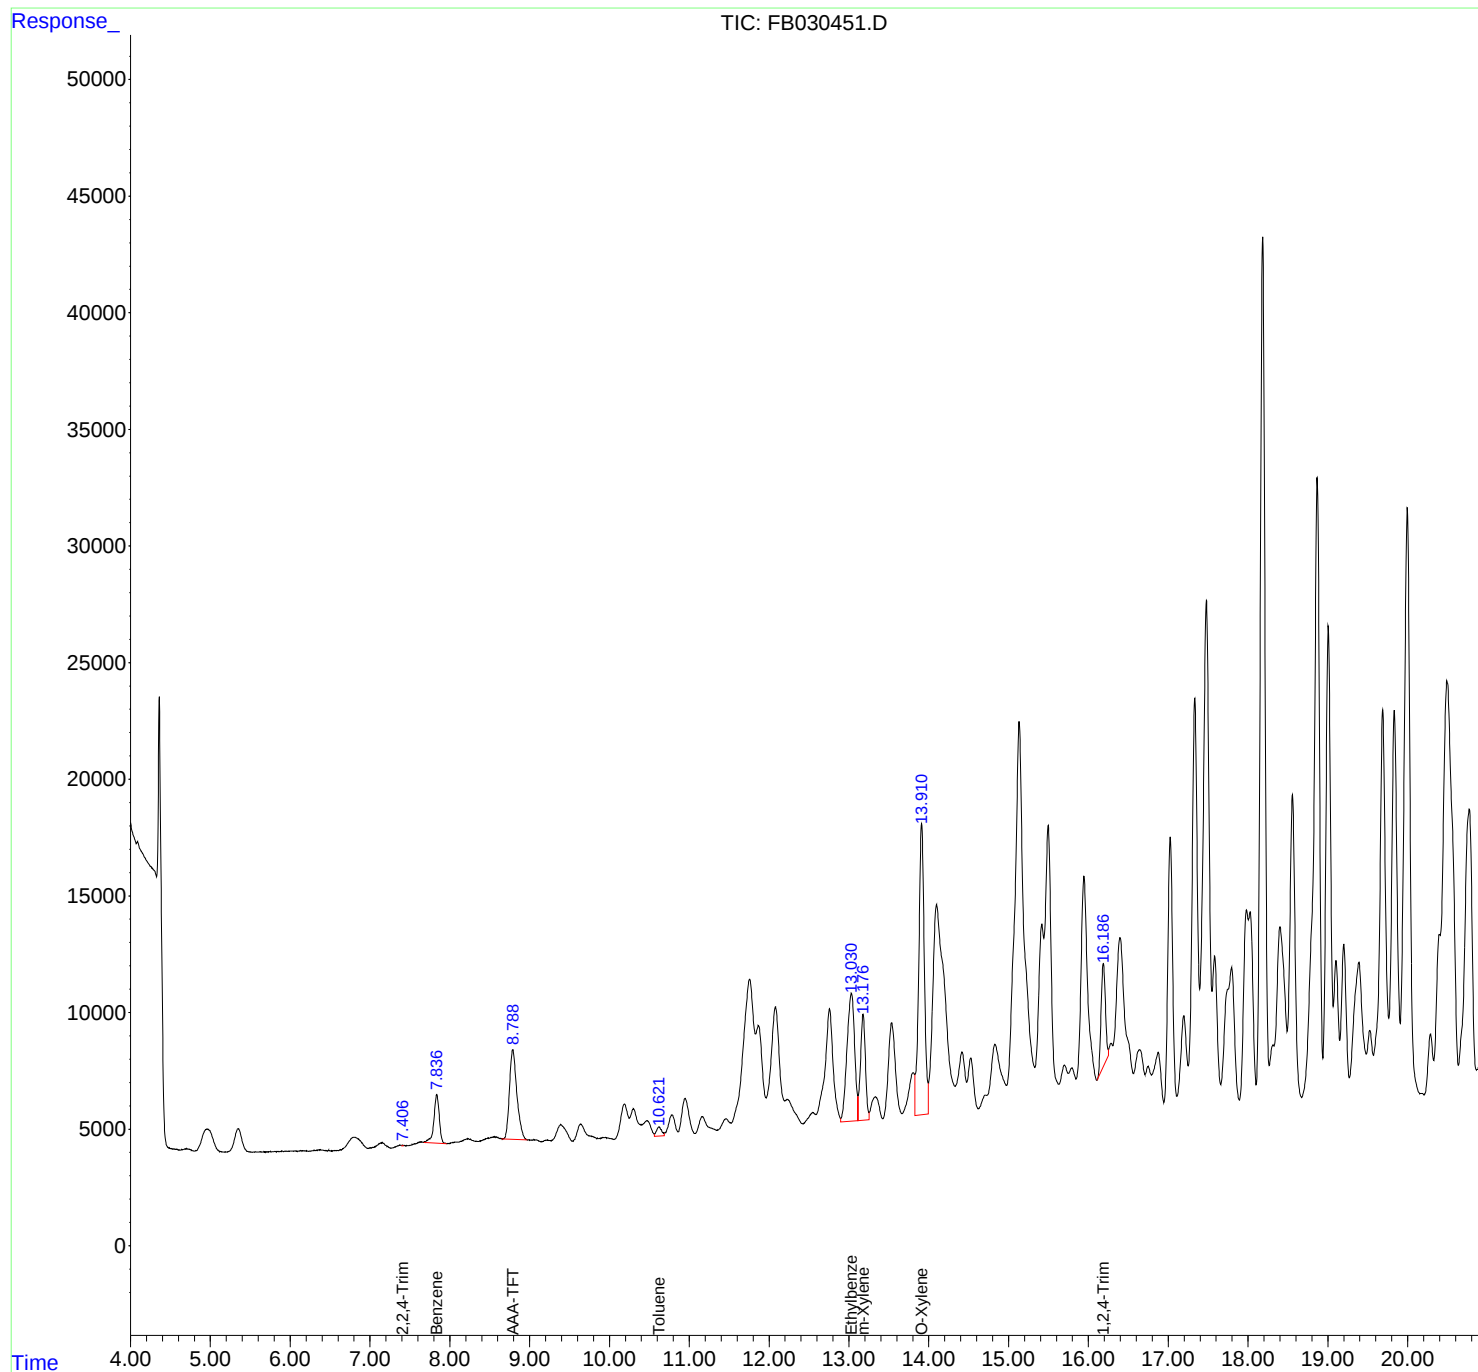


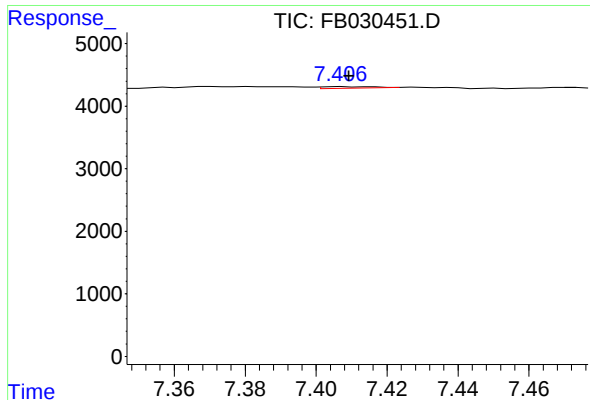

#2 2,2,4-Trimethylpentane


R.T.: 7.407 min
Delta R.T.: -0.002 min
Response: 222
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :

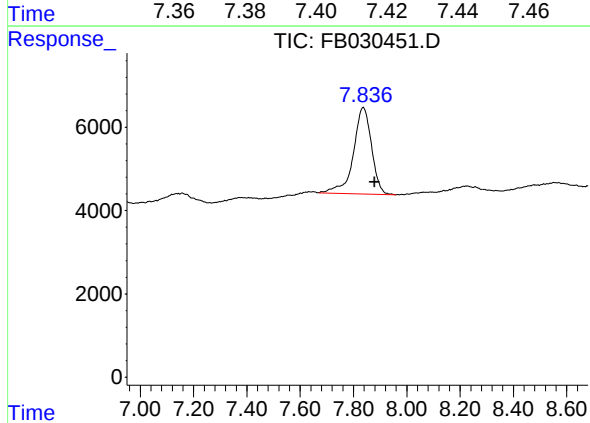


#4 Benzene

R.T.: 7.837 min
Delta R.T.: -0.042 min
Response: 98397
Conc: 4.80 ng/ml

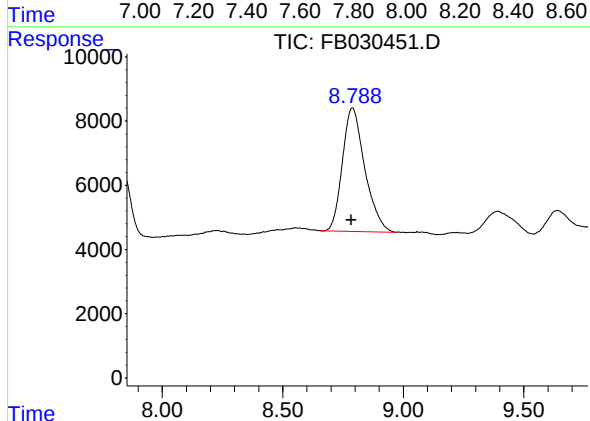


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.005 min
Response: 247816
Conc: 21.70 ng/ml

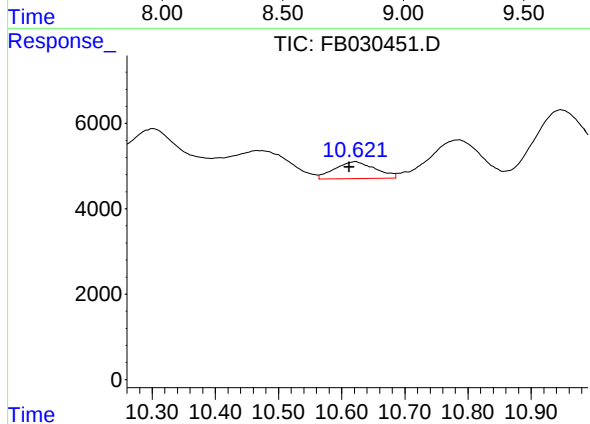

#6 Toluene


R.T.: 10.623 min
Delta R.T.: 0.010 min
Response: 17535
Conc: 0.87 ng/ml

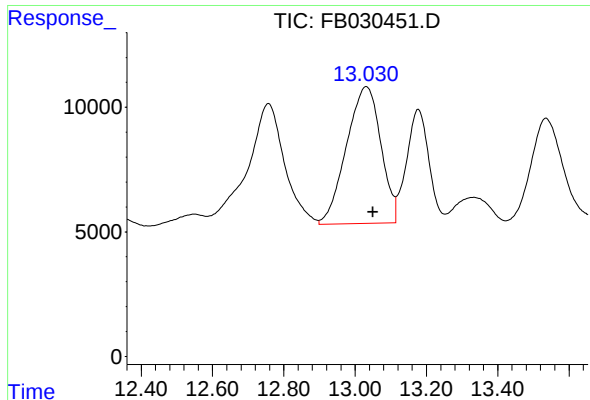

#7 Ethylbenzene


R.T.: 13.031 min
Delta R.T.: -0.018 min
Response: 368163
Conc: 18.44 ng/ml

Instrument :
FID_B
ClientSampleId :

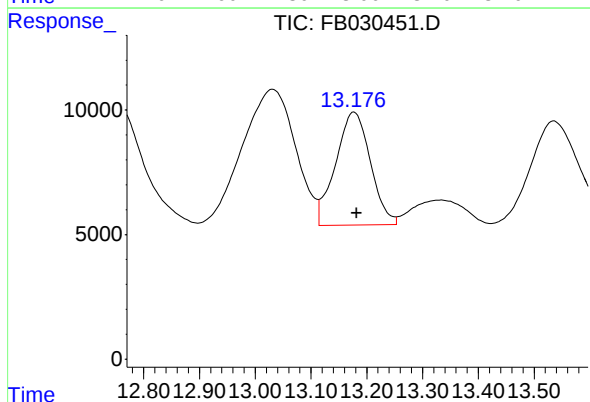


#8 m-Xylene

R.T.: 13.177 min
Delta R.T.: -0.004 min
Response: 196989
Conc: 9.99 ng/ml

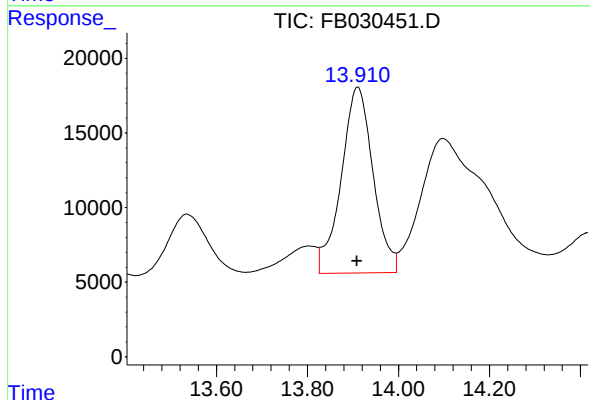

#9 o-Xylene

R.T.: 13.911 min
Delta R.T.: 0.003 min
Response: 606100
Conc: 30.80 ng/ml

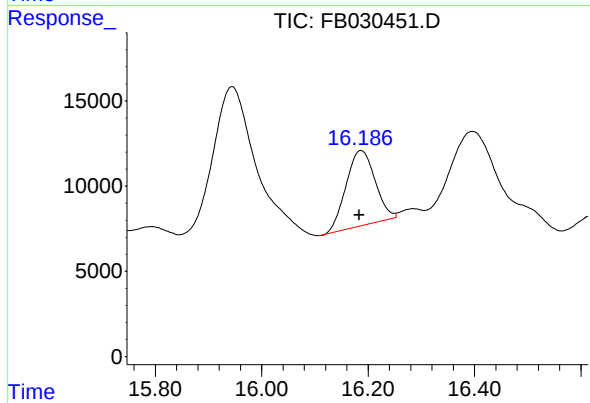

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.004 min
Response: 166792
Conc: 8.07 ng/ml