

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
 Data File : FB030452.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2023 16:00
 Operator : YP/AJ
 Sample : 05102-13MS
 Misc : 5.10G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 07 21:56:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	229607	20.110 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	305646	21.846 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	381956	23.134 ng/ml
3) t n-Heptane	7.743	124836	8.328 ng/ml
4) t Benzene	7.872	255321	12.445 ng/ml
6) t Toluene	10.614	563351	27.903 ng/ml
7) t Ethylbenzene	13.046	424938	21.289 ng/ml
8) t m-Xylene	13.182	500455	25.391 ng/ml
9) t O-Xylene	13.911	844344	42.900 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	388305	18.797 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030452.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 16:00
Operator : YP/AJ
Sample : 05102-13MS
Misc : 5.10G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 07 21:56:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

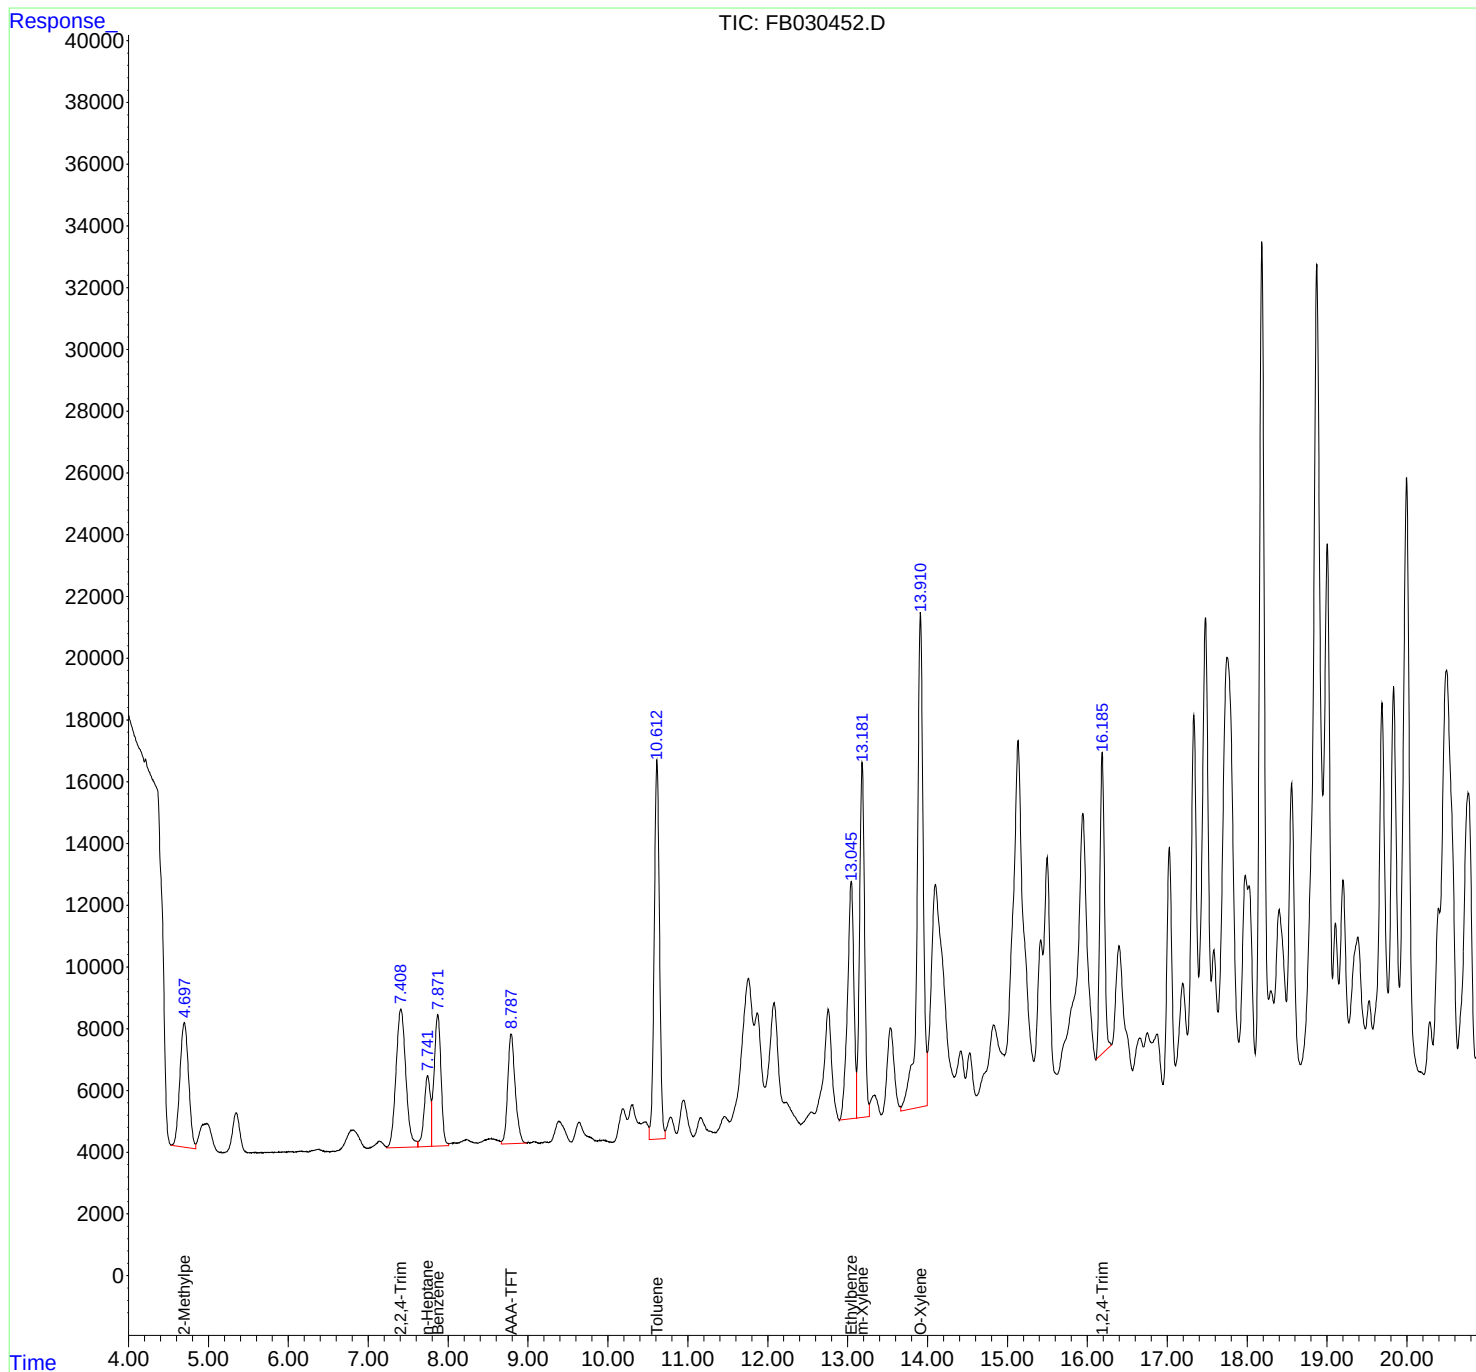


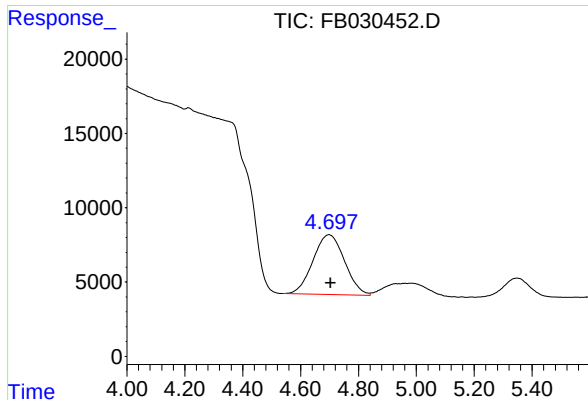

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 305646
Conc: 21.85 ng/ml

Instrument :
FID_B
ClientSampleId :

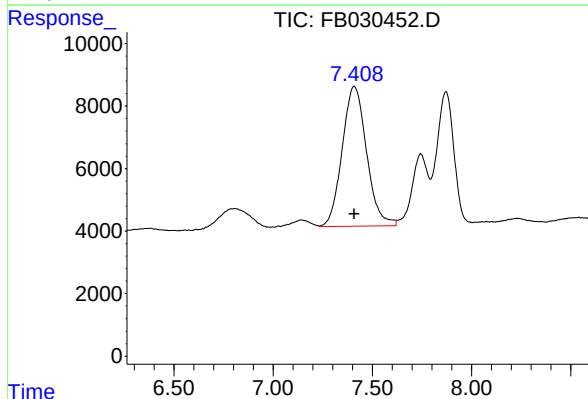


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 381956
Conc: 23.13 ng/ml

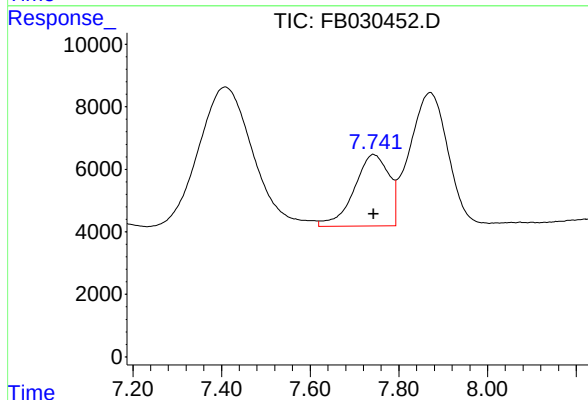


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 124836
Conc: 8.33 ng/ml

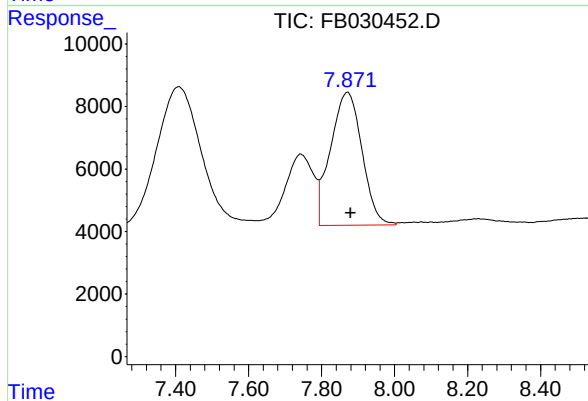

#4 Benzene


R.T.: 7.872 min
Delta R.T.: -0.008 min
Response: 255321
Conc: 12.44 ng/ml

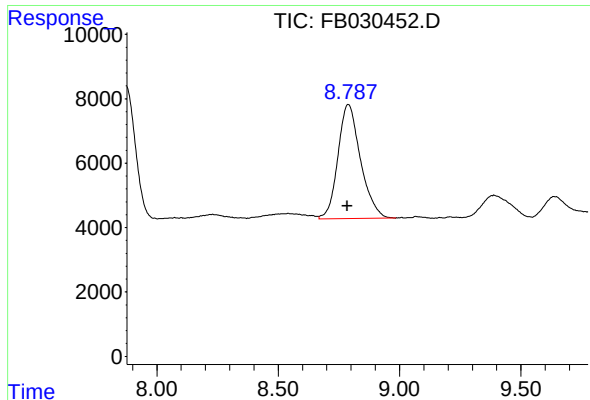

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.005 min
Response: 229607
Conc: 20.11 ng/ml

Instrument :
FID_B
ClientSampleId :

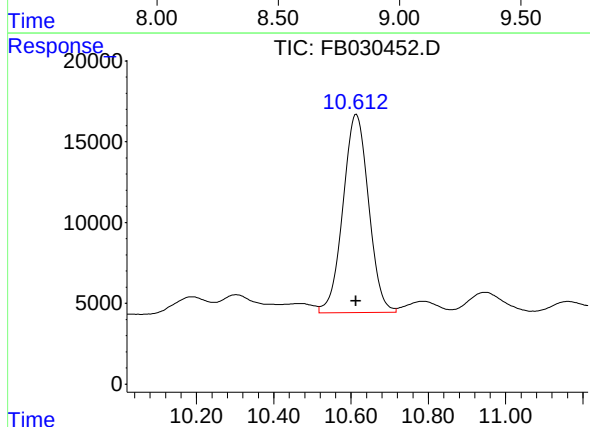


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.001 min
Response: 563351
Conc: 27.90 ng/ml

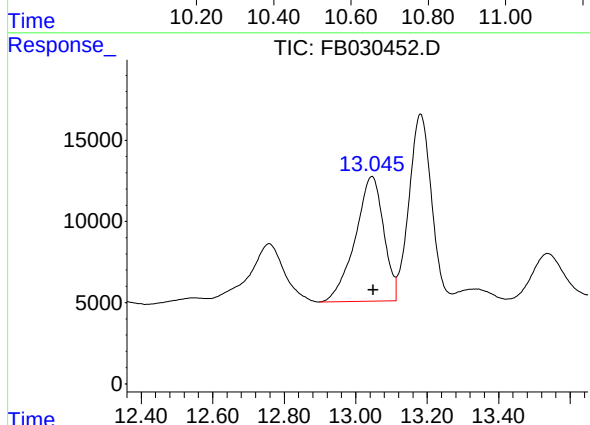


#7 Ethylbenzene

R.T.: 13.046 min
Delta R.T.: -0.004 min
Response: 424938
Conc: 21.29 ng/ml

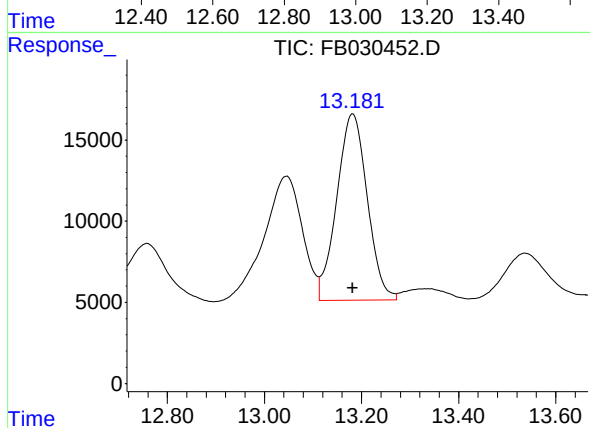

#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: 0.000 min
Response: 500455
Conc: 25.39 ng/ml

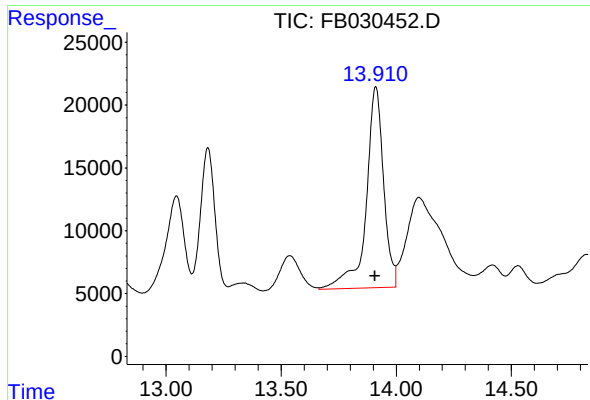


#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.003 min
Response: 844344
Conc: 42.90 ng/ml

Instrument :

FID_B

ClientSampleId :

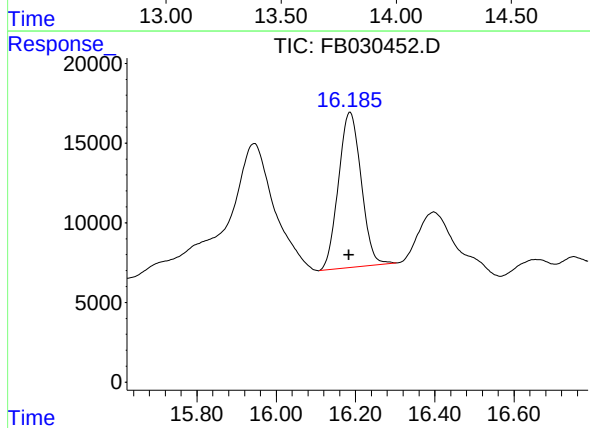

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.003 min
Response: 388305
Conc: 18.80 ng/ml