

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
 Data File : FB030449.D
 Signal(s) : FID2B.CH
 Acq On : 7 Nov 2023 21:07
 Operator : YP/AJ
 Sample : 05102-13MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 67S-IDW-01MS

Integration File: Calibration.e
 Quant Time: Nov 09 00:28:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.851	23379	2.048 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	8159	0.583 ng/ml
2) t 2,2,4-Trimethylpentane	7.402	2077	0.126 ng/ml
4) t Benzene	7.834	24261	1.182 ng/ml
7) t Ethylbenzene	13.032	37408	1.874 ng/ml
8) t m-Xylene	13.175	10269	0.521 ng/ml
9) t O-Xylene	13.922	12344	0.627 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030449.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 21:07
Operator : YP/AJ
Sample : 05102-13MS
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MS

Integration File: Calibration.e
Quant Time: Nov 09 00:28:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

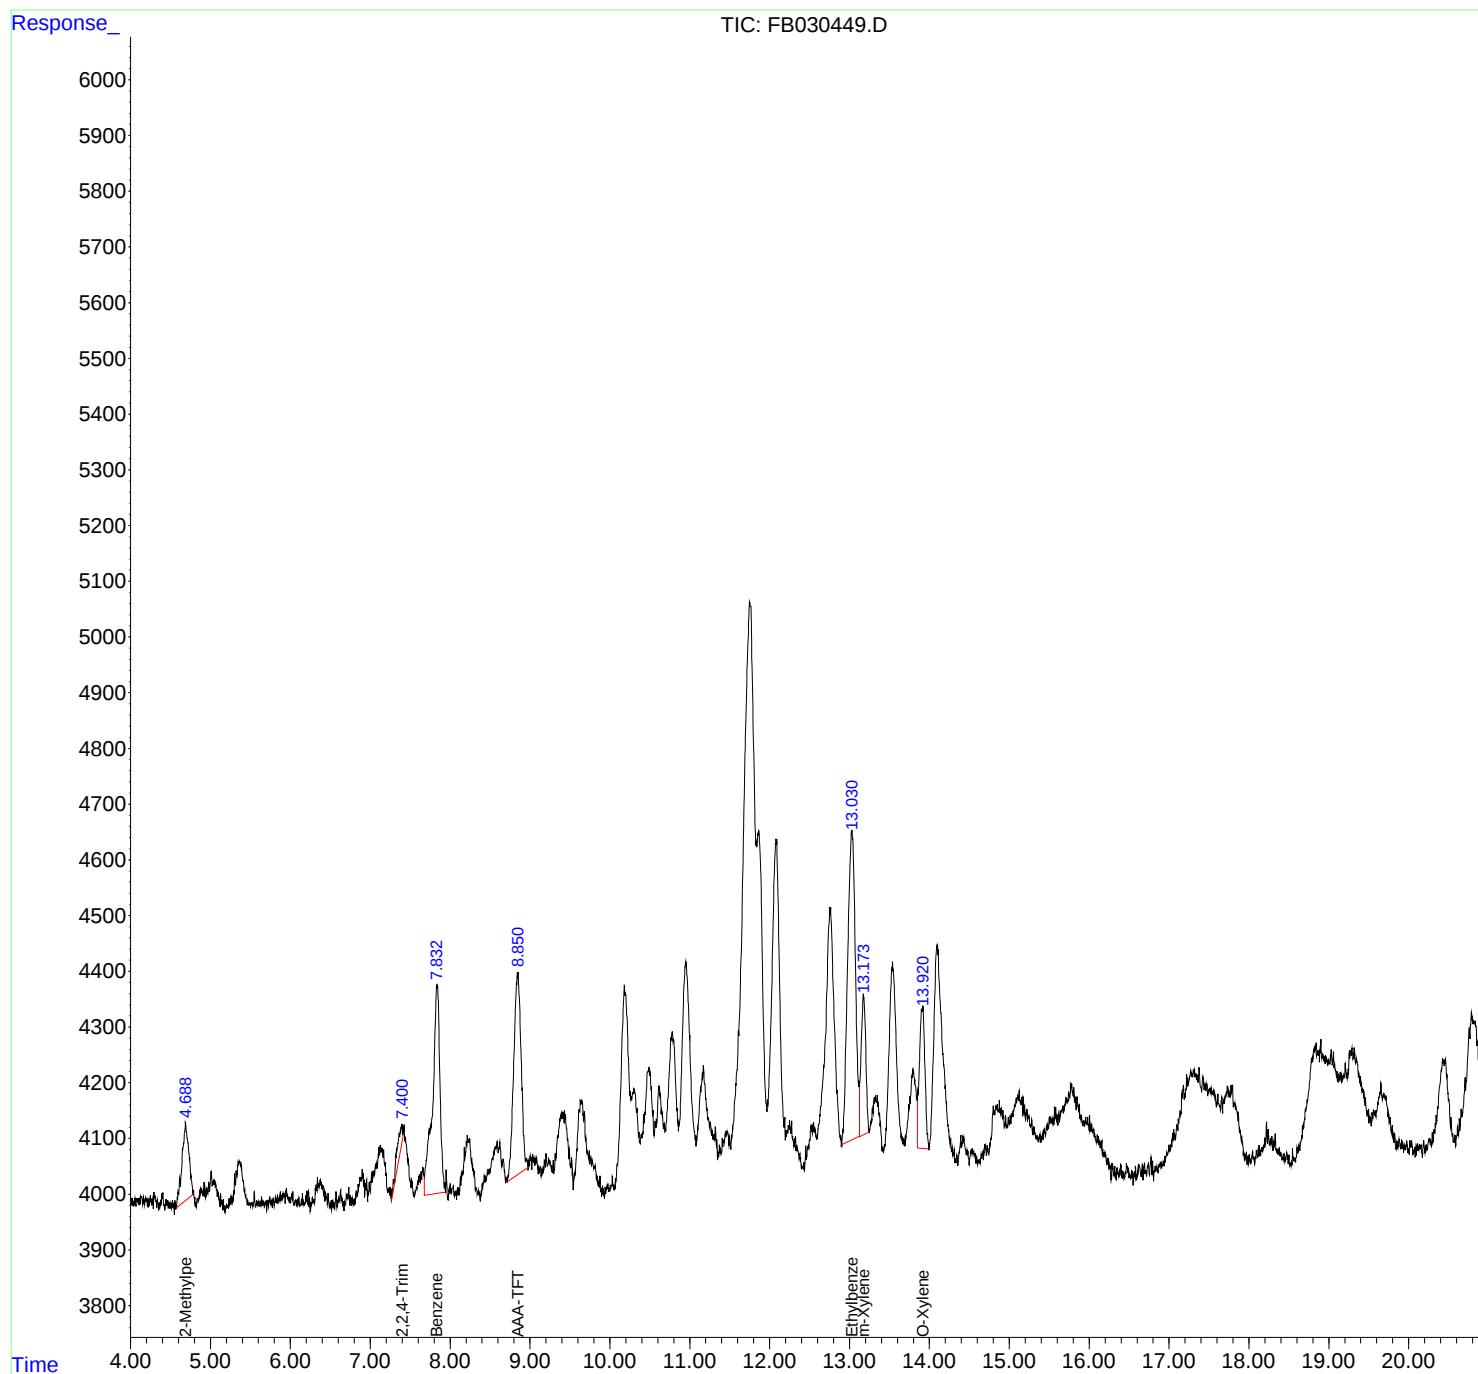


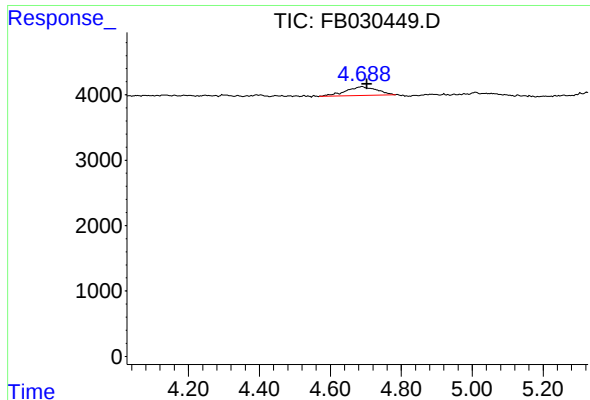

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: -0.014 min
Response: 8159
Conc: 0.58 ng/ml

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MS

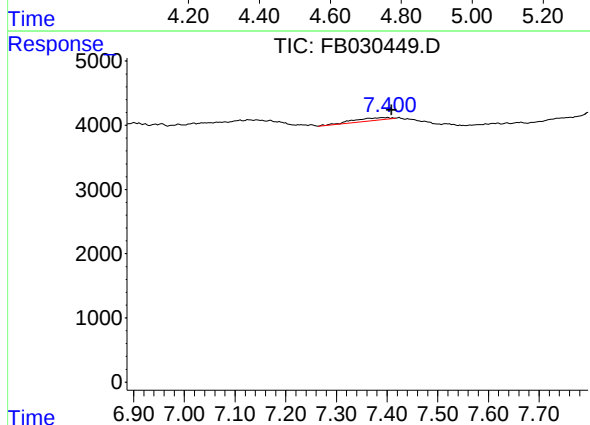


#2 2,2,4-Trimethylpentane

R.T.: 7.402 min
Delta R.T.: -0.008 min
Response: 2077
Conc: 0.13 ng/ml

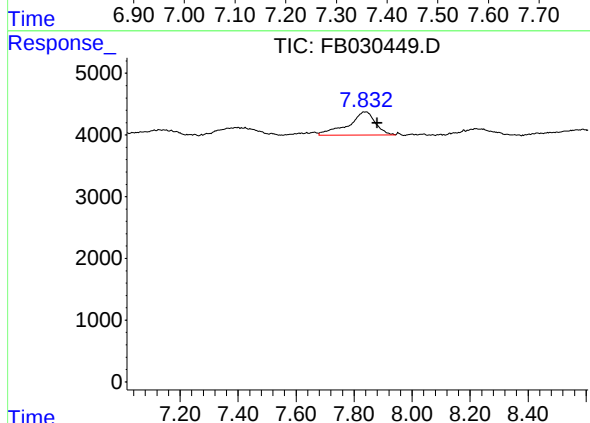


#4 Benzene

R.T.: 7.834 min
Delta R.T.: -0.046 min
Response: 24261
Conc: 1.18 ng/ml

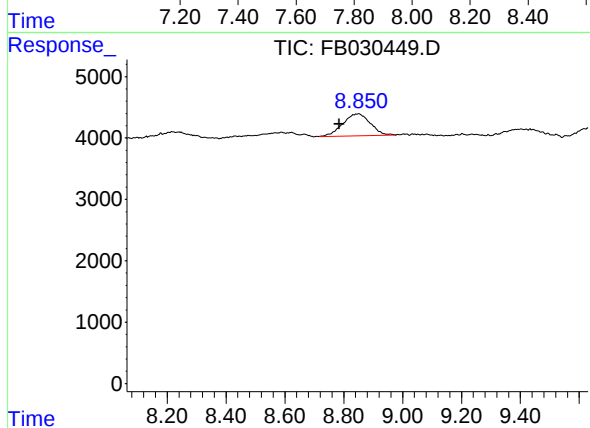

#5 AAA-TFT


R.T.: 8.851 min
Delta R.T.: 0.067 min
Response: 23379
Conc: 2.05 ng/ml

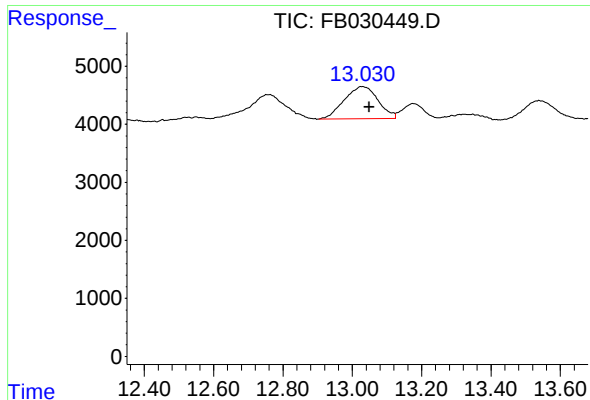

#7 Ethylbenzene


R.T.: 13.032 min
Delta R.T.: -0.018 min
Response: 37408
Conc: 1.87 ng/ml

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MS

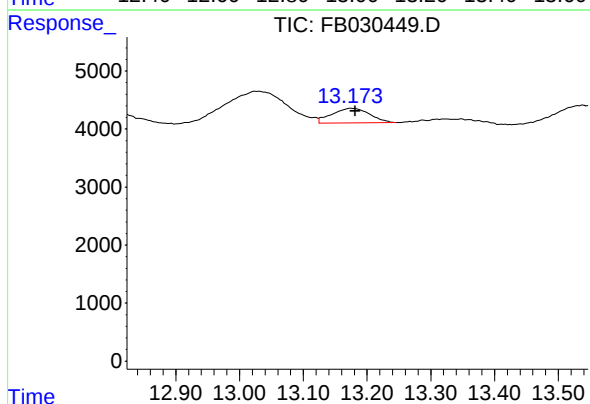

#8 m-Xylene

R.T.: 13.175 min
Delta R.T.: -0.007 min
Response: 10269
Conc: 0.52 ng/ml

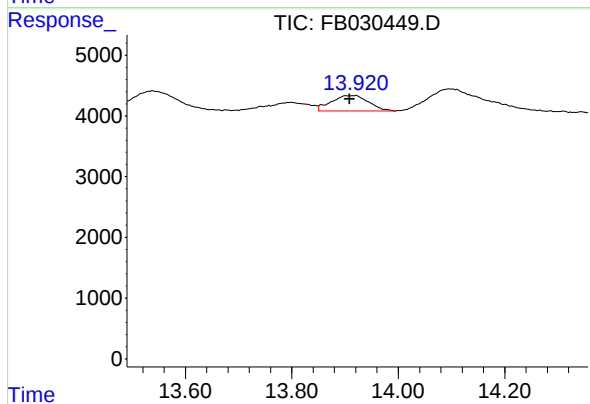

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.013 min
Response: 12344
Conc: 0.63 ng/ml