

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030452.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 23:01
Operator : YP/AJ
Sample : 05102-13MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MSD

Integration File: Calibration.e
Quant Time: Nov 09 00:28:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110723\
Data File : FB030452.D
Signal(s) : FID2B.CH
Acq On : 7 Nov 2023 23:01
Operator : YP/AJ
Sample : 05102-13MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MSD

Integration File: Calibration.e
Quant Time: Nov 09 00:28:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

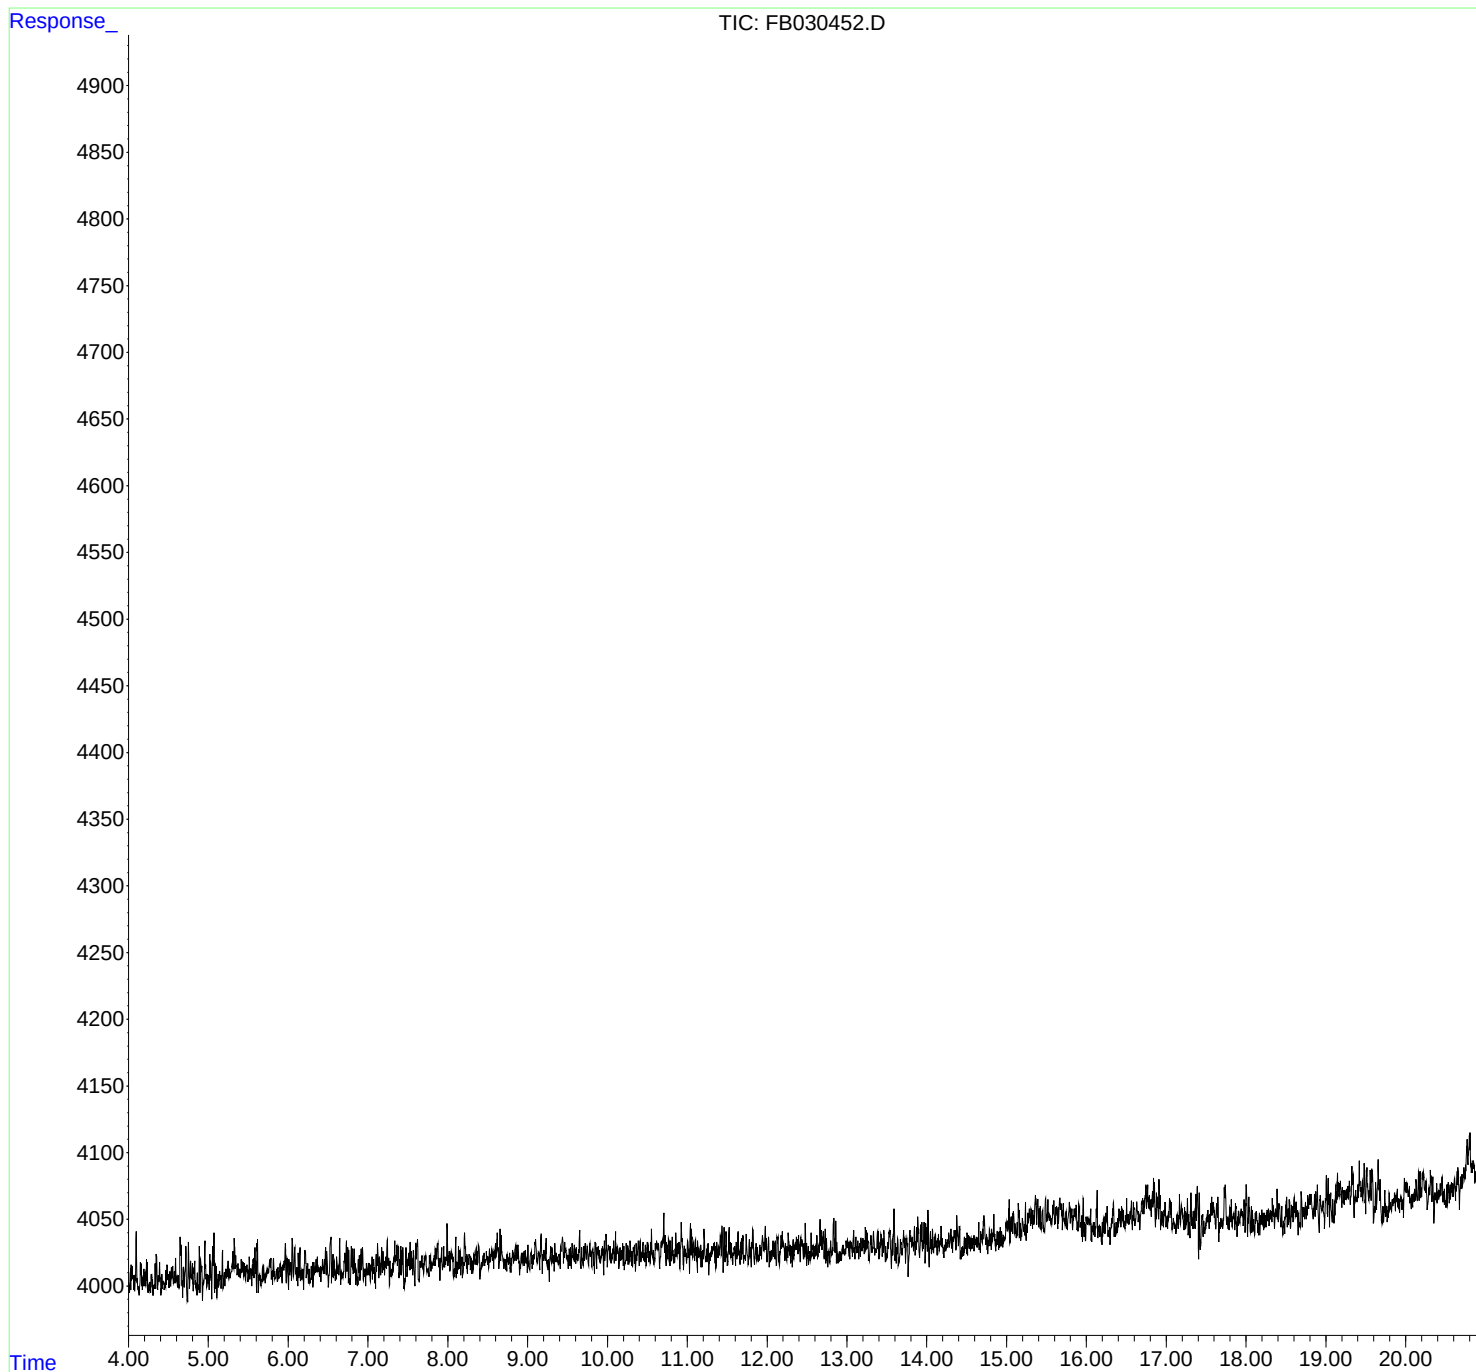

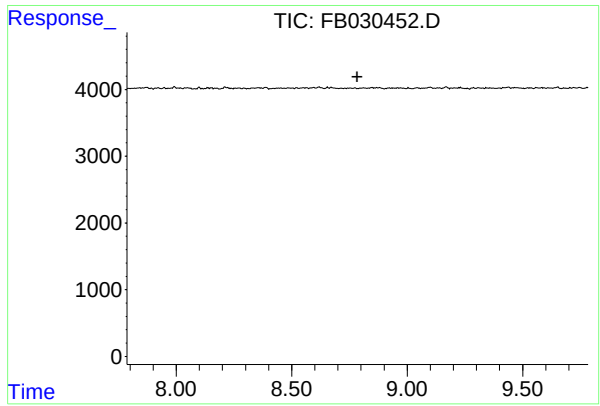

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.784 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
67S-IDW-01MSD